

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049094.D
 Acq On : 12 Jun 2022 16:23
 Operator : SY/MD
 Sample : N3255-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	80245	89506	10.66%	1.345%
2	1.896	165	173	187	rVB	63937	86323	10.28%	1.297%
3	2.414	330	334	342	rVB2	1450	1483	0.18%	0.022%
4	2.562	367	380	395	rBV	143836	237794	28.33%	3.573%
5	2.716	424	428	434	rVB	1166	1277	0.15%	0.019%
6	2.768	434	444	446	rBV2	1196	1908	0.23%	0.029%
7	2.835	461	465	469	rBV2	890	804	0.10%	0.012%
8	2.912	486	489	492	rBV	667	566	0.07%	0.009%
9	2.967	503	506	508	rBV	614	501	0.06%	0.008%
10	3.044	528	530	533	rBV2	565	279	0.03%	0.004%
11	3.240	588	591	593	rBV2	661	437	0.05%	0.007%
12	3.539	681	684	689	rVB	866	770	0.09%	0.012%
13	3.575	692	695	696	rBV	533	306	0.04%	0.005%
14	3.617	705	708	713	rVB2	1445	1008	0.12%	0.015%
15	3.646	714	717	720	rBV2	557	406	0.05%	0.006%
16	3.748	746	749	750	rBV	624	381	0.05%	0.006%
17	3.826	770	773	778	rBV2	683	536	0.06%	0.008%
18	3.906	792	798	800	rBV	1039	970	0.12%	0.015%
19	4.070	846	849	852	rBV2	690	539	0.06%	0.008%
20	4.173	878	881	882	rBV	546	305	0.04%	0.005%
21	4.244	901	903	906	rVB	407	199	0.02%	0.003%
22	4.269	906	911	913	rBV	747	694	0.08%	0.010%
23	4.459	966	970	979	rBV2	980	1144	0.14%	0.017%
24	4.494	979	981	983	rBV	484	328	0.04%	0.005%
25	4.555	997	1000	1003	rVB2	620	422	0.05%	0.006%
26	4.617	1003	1019	1045	rBV	108166	268480	31.99%	4.035%
27	4.999	1135	1138	1140	rVV	741	496	0.06%	0.007%
28	5.064	1143	1158	1179	rVB	162086	356696	42.50%	5.360%
29	5.269	1218	1222	1224	rBV	841	560	0.07%	0.008%
30	5.308	1232	1234	1236	rBV	673	300	0.04%	0.005%
31	5.343	1240	1245	1248	rVB2	1172	940	0.11%	0.014%
32	5.366	1248	1252	1255	rBV	620	604	0.07%	0.009%
33	5.436	1269	1274	1277	rBV2	660	806	0.10%	0.012%
34	5.559	1309	1312	1315	rBV2	680	525	0.06%	0.008%
35	5.633	1332	1335	1339	rBV	497	411	0.05%	0.006%
36	5.723	1341	1363	1384	rBV2	303980	839311	100.00%	12.613%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049094.D
 Acq On : 12 Jun 2022 16:23
 Operator : SY/MD
 Sample : N3255-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.922	1422	1425	1428	rBV	851	668	0.08%	0.010%
38	6.009	1447	1452	1455	rBV	486	505	0.06%	0.008%
39	6.028	1455	1458	1462	rVV	905	650	0.08%	0.010%
40	6.102	1479	1481	1484	rBV	365	273	0.03%	0.004%
41	6.247	1512	1526	1543	rBV	280620	530793	63.24%	7.976%
42	6.350	1555	1558	1560	rBV2	711	560	0.07%	0.008%
43	6.543	1603	1618	1633	rVB5	24302	48540	5.78%	0.729%
44	6.600	1633	1636	1638	rBV	630	376	0.04%	0.006%
45	6.690	1651	1664	1681	rBV	207889	398113	47.43%	5.983%
46	6.877	1716	1722	1724	rBV2	388	447	0.05%	0.007%
47	6.941	1738	1742	1745	rBV	973	863	0.10%	0.013%
48	7.063	1777	1780	1783	rBV2	624	316	0.04%	0.005%
49	7.137	1800	1803	1805	rBV2	332	204	0.02%	0.003%
50	7.243	1834	1836	1839	rBV	479	299	0.04%	0.004%
51	7.263	1839	1842	1849	rVV2	656	900	0.11%	0.014%
52	7.356	1868	1871	1873	rBV	874	656	0.08%	0.010%
53	7.414	1887	1889	1893	rBV	375	254	0.03%	0.004%
54	7.440	1894	1897	1901	rVB2	776	520	0.06%	0.008%
55	7.497	1913	1915	1919	rBV2	395	238	0.03%	0.004%
56	7.565	1925	1936	1954	rBV	93834	162675	19.38%	2.445%
57	7.684	1969	1973	1975	rBV3	1231	1062	0.13%	0.016%
58	7.809	2009	2012	2014	rBV2	390	215	0.03%	0.003%
59	7.896	2026	2039	2057	rBV	348197	599450	71.42%	9.008%
60	8.179	2117	2127	2143	rVB2	67640	112535	13.41%	1.691%
61	8.243	2143	2147	2152	rBV4	812	914	0.11%	0.014%
62	8.327	2170	2173	2175	rBV	459	308	0.04%	0.005%
63	8.382	2188	2190	2193	rVB	529	272	0.03%	0.004%
64	8.401	2193	2196	2198	rBV	1055	730	0.09%	0.011%
65	8.481	2215	2221	2224	rBV2	865	1015	0.12%	0.015%
66	8.530	2234	2236	2241	rVB	523	302	0.04%	0.005%
67	8.633	2257	2268	2300	rBV2	287461	554346	66.05%	8.330%
68	8.790	2315	2317	2320	rVB2	854	449	0.05%	0.007%
69	8.919	2354	2357	2361	rBV2	652	408	0.05%	0.006%
70	9.083	2404	2408	2414	rBV2	618	817	0.10%	0.012%
71	9.108	2414	2416	2421	rVB	939	596	0.07%	0.009%
72	9.179	2435	2438	2445	rVB2	726	755	0.09%	0.011%
73	9.208	2445	2447	2450	rBV	605	292	0.03%	0.004%
74	9.417	2500	2512	2530	rBV	398165	664174	79.13%	9.981%
75	9.639	2578	2581	2584	rVB2	1058	654	0.08%	0.010%
76	9.706	2599	2602	2608	rBV	677	676	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049094.D
 Acq On : 12 Jun 2022 16:23
 Operator : SY/MD
 Sample : N3255-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.735	2608	2611	2614	rVB	709	374	0.04%	0.006%
78	9.768	2619	2621	2623	rBV	422	246	0.03%	0.004%
79	9.848	2641	2646	2649	rBV2	1018	1211	0.14%	0.018%
80	9.925	2667	2670	2674	rVB	862	564	0.07%	0.008%
81	9.986	2686	2689	2692	rVB2	444	293	0.03%	0.004%
82	10.005	2692	2695	2697	rBV	404	231	0.03%	0.003%
83	10.118	2726	2730	2732	rBV2	1057	833	0.10%	0.013%
84	10.292	2782	2784	2786	rBV	656	335	0.04%	0.005%
85	10.394	2812	2816	2822	rBV2	870	1069	0.13%	0.016%
86	10.510	2847	2852	2853	rBV2	791	635	0.08%	0.010%
87	10.581	2869	2874	2877	rBV2	850	763	0.09%	0.011%
88	10.755	2916	2928	2944	rBV	328744	538957	64.21%	8.099%
89	10.903	2971	2974	2977	rBV2	802	538	0.06%	0.008%
90	11.163	3052	3055	3058	rBV	664	513	0.06%	0.008%
91	11.198	3063	3066	3069	rVV	540	330	0.04%	0.005%
92	11.668	3209	3212	3216	rBV2	673	473	0.06%	0.007%
93	11.812	3246	3257	3275	rBV	341919	546363	65.10%	8.210%
94	11.989	3310	3312	3313	rBV	709	312	0.04%	0.005%
95	12.044	3326	3329	3333	rBV	506	450	0.05%	0.007%
96	12.192	3363	3375	3399	rBV	347118	570497	67.97%	8.573%
97	12.465	3457	3460	3464	rBV2	682	633	0.08%	0.010%
98	13.105	3652	3659	3662	rBV2	792	1125	0.13%	0.017%
99	14.269	4018	4021	4027	rBV	1302	1343	0.16%	0.020%
100	14.475	4082	4085	4088	rBV2	737	556	0.07%	0.008%



Sum of corrected areas: 6654479

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049094.D
Acq On : 12 Jun 2022 16:23
Operator : SY/MD
Sample : N3255-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

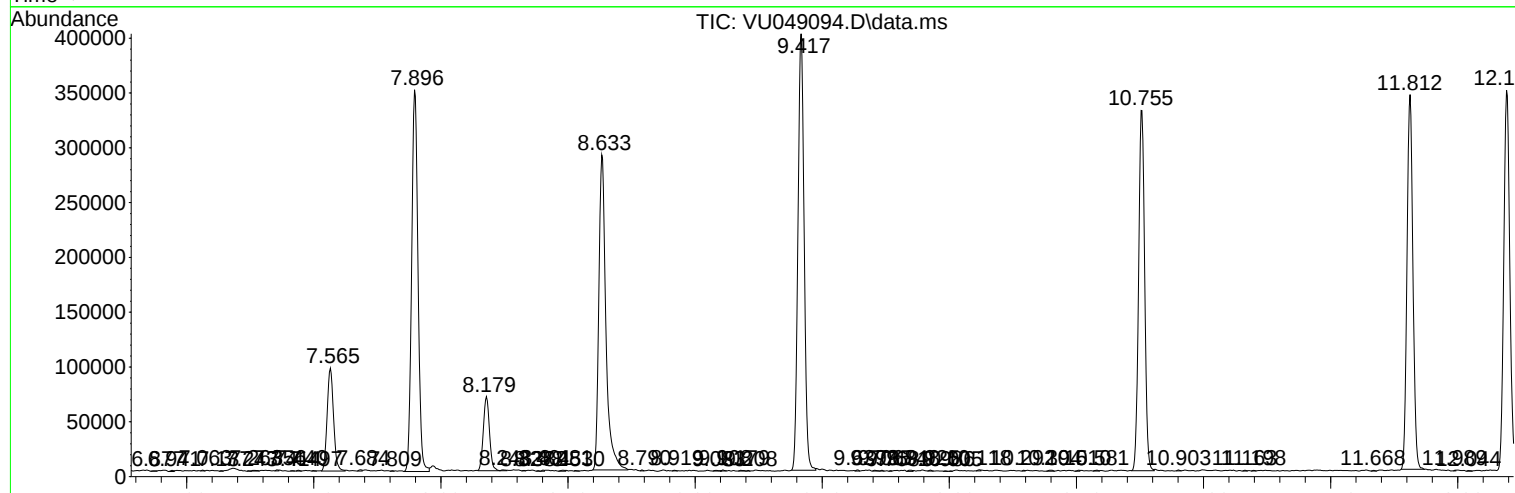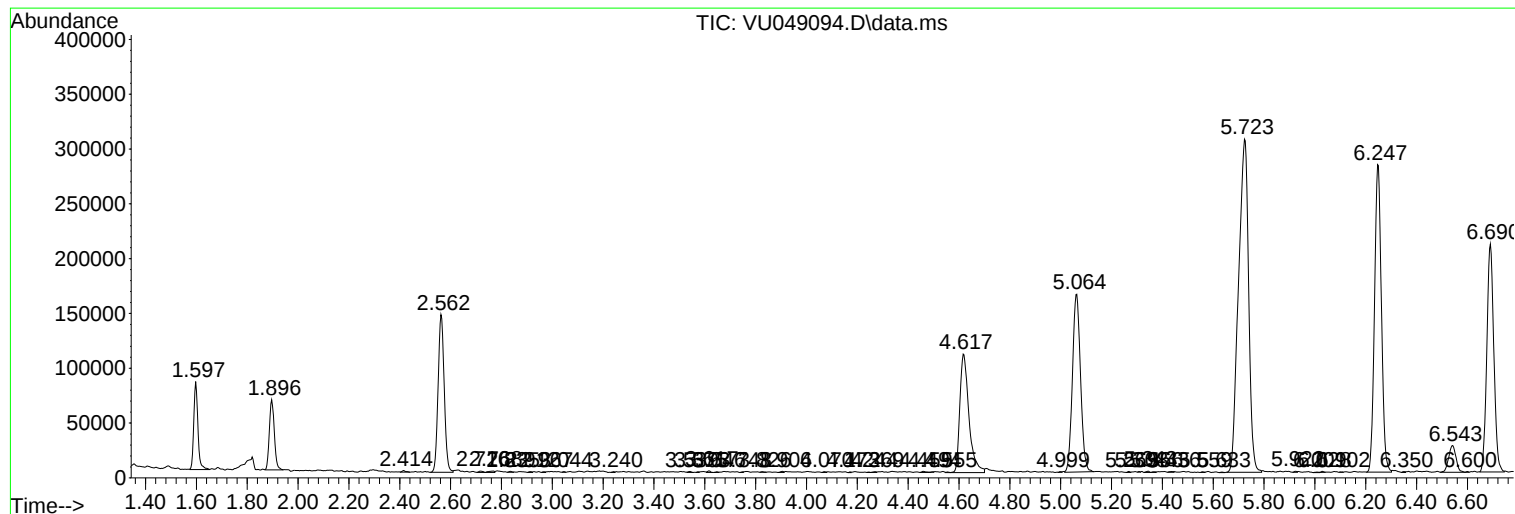

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049094.D
Acq On : 12 Jun 2022 16:23
Operator : SY/MD
Sample : N3255-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049094.D
Acq On : 12 Jun 2022 16:23
Operator : SY/MD
Sample : N3255-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc