

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049097.D
 Acq On : 12 Jun 2022 17:33
 Operator : SY/MD
 Sample : N3255-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	81589	90859	10.83%	1.400%
2	1.903	166	175	189	rBV	66431	89251	10.64%	1.375%
3	2.076	226	229	234	rVV3	775	657	0.08%	0.010%
4	2.150	249	252	255	rBV	753	582	0.07%	0.009%
5	2.199	264	267	270	rBV2	686	528	0.06%	0.008%
6	2.510	359	364	368	rBV3	626	610	0.07%	0.009%
7	2.565	369	381	394	rBV	152446	251648	29.99%	3.878%
8	2.723	426	430	432	rBV2	734	624	0.07%	0.010%
9	2.903	483	486	489	rVB	802	519	0.06%	0.008%
10	3.311	609	613	619	rBV	662	821	0.10%	0.013%
11	3.343	619	623	627	rBV2	719	619	0.07%	0.010%
12	3.462	656	660	663	rVB2	768	572	0.07%	0.009%
13	3.485	663	667	669	rBV	715	553	0.07%	0.009%
14	3.842	775	778	781	rBV	786	633	0.08%	0.010%
15	3.861	781	784	791	rVB2	1045	1217	0.15%	0.019%
16	3.893	791	794	797	rBV	654	599	0.07%	0.009%
17	4.086	849	854	860	rVB	951	1047	0.12%	0.016%
18	4.269	908	911	916	rVB	728	703	0.08%	0.011%
19	4.366	936	941	944	rBV	790	684	0.08%	0.011%
20	4.456	966	969	971	rBV	967	586	0.07%	0.009%
21	4.620	1008	1020	1044	rBV	101319	254890	30.37%	3.928%
22	4.793	1070	1074	1076	rBV2	639	510	0.06%	0.008%
23	4.967	1122	1128	1131	rBV2	1035	1234	0.15%	0.019%
24	4.989	1131	1135	1138	rVV	1124	1281	0.15%	0.020%
25	5.063	1142	1158	1177	rVV	164329	363017	43.26%	5.594%
26	5.147	1181	1184	1190	rVV2	943	964	0.11%	0.015%
27	5.240	1209	1213	1216	rBV	744	628	0.07%	0.010%
28	5.305	1228	1233	1236	rBV	1058	971	0.12%	0.015%
29	5.530	1300	1303	1306	rBV2	796	526	0.06%	0.008%
30	5.726	1342	1364	1386	rBV2	303756	839191	100.00%	12.931%
31	5.825	1393	1395	1399	rVB2	1290	853	0.10%	0.013%
32	6.044	1457	1463	1468	rBV2	1097	1286	0.15%	0.020%
33	6.108	1476	1483	1488	rBV2	889	1156	0.14%	0.018%
34	6.166	1498	1501	1505	rVB2	935	648	0.08%	0.010%
35	6.189	1505	1508	1511	rBV2	781	532	0.06%	0.008%
36	6.247	1513	1526	1545	rBV	269822	519058	61.85%	7.998%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049097.D
 Acq On : 12 Jun 2022 17:33
 Operator : SY/MD
 Sample : N3255-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.462	1591	1593	1598	rVB	1017	736	0.09%	0.011%
38	6.536	1608	1616	1626	rVB5	5972	11194	1.33%	0.172%
39	6.600	1629	1636	1642	rBV3	717	961	0.11%	0.015%
40	6.690	1647	1664	1684	rBV	199971	392511	46.77%	6.048%
41	6.983	1751	1755	1766	rVB2	926	1570	0.19%	0.024%
42	7.067	1777	1781	1784	rBV	767	633	0.08%	0.010%
43	7.182	1812	1817	1828	rVB6	2865	4826	0.58%	0.074%
44	7.356	1868	1871	1873	rBV	998	610	0.07%	0.009%
45	7.372	1873	1876	1879	rVB	962	629	0.07%	0.010%
46	7.407	1879	1887	1891	rBV	1092	1547	0.18%	0.024%
47	7.488	1908	1912	1916	rBV2	658	626	0.07%	0.010%
48	7.565	1924	1936	1954	rBV	88905	159681	19.03%	2.461%
49	7.687	1968	1974	1977	rBV4	1660	1622	0.19%	0.025%
50	7.735	1983	1989	1991	rBV2	569	591	0.07%	0.009%
51	7.899	2027	2040	2055	rBV	343729	596857	71.12%	9.197%
52	8.034	2079	2082	2086	rBV2	865	868	0.10%	0.013%
53	8.121	2106	2109	2114	rVB2	842	815	0.10%	0.013%
54	8.179	2114	2127	2140	rBV	63097	108466	12.93%	1.671%
55	8.462	2213	2215	2219	rVB	718	531	0.06%	0.008%
56	8.484	2219	2222	2224	rBV2	742	561	0.07%	0.009%
57	8.632	2256	2268	2294	rBV2	277074	529255	63.07%	8.155%
58	8.783	2312	2315	2316	rBV	1061	542	0.06%	0.008%
59	8.861	2337	2339	2345	rVB2	798	715	0.09%	0.011%
60	8.896	2345	2350	2353	rBV2	652	782	0.09%	0.012%
61	9.041	2391	2395	2398	rBV	1142	992	0.12%	0.015%
62	9.057	2398	2400	2404	rVB	1080	716	0.09%	0.011%
63	9.153	2427	2430	2435	rVV2	577	594	0.07%	0.009%
64	9.201	2441	2445	2451	rBV3	1115	1209	0.14%	0.019%
65	9.250	2457	2460	2465	rBV	680	695	0.08%	0.011%
66	9.308	2474	2478	2483	rBV2	802	803	0.10%	0.012%
67	9.417	2499	2512	2538	rBV	380095	636753	75.88%	9.812%
68	9.581	2558	2563	2566	rBV	572	601	0.07%	0.009%
69	9.700	2597	2600	2603	rBV	906	642	0.08%	0.010%
70	9.931	2670	2672	2677	rVB	798	506	0.06%	0.008%
71	10.099	2721	2724	2729	rVB	748	517	0.06%	0.008%
72	10.179	2746	2749	2752	rBV2	720	574	0.07%	0.009%
73	10.536	2857	2860	2865	rBV	610	605	0.07%	0.009%
74	10.754	2916	2928	2946	rBV	312624	504826	60.16%	7.779%
75	11.121	3035	3042	3044	rBV2	992	1317	0.16%	0.020%
76	11.224	3070	3074	3078	rBV2	625	666	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049097.D
 Acq On : 12 Jun 2022 17:33
 Operator : SY/MD
 Sample : N3255-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.262	3083	3086	3092	rVB	930	958	0.11%	0.015%
78	11.420	3132	3135	3139	rBV	840	538	0.06%	0.008%
79	11.565	3177	3180	3187	rVB2	716	750	0.09%	0.012%
80	11.597	3187	3190	3195	rBV2	606	698	0.08%	0.011%
81	11.716	3223	3227	3229	rBV	967	853	0.10%	0.013%
82	11.812	3245	3257	3276	rBV	326186	524746	62.53%	8.086%
83	12.089	3339	3343	3347	rBV2	933	813	0.10%	0.013%
84	12.192	3363	3375	3392	rBV	332357	547752	65.27%	8.440%
85	12.381	3431	3434	3438	rVB2	822	568	0.07%	0.009%
86	12.844	3574	3578	3583	rBV	706	874	0.10%	0.013%
87	12.976	3616	3619	3622	rBV	766	623	0.07%	0.010%
88	13.211	3685	3692	3696	rBV	1165	1407	0.17%	0.022%
89	13.381	3741	3745	3748	rBV2	605	532	0.06%	0.008%
90	13.465	3769	3771	3777	rVB	995	915	0.11%	0.014%
91	13.539	3786	3794	3796	rBV2	974	1231	0.15%	0.019%
92	13.748	3856	3859	3865	rBV3	646	771	0.09%	0.012%
93	14.047	3949	3952	3954	rBV2	994	715	0.09%	0.011%
94	14.211	4000	4003	4007	rBV3	799	733	0.09%	0.011%
95	14.397	4058	4061	4065	rBV2	968	971	0.12%	0.015%
96	14.532	4099	4103	4106	rBV	849	681	0.08%	0.010%
97	14.748	4164	4170	4172	rBV2	890	907	0.11%	0.014%
98	14.947	4229	4232	4234	rBV	741	522	0.06%	0.008%
99	14.986	4241	4244	4247	rBV2	772	522	0.06%	0.008%
100	16.047	4569	4574	4576	rBV3	1416	1369	0.16%	0.021%




Sum of corrected areas: 6489651

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049097.D
Acq On : 12 Jun 2022 17:33
Operator : SY/MD
Sample : N3255-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

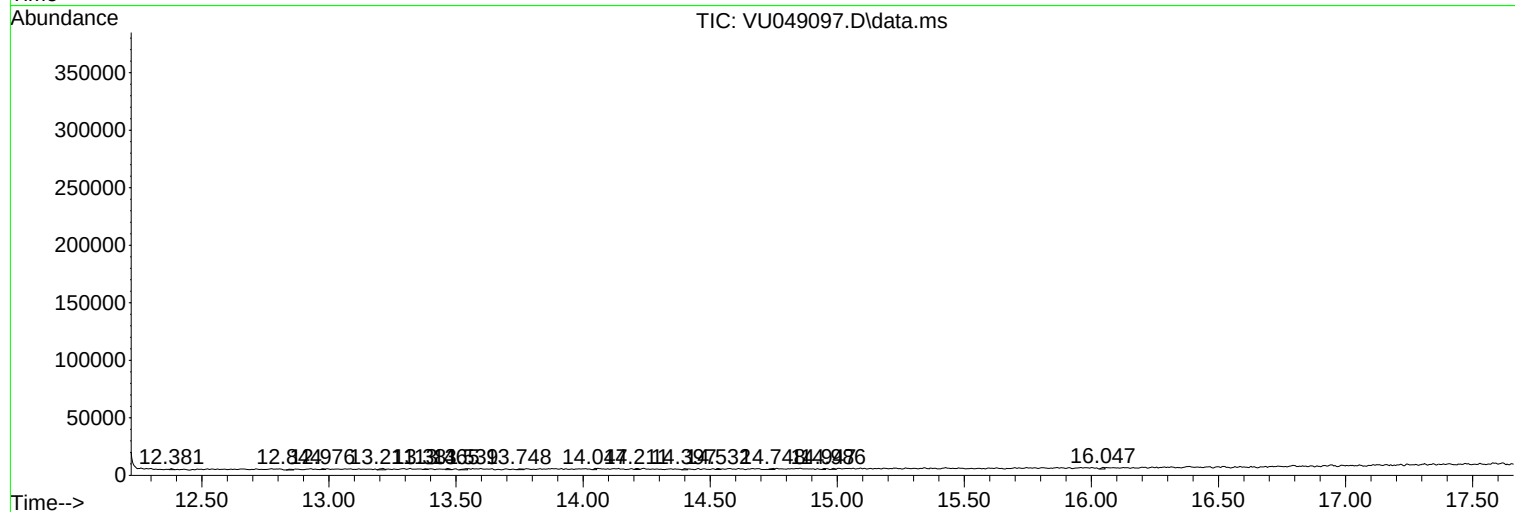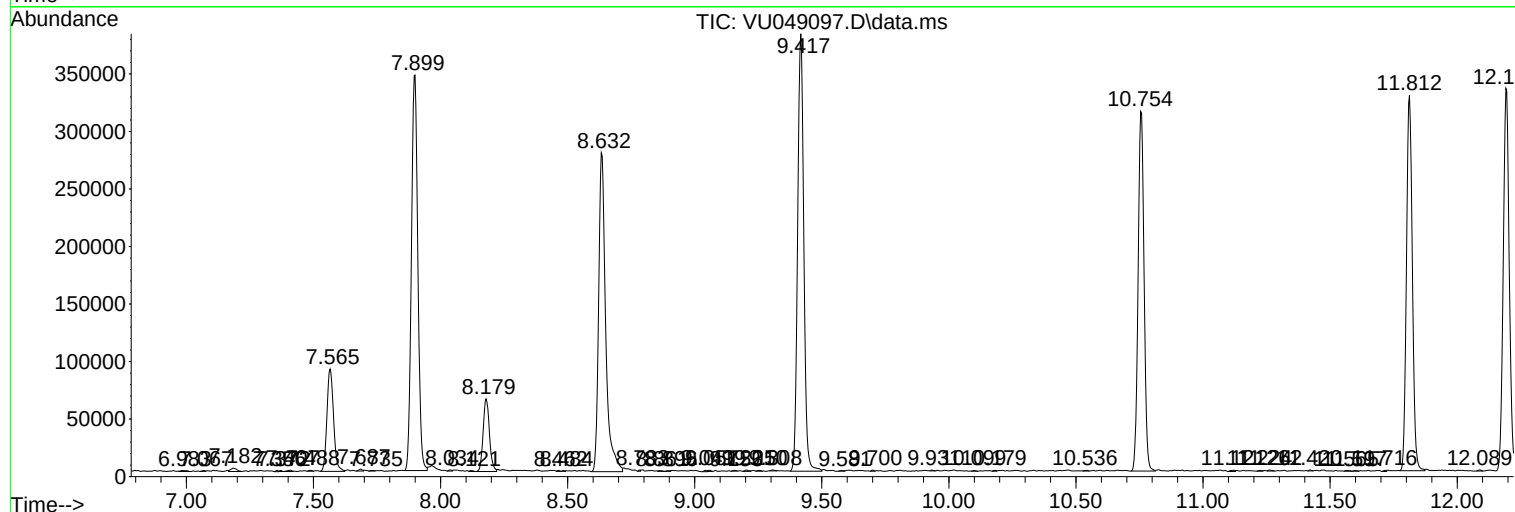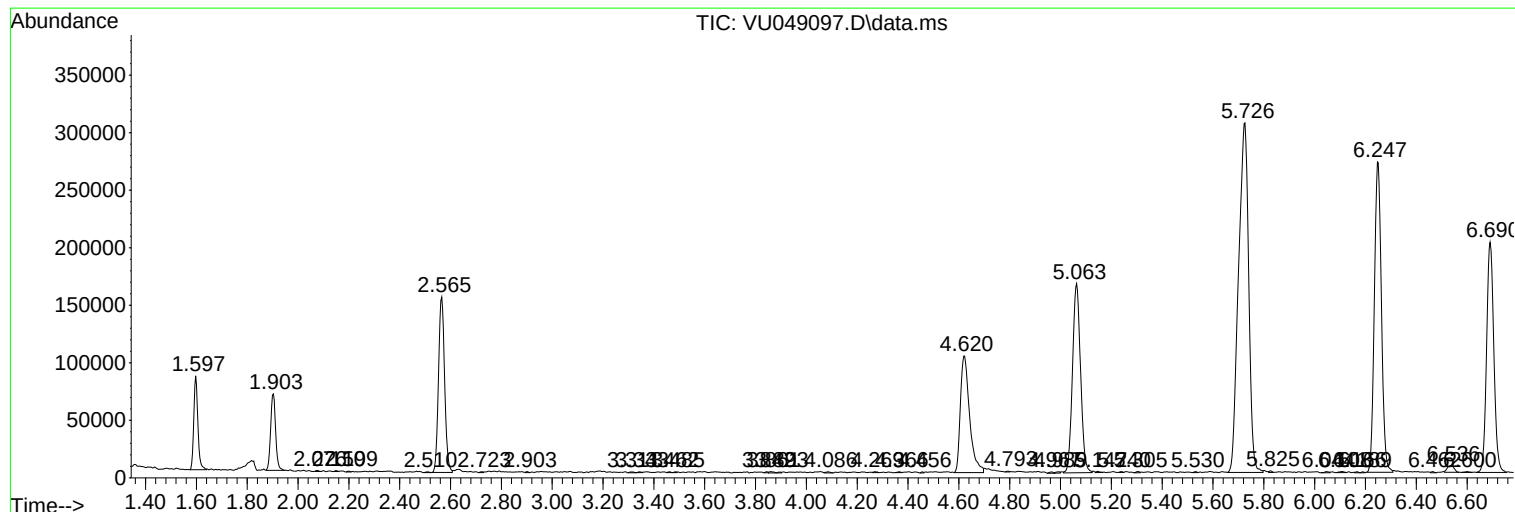

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049097.D
Acq On : 12 Jun 2022 17:33
Operator : SY/MD
Sample : N3255-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049097.D
Acq On : 12 Jun 2022 17:33
Operator : SY/MD
Sample : N3255-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------