

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049098.D
 Acq On : 12 Jun 2022 17:57
 Operator : SY/MD
 Sample : N3255-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049098.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	96	rBV	84315	96067	11.38%	1.465%
2	1.899	165	174	187	rBV	68583	93584	11.08%	1.427%
3	2.279	288	292	295	rBV4	1177	837	0.10%	0.013%
4	2.565	369	381	395	rBV	154090	253082	29.97%	3.858%
5	2.922	485	492	495	rBV	736	908	0.11%	0.014%
6	2.964	500	505	511	rBV2	715	865	0.10%	0.013%
7	2.996	511	515	518	rBV2	845	754	0.09%	0.011%
8	3.076	537	540	545	rVB	831	644	0.08%	0.010%
9	3.105	545	549	553	rBV	862	851	0.10%	0.013%
10	3.176	563	571	573	rBV2	1620	2206	0.26%	0.034%
11	3.340	615	622	628	rBV	900	1439	0.17%	0.022%
12	3.369	628	631	634	rVB	1024	630	0.07%	0.010%
13	3.491	662	669	672	rBV2	1090	1280	0.15%	0.020%
14	3.533	679	682	689	rVB2	606	559	0.07%	0.009%
15	3.713	733	738	743	rBV2	820	930	0.11%	0.014%
16	3.739	743	746	752	rVB2	717	740	0.09%	0.011%
17	3.851	775	781	783	rBV3	582	637	0.08%	0.010%
18	4.012	826	831	834	rVB	681	611	0.07%	0.009%
19	4.124	862	866	871	rVB	1080	885	0.10%	0.013%
20	4.282	911	915	921	rVB	999	1006	0.12%	0.015%
21	4.330	925	930	935	rBV	540	556	0.07%	0.008%
22	4.359	936	939	942	rBV2	833	555	0.07%	0.008%
23	4.423	954	959	965	rBV	1529	2035	0.24%	0.031%
24	4.620	1005	1020	1044	rBV	108787	264582	31.33%	4.034%
25	4.835	1084	1087	1092	rVB3	789	657	0.08%	0.010%
26	5.063	1141	1158	1176	rBV2	167331	371565	44.00%	5.664%
27	5.411	1262	1266	1270	rBV	1211	1044	0.12%	0.016%
28	5.523	1295	1301	1302	rBV2	637	670	0.08%	0.010%
29	5.578	1313	1318	1322	rBV	497	554	0.07%	0.008%
30	5.726	1341	1364	1382	rBV2	301864	844507	100.00%	12.874%
31	5.790	1382	1384	1387	rVB	982	551	0.07%	0.008%
32	5.880	1409	1412	1416	rBV2	797	591	0.07%	0.009%
33	5.989	1442	1446	1450	rBV	1124	1061	0.13%	0.016%
34	6.063	1465	1469	1473	rBV	1228	1171	0.14%	0.018%
35	6.102	1477	1481	1487	rVV2	703	851	0.10%	0.013%
36	6.250	1514	1527	1547	rVV	260446	493822	58.47%	7.528%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049098.D
 Acq On : 12 Jun 2022 17:57
 Operator : SY/MD
 Sample : N3255-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.420	1575	1580	1584	rBV2	1041	883	0.10%	0.013%
38	6.539	1607	1617	1633	rVB6	29057	56718	6.72%	0.865%
39	6.690	1649	1664	1685	rBV	205092	400308	47.40%	6.103%
40	6.777	1687	1691	1694	rVB2	1002	801	0.09%	0.012%
41	7.015	1760	1765	1769	rVB2	643	757	0.09%	0.012%
42	7.134	1798	1802	1804	rBV	878	646	0.08%	0.010%
43	7.173	1811	1814	1822	rBV4	914	1000	0.12%	0.015%
44	7.308	1853	1856	1861	rBV2	486	574	0.07%	0.009%
45	7.401	1882	1885	1889	rVB	889	667	0.08%	0.010%
46	7.439	1894	1897	1900	rBV	797	547	0.06%	0.008%
47	7.517	1915	1921	1925	rBV	1079	1465	0.17%	0.022%
48	7.565	1925	1936	1952	rVV	92441	160080	18.96%	2.440%
49	7.684	1969	1973	1977	rBV3	1704	1324	0.16%	0.020%
50	7.729	1984	1987	1992	rVB	897	596	0.07%	0.009%
51	7.896	2025	2039	2054	rBV	349177	612640	72.54%	9.340%
52	8.121	2105	2109	2111	rBV	839	553	0.07%	0.008%
53	8.179	2115	2127	2141	rBV	67386	112616	13.34%	1.717%
54	8.536	2233	2238	2241	rBV	839	763	0.09%	0.012%
55	8.632	2255	2268	2302	rBV2	275936	542371	64.22%	8.268%
56	8.918	2352	2357	2359	rBV	922	898	0.11%	0.014%
57	8.935	2359	2362	2368	rVB	1155	941	0.11%	0.014%
58	9.028	2387	2391	2394	rBV2	711	564	0.07%	0.009%
59	9.417	2499	2512	2537	rBV	366325	609935	72.22%	9.298%
60	9.867	2646	2652	2656	rVV	892	811	0.10%	0.012%
61	9.893	2656	2660	2663	rBV	680	627	0.07%	0.010%
62	10.221	2756	2762	2765	rBV2	881	1026	0.12%	0.016%
63	10.349	2798	2802	2806	rVB	804	738	0.09%	0.011%
64	10.652	2890	2896	2899	rBV	573	667	0.08%	0.010%
65	10.690	2903	2908	2910	rBV2	703	631	0.07%	0.010%
66	10.758	2916	2929	2947	rVB	320289	521680	61.77%	7.953%
67	10.832	2947	2952	2954	rBV	1035	889	0.11%	0.014%
68	10.880	2963	2967	2970	rBV	939	813	0.10%	0.012%
69	10.989	2998	3001	3006	rVV	953	982	0.12%	0.015%
70	11.015	3006	3009	3013	rVV	892	698	0.08%	0.011%
71	11.082	3027	3030	3034	rVB	1078	799	0.09%	0.012%
72	11.439	3138	3141	3146	rVB	802	630	0.07%	0.010%
73	11.471	3146	3151	3154	rBV	719	794	0.09%	0.012%
74	11.812	3244	3257	3273	rBV	312467	501355	59.37%	7.643%
75	11.922	3287	3291	3294	rBV2	744	629	0.07%	0.010%
76	11.957	3298	3302	3307	rBV2	720	761	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049098.D
 Acq On : 12 Jun 2022 17:57
 Operator : SY/MD
 Sample : N3255-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.996	3311	3314	3318	rVB	832	599	0.07%	0.009%
78	12.057	3329	3333	3336	rBV	997	759	0.09%	0.012%
79	12.076	3336	3339	3344	rVB2	662	559	0.07%	0.009%
80	12.192	3363	3375	3396	rBV	340183	557939	66.07%	8.506%
81	12.269	3396	3399	3403	rBV4	677	605	0.07%	0.009%
82	12.430	3444	3449	3454	rVB	630	725	0.09%	0.011%
83	12.590	3493	3499	3503	rBV	722	756	0.09%	0.012%
84	12.812	3565	3568	3573	rBV	844	578	0.07%	0.009%
85	12.999	3622	3626	3628	rBV	680	613	0.07%	0.009%
86	13.111	3656	3661	3665	rBV	791	774	0.09%	0.012%
87	13.153	3671	3674	3679	rBV	1157	1031	0.12%	0.016%
88	13.420	3753	3757	3761	rBV2	933	825	0.10%	0.013%
89	13.484	3774	3777	3781	rBV2	741	661	0.08%	0.010%
90	13.722	3848	3851	3857	rBV2	660	708	0.08%	0.011%
91	13.915	3908	3911	3915	rBV2	897	726	0.09%	0.011%
92	13.973	3924	3929	3932	rBV2	618	556	0.07%	0.008%
93	14.137	3977	3980	3986	rVB3	665	720	0.09%	0.011%
94	14.372	4050	4053	4056	rBV	901	562	0.07%	0.009%
95	14.523	4096	4100	4103	rBV	911	794	0.09%	0.012%
96	14.545	4103	4107	4111	rVV3	665	727	0.09%	0.011%
97	14.626	4129	4132	4138	rBV3	705	721	0.09%	0.011%
98	14.873	4206	4209	4212	rBV2	711	584	0.07%	0.009%
99	15.568	4421	4425	4426	rBV2	1108	869	0.10%	0.013%
100	16.304	4651	4654	4656	rBV4	1116	684	0.08%	0.010%




Sum of corrected areas: 6559539

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049098.D
Acq On : 12 Jun 2022 17:57
Operator : SY/MD
Sample : N3255-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

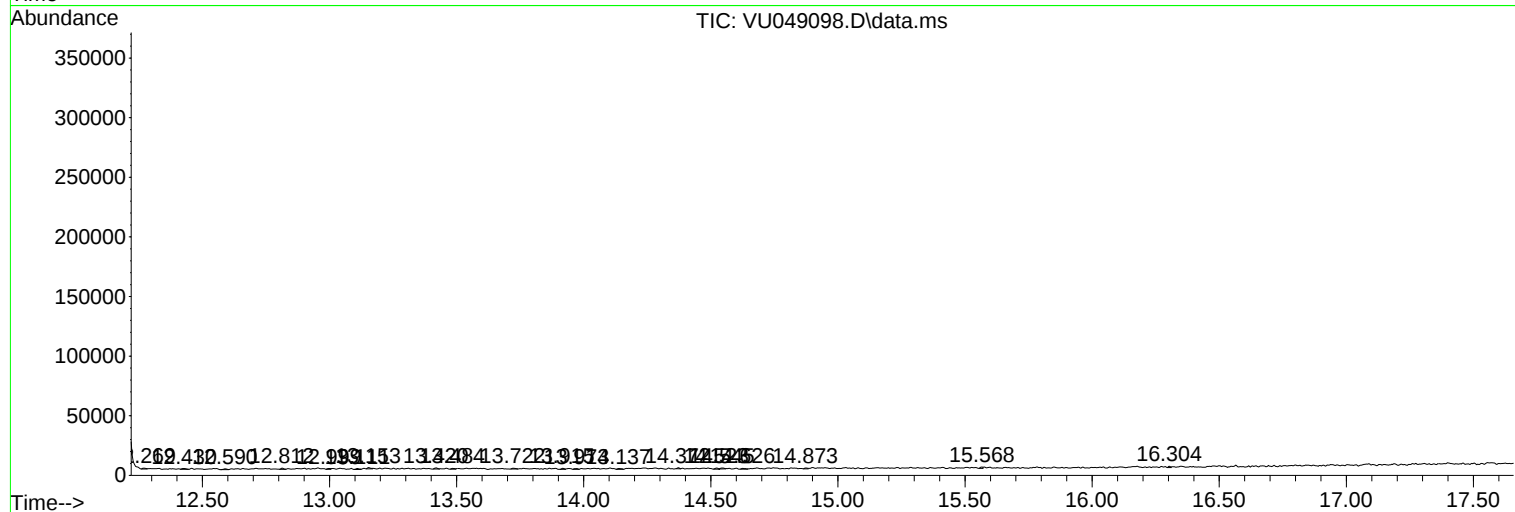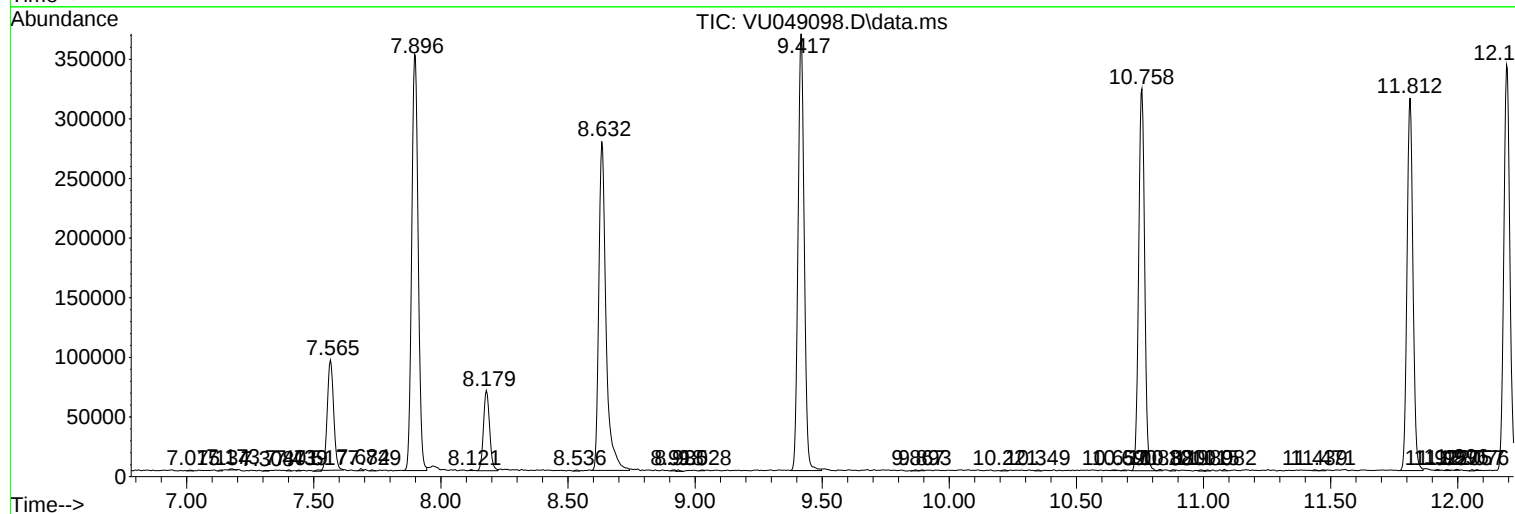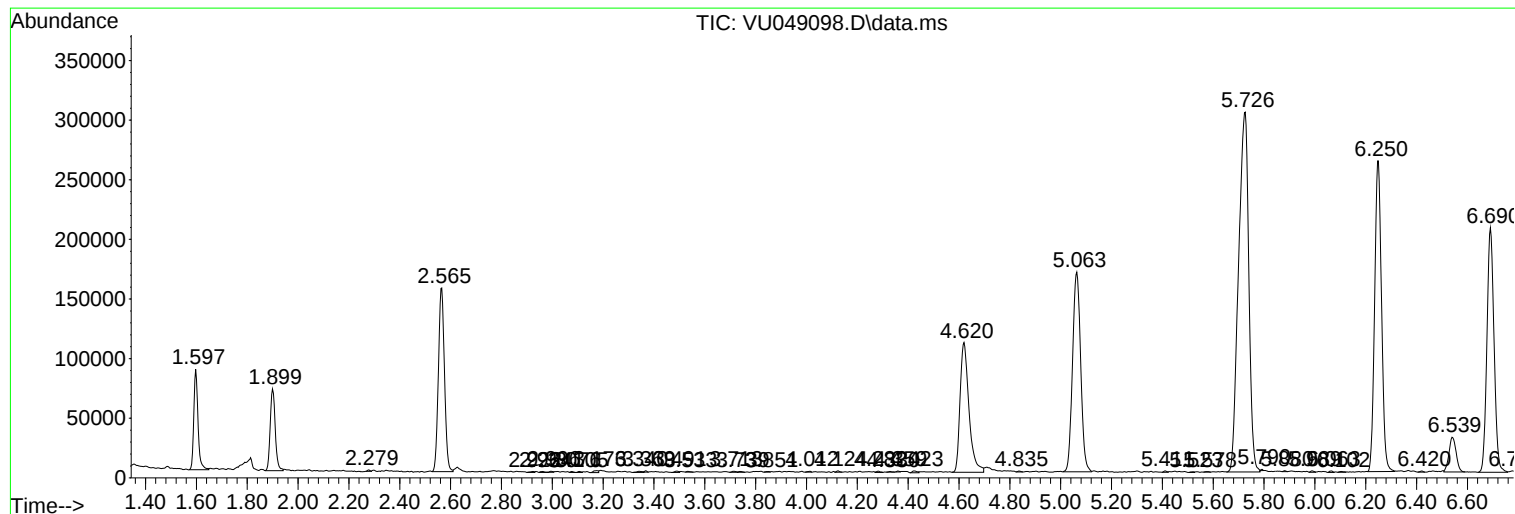

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049098.D
Acq On : 12 Jun 2022 17:57
Operator : SY/MD
Sample : N3255-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049098.D
Acq On : 12 Jun 2022 17:57
Operator : SY/MD
Sample : N3255-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------