

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049099.D
 Acq On : 12 Jun 2022 18:20
 Operator : SY/MD
 Sample : N3255-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049099.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	101	rVB	87664	105593	11.67%	1.510%
2	1.903	168	175	191	rVB	73676	95982	10.60%	1.372%
3	2.237	277	279	282	rBV	571	431	0.05%	0.006%
4	2.465	347	350	355	rBV3	614	731	0.08%	0.010%
5	2.565	368	381	400	rBV	163072	278249	30.74%	3.978%
6	3.060	532	535	537	rBV2	501	348	0.04%	0.005%
7	3.141	556	560	563	rBV	916	617	0.07%	0.009%
8	3.350	620	625	627	rBV	644	747	0.08%	0.011%
9	3.427	645	649	651	rBV2	555	336	0.04%	0.005%
10	3.443	651	654	657	rBV	656	332	0.04%	0.005%
11	3.475	662	664	666	rBV	529	340	0.04%	0.005%
12	3.662	719	722	724	rBV	954	655	0.07%	0.009%
13	3.758	749	752	754	rBV	743	508	0.06%	0.007%
14	3.829	771	774	776	rBV	358	234	0.03%	0.003%
15	3.922	800	803	808	rVB	665	576	0.06%	0.008%
16	4.099	855	858	861	rBV2	626	466	0.05%	0.007%
17	4.147	867	873	876	rBV	664	721	0.08%	0.010%
18	4.295	917	919	921	rBV	554	291	0.03%	0.004%
19	4.510	982	986	991	rVB	726	639	0.07%	0.009%
20	4.626	1009	1022	1056	rBV	106320	295149	32.61%	4.219%
21	4.838	1086	1088	1091	rBV	692	439	0.05%	0.006%
22	4.896	1103	1106	1108	rBV	490	314	0.03%	0.004%
23	5.063	1140	1158	1177	rBV	176295	388428	42.91%	5.553%
24	5.215	1202	1205	1208	rBV	562	456	0.05%	0.007%
25	5.234	1208	1211	1214	rVV	615	432	0.05%	0.006%
26	5.272	1220	1223	1225	rBV	783	516	0.06%	0.007%
27	5.395	1258	1261	1265	rBV	768	531	0.06%	0.008%
28	5.446	1274	1277	1280	rBV	532	295	0.03%	0.004%
29	5.510	1293	1297	1304	rVB	869	1102	0.12%	0.016%
30	5.552	1306	1310	1316	rBV	1012	1013	0.11%	0.014%
31	5.633	1332	1335	1336	rBV	696	465	0.05%	0.007%
32	5.723	1343	1363	1385	rBV2	324722	905188	100.00%	12.940%
33	5.870	1406	1409	1412	rBV2	518	438	0.05%	0.006%
34	5.906	1417	1420	1422	rBV	695	485	0.05%	0.007%
35	5.967	1435	1439	1444	rBV3	1068	967	0.11%	0.014%
36	6.031	1456	1459	1461	rBV	460	344	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049099.D
 Acq On : 12 Jun 2022 18:20
 Operator : SY/MD
 Sample : N3255-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.115	1481	1485	1490	rBV2	695	620	0.07%	0.009%
38	6.141	1490	1493	1496	rVB	744	376	0.04%	0.005%
39	6.250	1512	1527	1544	rBV	306135	587115	64.86%	8.393%
40	6.475	1595	1597	1600	rVB	575	282	0.03%	0.004%
41	6.581	1627	1630	1633	rBV	503	335	0.04%	0.005%
42	6.690	1646	1664	1680	rBV2	216870	420171	46.42%	6.007%
43	6.835	1704	1709	1712	rBV	566	582	0.06%	0.008%
44	6.964	1740	1749	1752	rVB	581	805	0.09%	0.012%
45	6.983	1752	1755	1757	rBV	532	315	0.03%	0.005%
46	6.999	1757	1760	1761	rBV	506	287	0.03%	0.004%
47	7.099	1788	1791	1793	rBV2	688	455	0.05%	0.007%
48	7.494	1912	1914	1917	rVB	746	439	0.05%	0.006%
49	7.513	1917	1920	1923	rBV	961	620	0.07%	0.009%
50	7.565	1923	1936	1950	rVV	92933	167010	18.45%	2.388%
51	7.838	2018	2021	2022	rBV	504	286	0.03%	0.004%
52	7.896	2027	2039	2056	rBV	367533	643760	71.12%	9.203%
53	8.179	2115	2127	2144	rBV	71018	116774	12.90%	1.669%
54	8.388	2186	2192	2197	rBV2	1085	1541	0.17%	0.022%
55	8.513	2228	2231	2233	rBV	501	275	0.03%	0.004%
56	8.568	2245	2248	2253	rBV	673	587	0.06%	0.008%
57	8.636	2258	2269	2299	rVV2	295652	575800	63.61%	8.231%
58	8.822	2326	2327	2330	rVB3	740	312	0.03%	0.004%
59	8.845	2330	2334	2338	rVB	1015	707	0.08%	0.010%
60	8.874	2338	2343	2348	rBV	936	736	0.08%	0.011%
61	8.899	2348	2351	2353	rBV2	735	384	0.04%	0.005%
62	8.935	2358	2362	2366	rBV2	1150	1033	0.11%	0.015%
63	8.973	2371	2374	2375	rBV	427	230	0.03%	0.003%
64	9.066	2399	2403	2408	rBV	813	933	0.10%	0.013%
65	9.095	2408	2412	2416	rVB	720	604	0.07%	0.009%
66	9.121	2416	2420	2425	rBV	746	676	0.07%	0.010%
67	9.144	2425	2427	2430	rBV2	560	396	0.04%	0.006%
68	9.198	2441	2444	2446	rBV2	498	345	0.04%	0.005%
69	9.285	2469	2471	2475	rVB	837	443	0.05%	0.006%
70	9.349	2488	2491	2493	rBV	524	385	0.04%	0.006%
71	9.417	2500	2512	2542	rBV	428768	713527	78.83%	10.200%
72	9.584	2560	2564	2565	rBV	609	431	0.05%	0.006%
73	9.976	2684	2686	2688	rBV	505	314	0.03%	0.004%
74	10.166	2738	2745	2748	rBV	1003	1218	0.13%	0.017%
75	10.243	2766	2769	2770	rBV	382	227	0.03%	0.003%
76	10.378	2808	2811	2813	rBV	569	404	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049099.D
 Acq On : 12 Jun 2022 18:20
 Operator : SY/MD
 Sample : N3255-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	10.459	2833	2836	2839	rVB	535	319	0.04%	0.005%
78	10.497	2844	2848	2853	rBV	747	976	0.11%	0.014%
79	10.755	2916	2928	2951	rBV	323291	531142	58.68%	7.593%
80	10.928	2980	2982	2984	rBV	440	242	0.03%	0.003%
81	11.025	3009	3012	3016	rVB	457	275	0.03%	0.004%
82	11.057	3016	3022	3031	rBV2	552	980	0.11%	0.014%
83	11.227	3072	3075	3078	rBV	783	576	0.06%	0.008%
84	11.478	3150	3153	3156	rBV3	780	519	0.06%	0.007%
85	11.594	3185	3189	3191	rBV	1178	859	0.09%	0.012%
86	11.812	3245	3257	3271	rBV	354885	563727	62.28%	8.059%
87	11.899	3281	3284	3288	rBV2	990	731	0.08%	0.010%
88	11.973	3304	3307	3310	rBV2	757	492	0.05%	0.007%
89	12.105	3344	3348	3350	rBV	999	674	0.07%	0.010%
90	12.192	3363	3375	3390	rBV	346643	560010	61.87%	8.006%
91	12.327	3414	3417	3422	rVB	499	426	0.05%	0.006%
92	12.353	3422	3425	3429	rBV2	882	799	0.09%	0.011%
93	12.488	3464	3467	3471	rVB	698	410	0.05%	0.006%
94	12.513	3471	3475	3479	rBV	741	562	0.06%	0.008%
95	12.549	3482	3486	3490	rBV	1089	903	0.10%	0.013%
96	12.594	3495	3500	3502	rBV2	805	722	0.08%	0.010%
97	12.693	3527	3531	3535	rBV2	978	870	0.10%	0.012%
98	13.272	3708	3711	3717	rBV	718	725	0.08%	0.010%
99	13.520	3786	3788	3791	rBV2	610	402	0.04%	0.006%
100	13.889	3894	3903	3906	rBV2	1174	1686	0.19%	0.024%




Sum of corrected areas: 6995125

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049099.D
Acq On : 12 Jun 2022 18:20
Operator : SY/MD
Sample : N3255-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

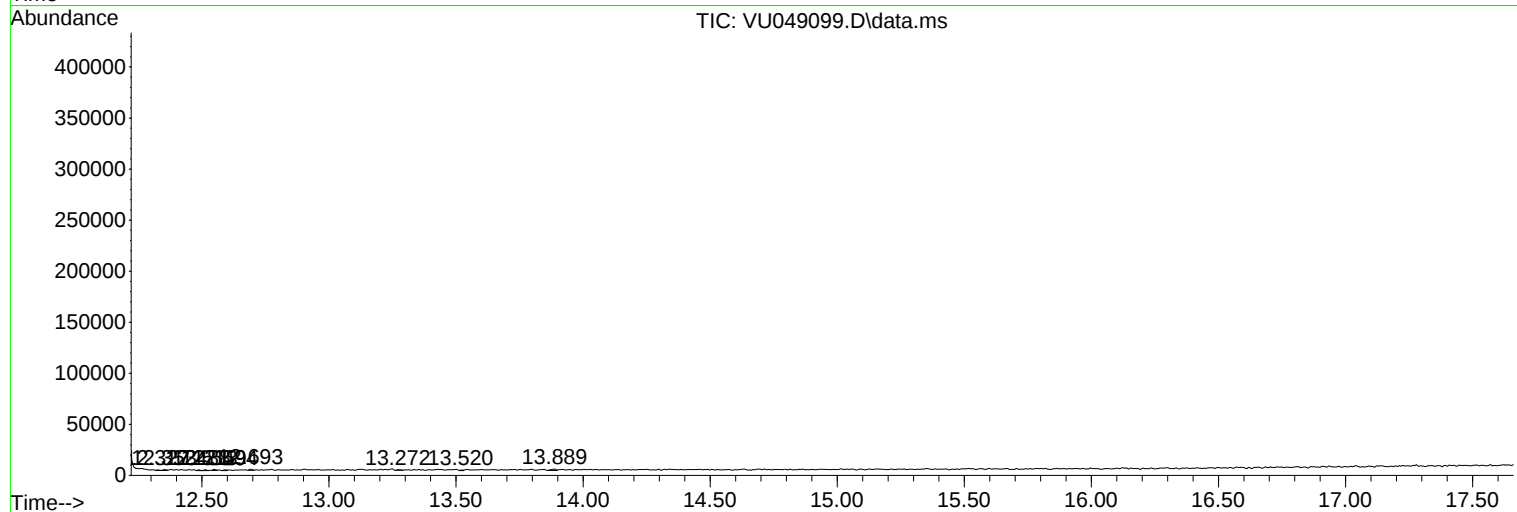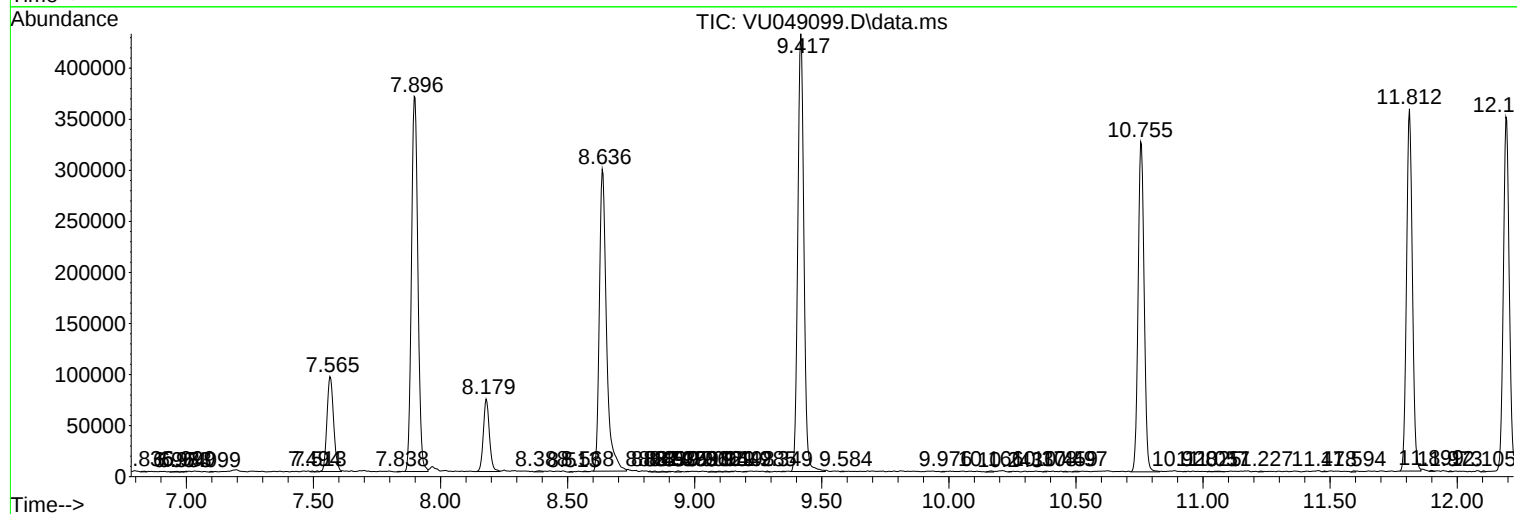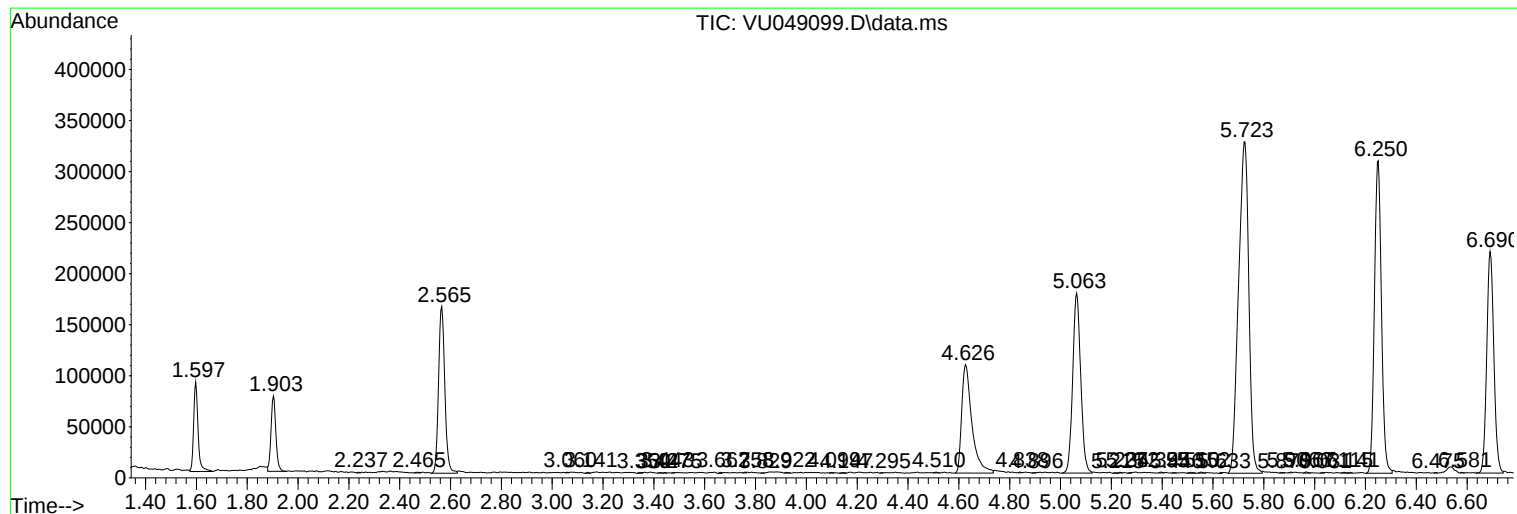

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049099.D
Acq On : 12 Jun 2022 18:20
Operator : SY/MD
Sample : N3255-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049099.D
Acq On : 12 Jun 2022 18:20
Operator : SY/MD
Sample : N3255-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------