

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049100.D
 Acq On : 12 Jun 2022 18:43
 Operator : SY/MD
 Sample : N3255-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

Signal : TIC: VU049100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.520	53	56	61	rVB3	1832	1521	0.17%	0.021%
2	1.597	72	80	97	rBV	86779	101587	11.30%	1.398%
3	1.903	168	175	190	rVB	72813	99177	11.04%	1.364%
4	1.977	195	198	204	rVB2	1132	1014	0.11%	0.014%
5	2.006	204	207	211	rBV3	855	771	0.09%	0.011%
6	2.234	274	278	282	rBV3	960	831	0.09%	0.011%
7	2.453	343	346	350	rBV	835	802	0.09%	0.011%
8	2.565	368	381	396	rBV2	168551	286965	31.93%	3.948%
9	2.810	454	457	460	rBV3	844	657	0.07%	0.009%
10	3.154	559	564	567	rBV2	709	775	0.09%	0.011%
11	3.359	620	628	630	rBV	546	608	0.07%	0.008%
12	3.375	630	633	639	rVB	725	765	0.09%	0.011%
13	3.507	670	674	680	rVB	1170	1118	0.12%	0.015%
14	3.623	704	710	714	rBV2	940	961	0.11%	0.013%
15	3.742	743	747	756	rVB2	1031	1190	0.13%	0.016%
16	3.784	756	760	763	rBV	993	836	0.09%	0.012%
17	3.851	777	781	785	rVV2	633	673	0.07%	0.009%
18	4.038	830	839	844	rBV	1010	1590	0.18%	0.022%
19	4.118	859	864	870	rVV	471	629	0.07%	0.009%
20	4.173	878	881	884	rVB	1775	1165	0.13%	0.016%
21	4.218	891	895	898	rBV	944	911	0.10%	0.013%
22	4.298	915	920	922	rBV2	639	631	0.07%	0.009%
23	4.382	944	946	956	rVB	837	1074	0.12%	0.015%
24	4.469	965	973	977	rBV	1338	1455	0.16%	0.020%
25	4.626	1009	1022	1053	rBV	103753	294921	32.82%	4.058%
26	4.906	1106	1109	1114	rVB	898	827	0.09%	0.011%
27	5.063	1141	1158	1180	rBV	173743	382068	42.52%	5.257%
28	5.314	1224	1236	1246	rBV6	4425	9788	1.09%	0.135%
29	5.372	1251	1254	1260	rBV2	629	783	0.09%	0.011%
30	5.514	1293	1298	1301	rBV2	717	639	0.07%	0.009%
31	5.723	1343	1363	1392	rBV2	324963	898654	100.00%	12.364%
32	5.858	1402	1405	1409	rBV2	976	842	0.09%	0.012%
33	5.925	1422	1426	1429	rBV4	707	680	0.08%	0.009%
34	6.108	1479	1483	1490	rVB2	734	862	0.10%	0.012%
35	6.173	1499	1503	1509	rBV2	700	624	0.07%	0.009%
36	6.250	1512	1527	1554	rBV	290659	556986	61.98%	7.663%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049100.D
 Acq On : 12 Jun 2022 18:43
 Operator : SY/MD
 Sample : N3255-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.391	1567	1571	1577	rBV3	1306	1576	0.18%	0.022%
38	6.481	1595	1599	1605	rVB	887	810	0.09%	0.011%
39	6.543	1605	1618	1635	rBV	197129	372759	41.48%	5.129%
40	6.690	1650	1664	1685	rBV	219951	421599	46.91%	5.800%
41	6.797	1693	1697	1702	rBV3	907	933	0.10%	0.013%
42	6.842	1708	1711	1719	rVB2	983	1138	0.13%	0.016%
43	6.935	1736	1740	1745	rBV	648	728	0.08%	0.010%
44	7.054	1773	1777	1784	rVB	1072	1131	0.13%	0.016%
45	7.112	1792	1795	1798	rVB	866	655	0.07%	0.009%
46	7.131	1798	1801	1807	rBV2	619	657	0.07%	0.009%
47	7.179	1811	1816	1817	rBV2	1892	1529	0.17%	0.021%
48	7.269	1839	1844	1850	rVB2	1020	1204	0.13%	0.017%
49	7.305	1850	1855	1862	rBV2	1263	1887	0.21%	0.026%
50	7.565	1924	1936	1953	rBV2	92525	166063	18.48%	2.285%
51	7.684	1967	1973	1975	rBV2	1134	1114	0.12%	0.015%
52	7.899	2026	2040	2057	rVV	367154	640760	71.30%	8.816%
53	8.179	2116	2127	2141	rBV	66252	115103	12.81%	1.584%
54	8.298	2160	2164	2168	rBV3	905	701	0.08%	0.010%
55	8.481	2216	2221	2232	rVB3	679	1486	0.17%	0.020%
56	8.530	2232	2236	2241	rBB	908	680	0.08%	0.009%
57	8.636	2257	2269	2297	rBV2	284584	560897	62.42%	7.717%
58	8.967	2369	2372	2382	rVB	829	1251	0.14%	0.017%
59	9.012	2382	2386	2392	rVB	795	818	0.09%	0.011%
60	9.211	2445	2448	2451	rBV2	847	741	0.08%	0.010%
61	9.253	2458	2461	2466	rBV2	851	765	0.09%	0.011%
62	9.311	2476	2479	2483	rBV	771	643	0.07%	0.009%
63	9.417	2499	2512	2529	rBV	401115	663340	73.81%	9.126%
64	9.575	2557	2561	2565	rBV2	835	629	0.07%	0.009%
65	9.620	2568	2575	2577	rBV	1311	1219	0.14%	0.017%
66	9.822	2635	2638	2645	rBV2	837	998	0.11%	0.014%
67	10.025	2696	2701	2707	rBV	1017	1377	0.15%	0.019%
68	10.340	2795	2799	2804	rBV	662	758	0.08%	0.010%
69	10.488	2841	2845	2849	rVB	1091	858	0.10%	0.012%
70	10.658	2892	2898	2903	rBV2	730	1042	0.12%	0.014%
71	10.755	2915	2928	2945	rBV	325892	529675	58.94%	7.287%
72	10.899	2970	2973	2976	rVB2	1123	686	0.08%	0.009%
73	11.031	3011	3014	3020	rBV	769	723	0.08%	0.010%
74	11.095	3031	3034	3038	rVV2	934	776	0.09%	0.011%
75	11.250	3077	3082	3087	rBV	766	1018	0.11%	0.014%
76	11.456	3143	3146	3149	rVB	826	610	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049100.D
 Acq On : 12 Jun 2022 18:43
 Operator : SY/MD
 Sample : N3255-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.607	3189	3193	3198	rBV2	800	927	0.10%	0.013%
78	11.812	3244	3257	3278	rBV	335076	529510	58.92%	7.285%
79	12.009	3313	3318	3323	rBV	779	865	0.10%	0.012%
80	12.192	3363	3375	3391	rVV	341263	561910	62.53%	7.731%
81	12.430	3441	3449	3453	rVB2	1122	1476	0.16%	0.020%
82	12.462	3453	3459	3461	rBV2	930	980	0.11%	0.013%
83	12.533	3475	3481	3485	rVB	1168	1336	0.15%	0.018%
84	12.555	3485	3488	3491	rBV2	1268	828	0.09%	0.011%
85	12.732	3539	3543	3546	rBV2	950	929	0.10%	0.013%
86	12.925	3599	3603	3606	rBV2	810	783	0.09%	0.011%
87	13.005	3625	3628	3633	rBV	847	720	0.08%	0.010%
88	13.121	3660	3664	3670	rVB2	886	877	0.10%	0.012%
89	13.311	3720	3723	3726	rBV2	753	618	0.07%	0.009%
90	13.600	3808	3813	3818	rBV2	951	1148	0.13%	0.016%
91	13.626	3818	3821	3825	rVB2	835	641	0.07%	0.009%
92	13.681	3835	3838	3841	rBV	1096	665	0.07%	0.009%
93	13.726	3847	3852	3855	rBV2	511	641	0.07%	0.009%
94	13.806	3870	3877	3881	rBV2	1152	1523	0.17%	0.021%
95	14.005	3935	3939	3943	rBV3	764	838	0.09%	0.012%
96	14.205	3998	4001	4007	rBV2	852	606	0.07%	0.008%
97	14.240	4008	4012	4017	rVV3	797	947	0.11%	0.013%
98	15.288	4334	4338	4345	rBV4	1014	1278	0.14%	0.018%
99	15.401	4370	4373	4376	rBV3	1223	882	0.10%	0.012%
100	16.060	4576	4578	4582	rBV	1106	732	0.08%	0.010%




Sum of corrected areas: 7268377

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049100.D
Acq On : 12 Jun 2022 18:43
Operator : SY/MD
Sample : N3255-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

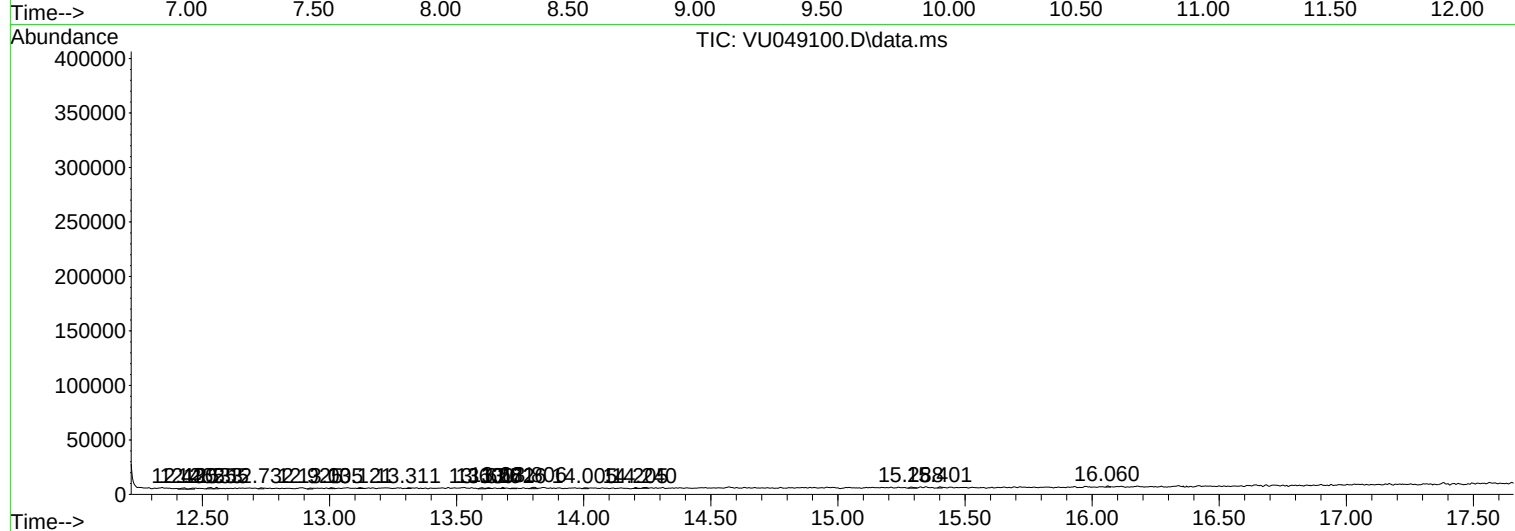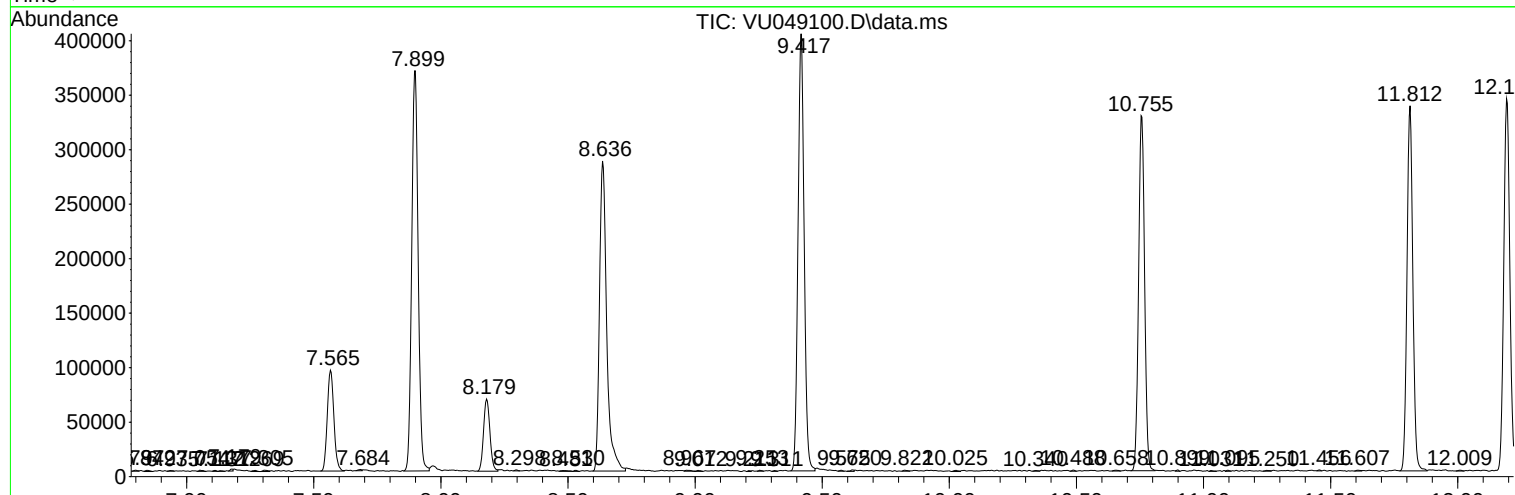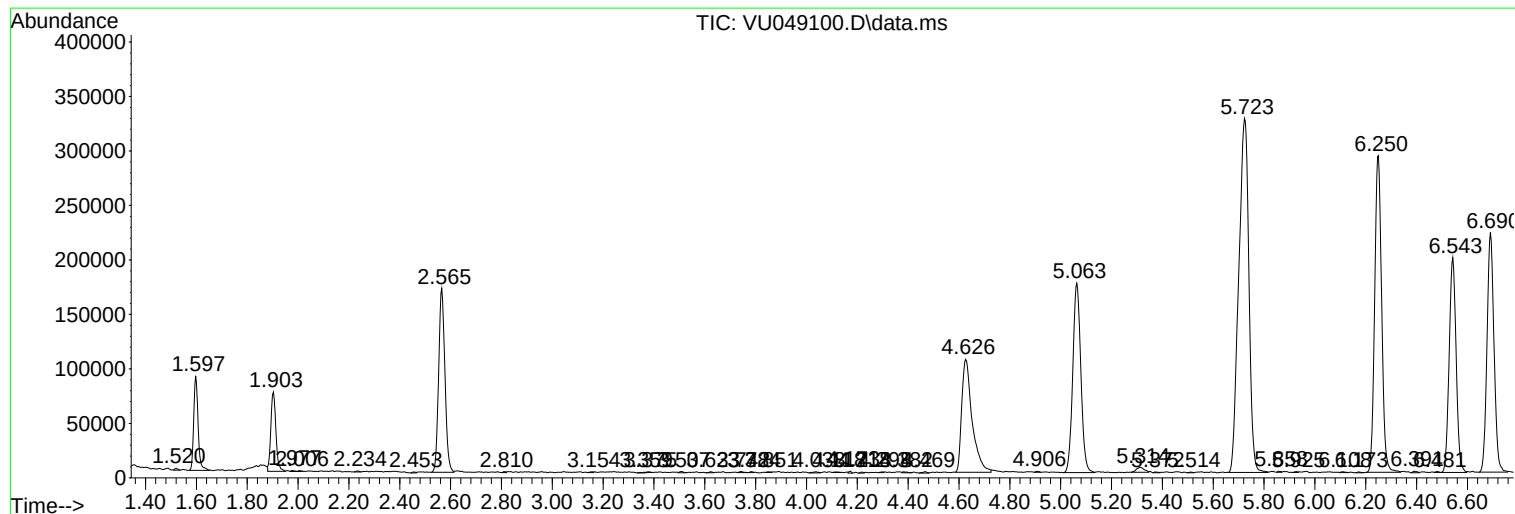

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049100.D
Acq On : 12 Jun 2022 18:43
Operator : SY/MD
Sample : N3255-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049100.D
Acq On : 12 Jun 2022 18:43
Operator : SY/MD
Sample : N3255-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------