
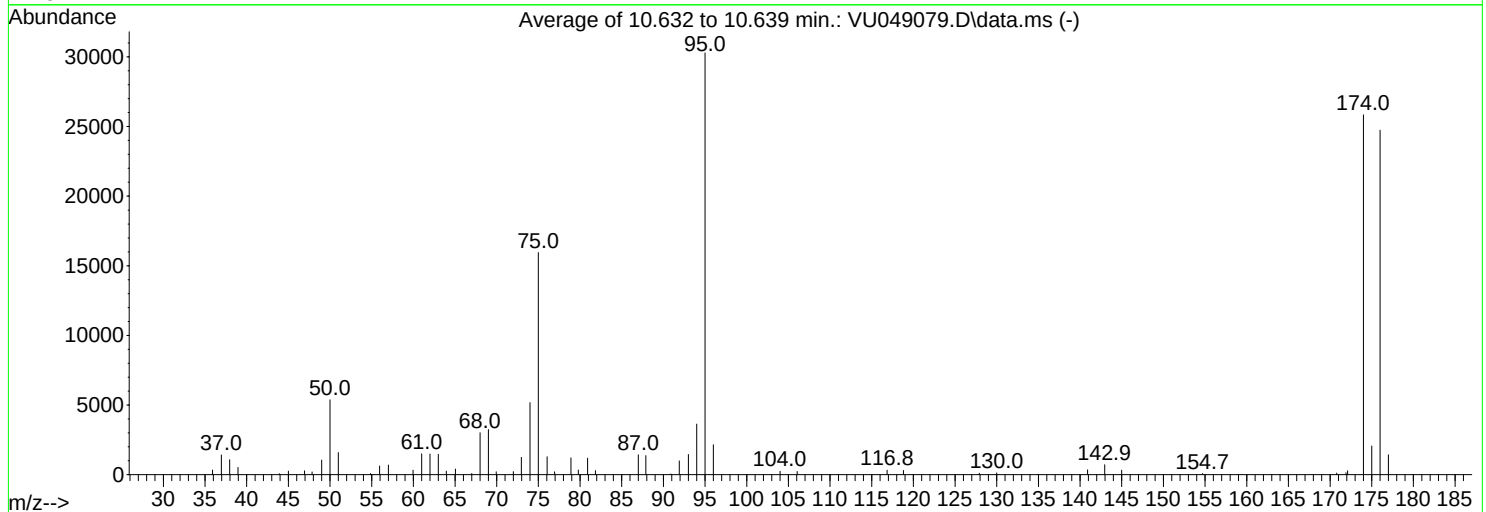


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049079.D
 Acq On : 12 Jun 2022 09:36
 Operator : SY/MD
 Sample : BFB096
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB096

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis
 Last Update : Mon Jun 13 05:01:30 2022

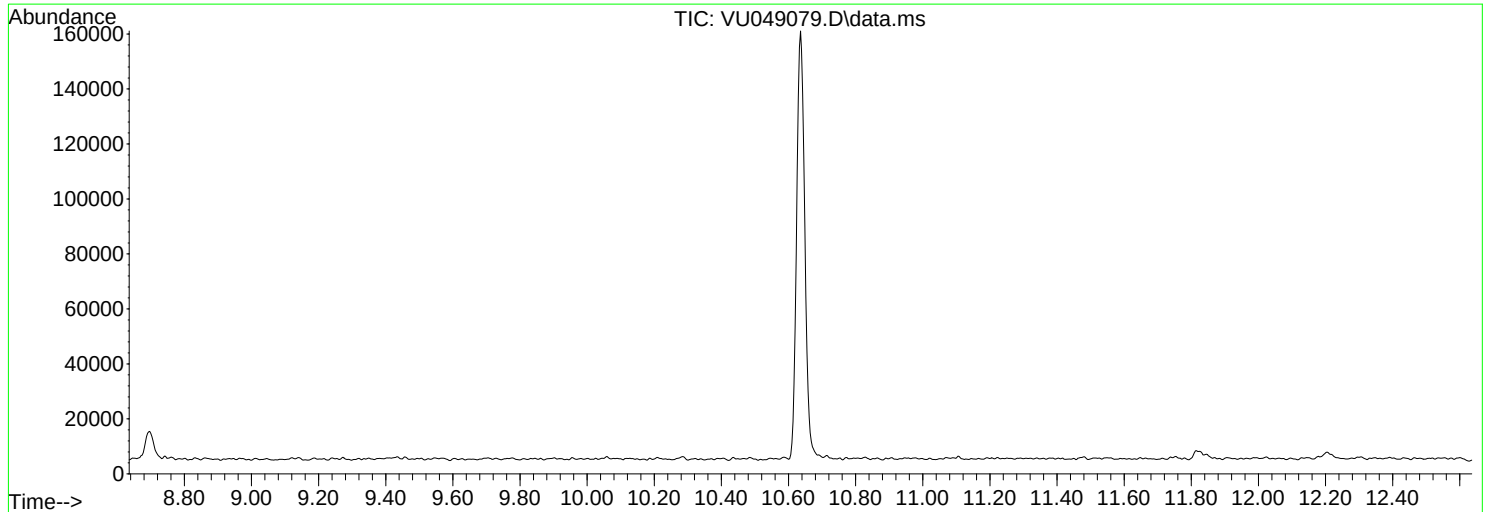

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	5373	PASS
75	95	30	80	52.7	15950	PASS
95	95	100	100	100.0	30291	PASS
96	95	5	9	7.1	2154	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.3	25843	PASS
175	174	5	9	8.0	2055	PASS
176	174	95	101	95.7	24736	PASS
177	176	5	9	5.8	1428	PASS

m/z	Abundance
39.90	5322.0
44.00	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096

m/z	Abundance
35.90	313.0
37.00	1318.0
38.00	1040.0
39.10	464.0
39.90	5232.0
43.90	317.0
45.00	257.0
47.00	353.0
47.90	213.0
49.00	942.0
50.00	5284.0
51.00	1675.0
54.80	115.0
56.00	570.0
57.00	723.0
59.90	306.0
61.00	1507.0
62.00	1516.0
63.00	1346.0
64.00	261.0
65.10	397.0
67.00	117.0
68.00	3201.0
69.00	3094.0
70.00	146.0
72.10	231.0
73.00	1150.0
74.00	5344.0
75.00	16021.0
76.00	1190.0
76.90	187.0
78.90	1233.0
79.80	306.0
80.90	1231.0
81.80	297.0
87.00	1422.0
87.90	1220.0
91.90	1026.0
93.00	1386.0
94.00	3661.0
95.00	30192.0
96.00	2087.0
104.00	263.0
106.00	163.0
116.90	308.0
118.90	339.0
130.00	100.0
140.90	391.0
142.90	707.0
145.00	334.0
154.70	129.0
170.90	127.0
171.90	400.0
174.00	25488.0
175.00	1947.0
176.00	24184.0
177.00	1406.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096

m/z	Abundance
35.90	361.0
36.90	1444.0
37.90	1067.0
38.90	480.0
39.90	5277.0
43.90	296.0
45.00	247.0
47.00	263.0
47.90	196.0
49.00	1080.0
50.00	5550.0
51.00	1605.0
54.90	135.0
55.90	679.0
57.00	724.0
59.90	333.0
61.00	1540.0
62.00	1488.0
63.00	1494.0
63.90	271.0
65.00	427.0
67.00	127.0
68.00	3146.0
69.00	3401.0
70.00	213.0
72.00	219.0
73.00	1302.0
74.00	5345.0
75.00	16257.0
76.00	1314.0
76.90	210.0
78.90	1225.0
79.80	349.0
80.90	1209.0
81.80	287.0
87.00	1485.0
87.90	1365.0
91.90	1024.0
93.00	1541.0
94.00	3728.0
95.00	31064.0
96.00	2210.0
104.00	265.0
106.10	264.0
116.90	336.0
118.80	316.0
127.90	158.0
130.00	125.0
140.90	348.0
143.00	729.0
145.00	344.0
154.70	126.0
170.80	104.0
172.10	431.0
174.00	26616.0
175.00	2104.0
176.00	25344.0
177.00	1463.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096

m/z	Abundance
35.90	331.0
37.00	1470.0
37.90	1089.0
38.90	607.0
39.90	5264.0
43.90	283.0
45.00	239.0
46.80	206.0
47.70	171.0
49.00	1107.0
50.00	5284.0
51.00	1490.0
55.90	606.0
57.00	634.0
60.00	320.0
61.00	1422.0
62.00	1433.0
63.00	1542.0
63.90	242.0
65.00	381.0
68.00	2693.0
69.00	3225.0
69.90	264.0
71.90	193.0
72.90	1268.0
74.00	4824.0
75.00	15571.0
76.10	1360.0
77.00	232.0
78.90	1178.0
79.80	347.0
80.90	1100.0
81.90	283.0
87.00	1378.0
87.90	1521.0
90.90	123.0
91.90	902.0
93.00	1424.0
94.00	3496.0
95.00	29616.0
96.00	2164.0
104.00	192.0
106.10	274.0
116.80	326.0
118.70	254.0
127.90	166.0
130.00	148.0
140.90	297.0
143.00	703.0
145.00	273.0
170.70	101.0
172.10	399.0
174.00	25424.0
175.00	2113.0
176.00	24680.0
177.00	1416.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096