


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061223\
Data File : VU054478.D
Acq On : 12 Jun 2023 10:11
Operator : MD/SY
Sample : BFB017
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB017

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Jun 14 00:05:43 2023

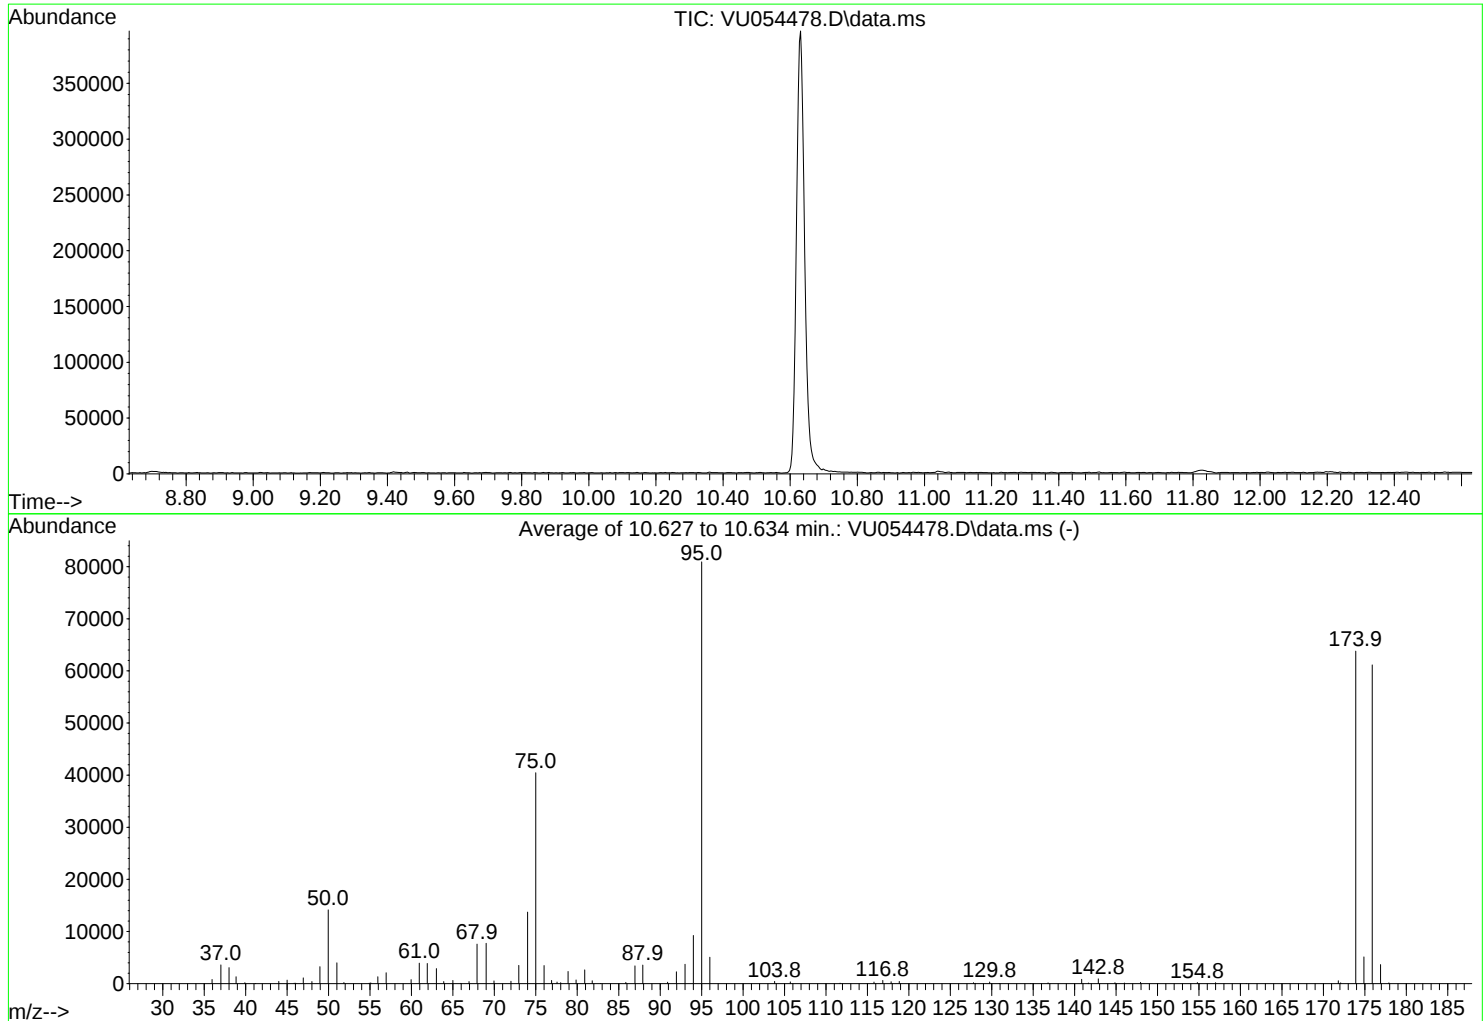

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	14164	PASS
75	95	30	80	50.0	40459	PASS
95	95	100	100	100.0	80920	PASS
96	95	5	9	6.3	5067	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.8	63795	PASS
175	174	5	9	8.0	5127	PASS
176	174	95	101	95.8	61147	PASS
177	176	5	9	6.0	3656	PASS

m/z	Abundance
39.90	271.0
44.00	642.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017

m/z	Abundance
35.90	815.0
37.00	3627.0
38.00	3189.0
38.90	1327.0
39.90	437.0
44.00	1012.0
45.00	637.0
45.80	134.0
46.10	129.0
46.90	1151.0
47.90	366.0
48.90	3314.0
50.00	14653.0
51.00	4123.0
51.80	244.0
54.90	249.0
55.90	1320.0
57.00	2072.0
59.90	883.0
61.00	3785.0
61.90	3997.0
63.00	2866.0
63.90	438.0
65.00	636.0
66.90	388.0
67.90	7673.0
69.00	7758.0
70.00	553.0
72.00	516.0
72.90	3548.0
74.00	13931.0
75.00	40576.0
76.00	3565.0
76.90	699.0
77.50	378.0
78.90	2398.0
79.80	751.0
80.90	2711.0
81.80	540.0
85.80	239.0
86.90	3523.0
87.90	3356.0
90.90	283.0
91.90	2416.0
93.00	3976.0
94.00	9157.0
95.00	83168.0
96.00	4778.0
103.80	416.0
105.70	378.0
111.70	136.0
115.80	263.0
116.80	646.0
117.80	387.0
118.90	434.0
127.80	321.0
129.70	385.0
130.90	104.0
135.00	102.0
136.80	191.0
140.90	966.0
141.70	103.0
142.90	953.0
144.90	208.0
146.10	103.0
147.90	239.0
154.80	245.0
157.00	147.0
160.70	103.0
171.80	465.0
172.10	469.0
173.90	63040.0
174.90	5023.0
175.90	59272.0
176.90	3623.0
177.90	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017

m/z	Abundance
35.90	859.0
37.00	3723.0
38.00	3156.0
38.90	1296.0
39.90	467.0
44.00	1080.0
45.00	703.0
45.90	126.0
47.00	1177.0
48.00	415.0
49.00	3400.0
50.00	14458.0
51.00	4034.0
51.90	210.0
55.10	234.0
55.90	1354.0
57.00	2133.0
59.90	772.0
61.00	4125.0
61.90	4010.0
63.00	2942.0
63.90	398.0
65.00	611.0
66.00	103.0
66.90	424.0
67.90	7713.0
69.00	7954.0
69.90	529.0
72.00	511.0
73.00	3585.0
74.00	14245.0
75.00	41616.0
76.00	3638.0
76.90	656.0
77.50	291.0
78.00	260.0
78.90	2427.0
79.90	686.0
80.90	2676.0
81.80	591.0
82.80	110.0
85.80	260.0
86.90	3540.0
87.90	3657.0
90.90	308.0
91.90	2273.0
93.00	3757.0
94.00	9553.0
95.00	83376.0
96.00	5186.0
103.80	432.0
105.70	355.0
111.70	125.0
115.80	302.0
116.90	651.0
117.80	388.0
118.80	475.0
127.80	271.0
129.70	293.0
136.80	188.0
140.90	858.0
141.60	135.0
142.90	945.0
144.80	206.0
146.00	131.0
147.90	251.0
154.80	213.0
157.00	190.0
171.80	561.0
173.90	65936.0
174.90	5348.0
175.90	63136.0
176.90	3749.0
177.90	173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017

m/z	Abundance
36.00	772.0
37.00	3432.0
38.00	2863.0
38.80	1381.0
39.90	464.0
41.20	100.0
44.00	1084.0
45.00	707.0
46.00	143.0
47.00	987.0
48.10	463.0
49.00	3040.0
49.90	13382.0
51.00	3805.0
51.90	183.0
55.10	199.0
56.00	1295.0
56.90	2039.0
60.00	657.0
60.90	3917.0
61.90	3629.0
63.00	2866.0
63.90	332.0
65.00	570.0
65.90	100.0
67.00	379.0
67.90	7361.0
69.00	7485.0
69.90	469.0
72.00	400.0
73.00	3393.0
74.00	12947.0
75.00	39184.0
76.00	3254.0
76.90	489.0
77.60	232.0
78.00	262.0
78.90	2193.0
79.90	667.0
80.90	2554.0
81.80	571.0
85.90	201.0
87.00	3196.0
87.90	3719.0
90.90	292.0
92.00	2096.0
93.00	3411.0
94.00	9052.0
95.00	76216.0
96.00	5238.0
103.80	410.0
105.70	306.0
115.80	358.0
116.90	547.0
117.90	375.0
118.80	416.0
128.00	233.0
129.80	240.0
134.70	108.0
136.70	126.0
140.80	675.0
141.60	128.0
142.80	879.0
144.80	160.0
145.90	170.0
148.00	219.0
154.80	204.0
157.00	222.0
171.80	614.0
173.90	62408.0
174.90	5010.0
175.90	61032.0
176.90	3595.0
177.90	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017