

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061224\
 Data File : VU059215.D
 Acq On : 12 Jun 2024 10:52
 Operator : MD/SY
 Sample : VU0612WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0612WBL01

Quant Time: Jun 13 03:00:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060524DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jun 06 08:51:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.110	96	40582	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	11768	0.852	ug/l	0.00
Spiked Amount	1.000		Recovery	=	85.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	12656	0.876	ug/l	0.00
Spiked Amount	1.000		Recovery	=	88.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061224\
Data File : VU059215.D
Acq On : 12 Jun 2024 10:52
Operator : MD/SY
Sample : VU0612WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0612WBL01

Quant Time: Jun 13 03:00:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jun 06 08:51:44 2024
Response via : Initial Calibration




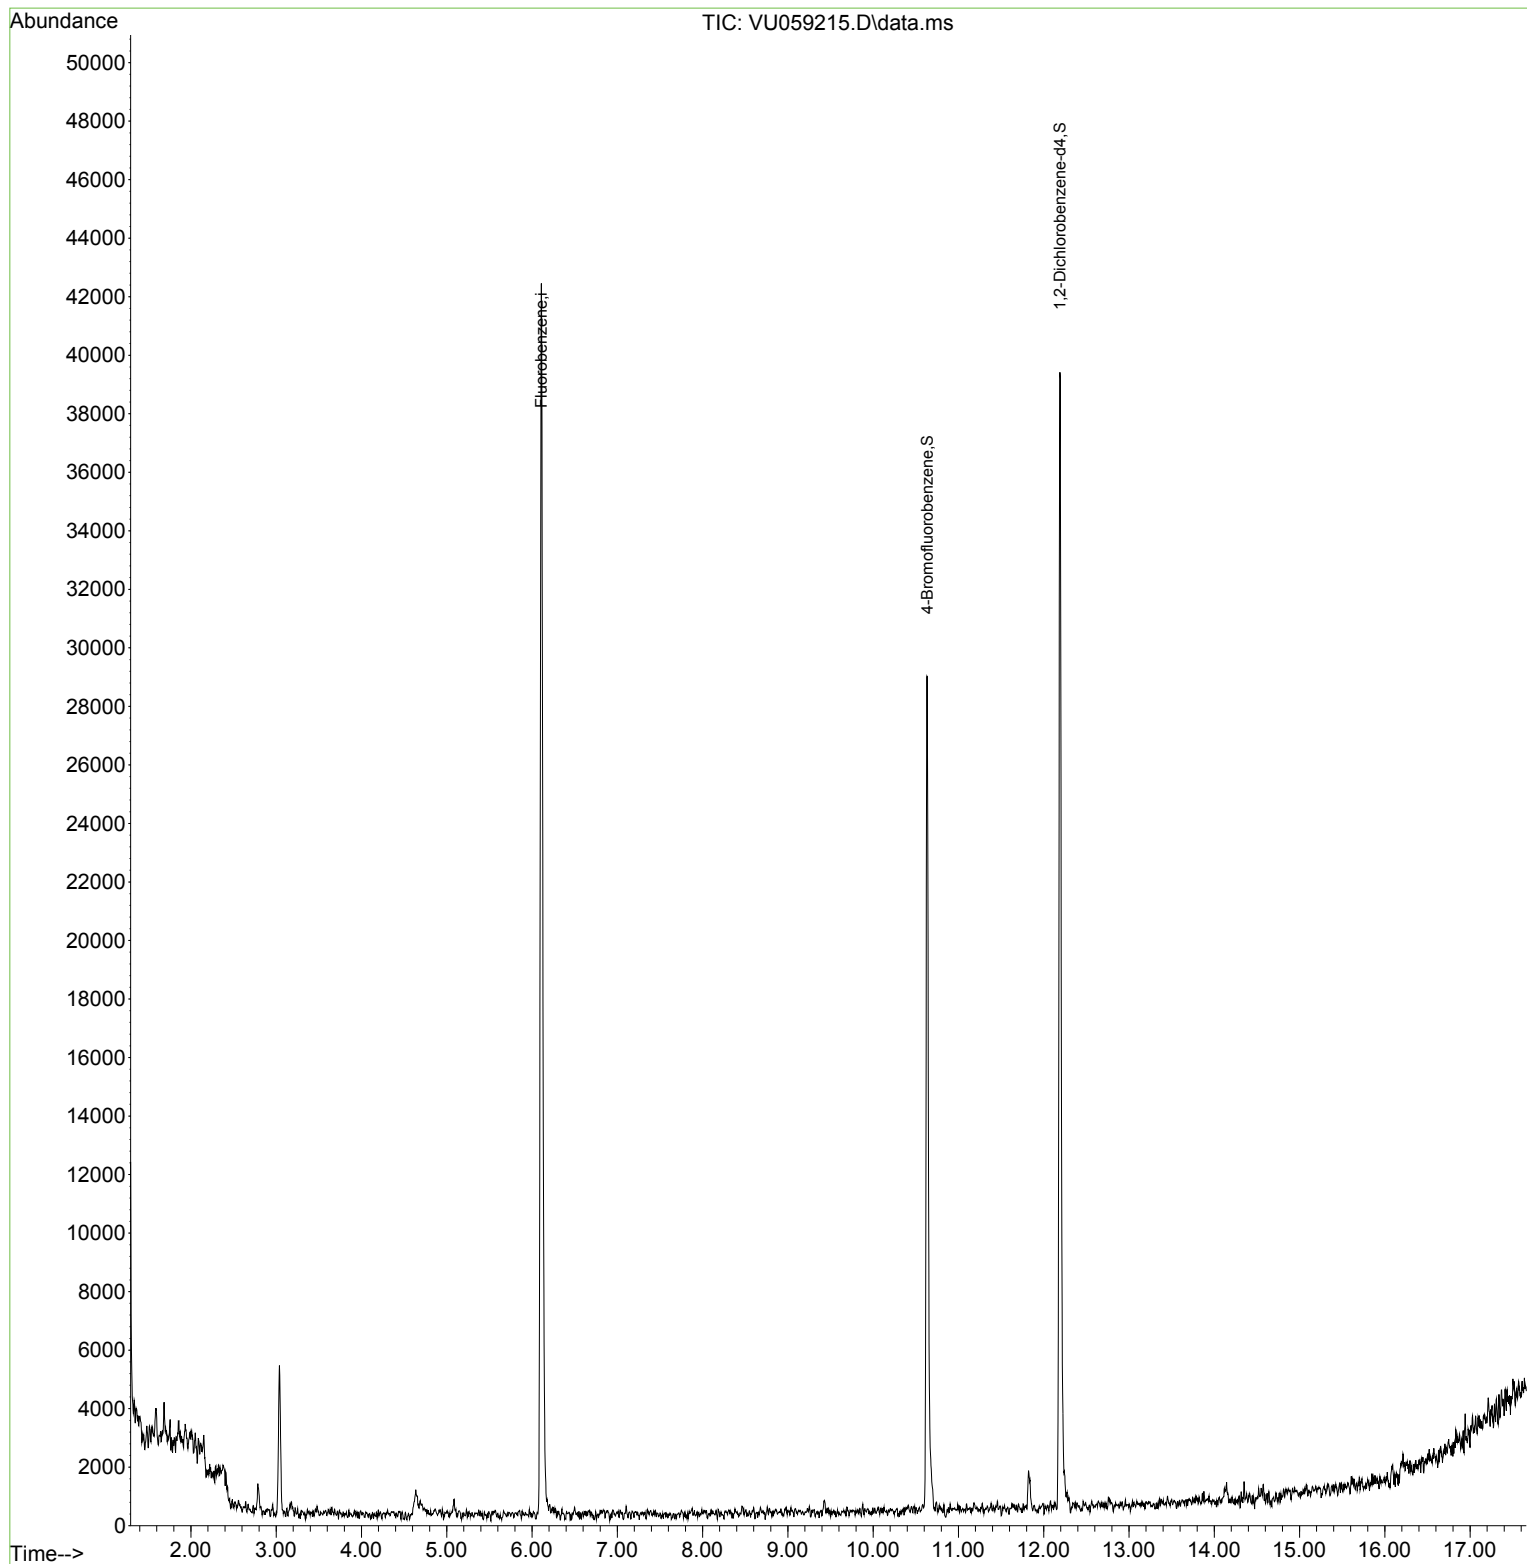


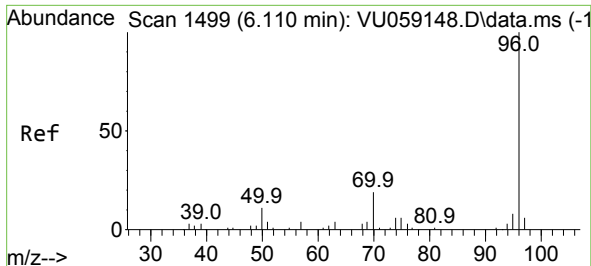

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.110 min Scan# 1499
Delta R.T. -0.000 min
Lab File: VU059215.D
Acq: 12 Jun 2024 10:52




Instrument :
MSVOA_U
ClientSampleId :
VU0612WBL01


Tgt Ion: 96	Resp: 40582
Ion Ratio	Lower Upper
96 100	
70 21.5	16.6 24.8
95 10.3	7.1 10.7
97 6.1	0.0 0.0#

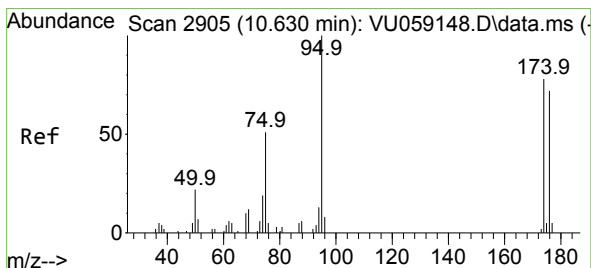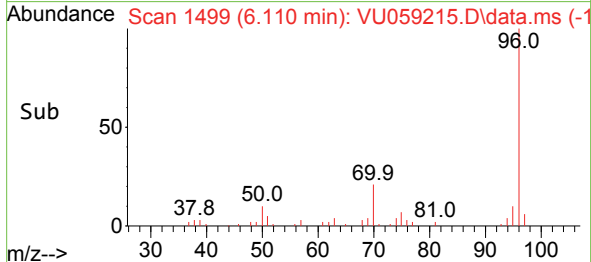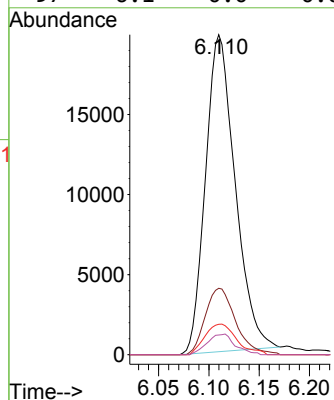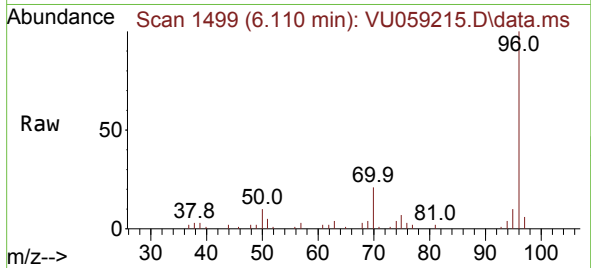

#57
4-Bromofluorobenzene
Concen: 0.852 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.003 min
Lab File: VU059215.D
Acq: 12 Jun 2024 10:52


Tgt Ion: 95	Resp: 11768
Ion Ratio	Lower Upper
95 100	
174 80.5	59.6 89.4
176 75.7	57.3 85.9

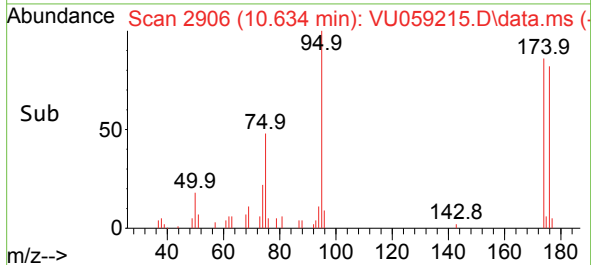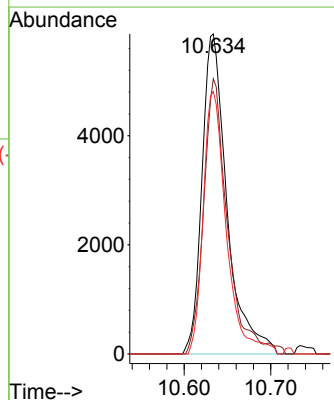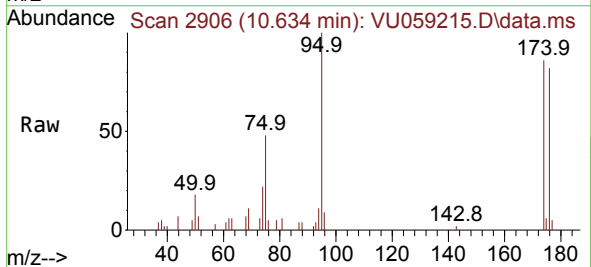

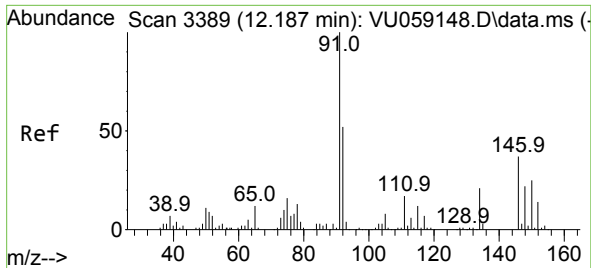

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.876 ug/l
 RT: 12.190 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU059215.D
 Acq: 12 Jun 2024 10:52

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0612WBL01

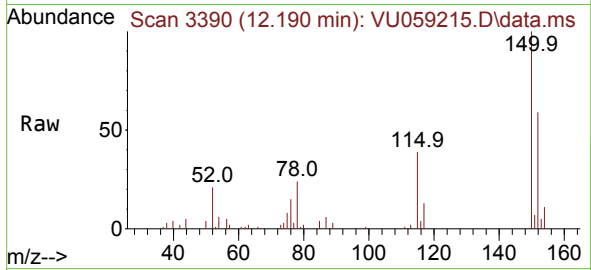

Tgt Ion:152 Resp: 12656
 Ion Ratio Lower Upper
 152 100
 115 61.1 0.0 293.2
 150 155.8 0.0 636.0

