


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061224\
Data File : VU059213.D
Acq On : 12 Jun 2024 08:12
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060524DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Jun 06 08:51:44 2024

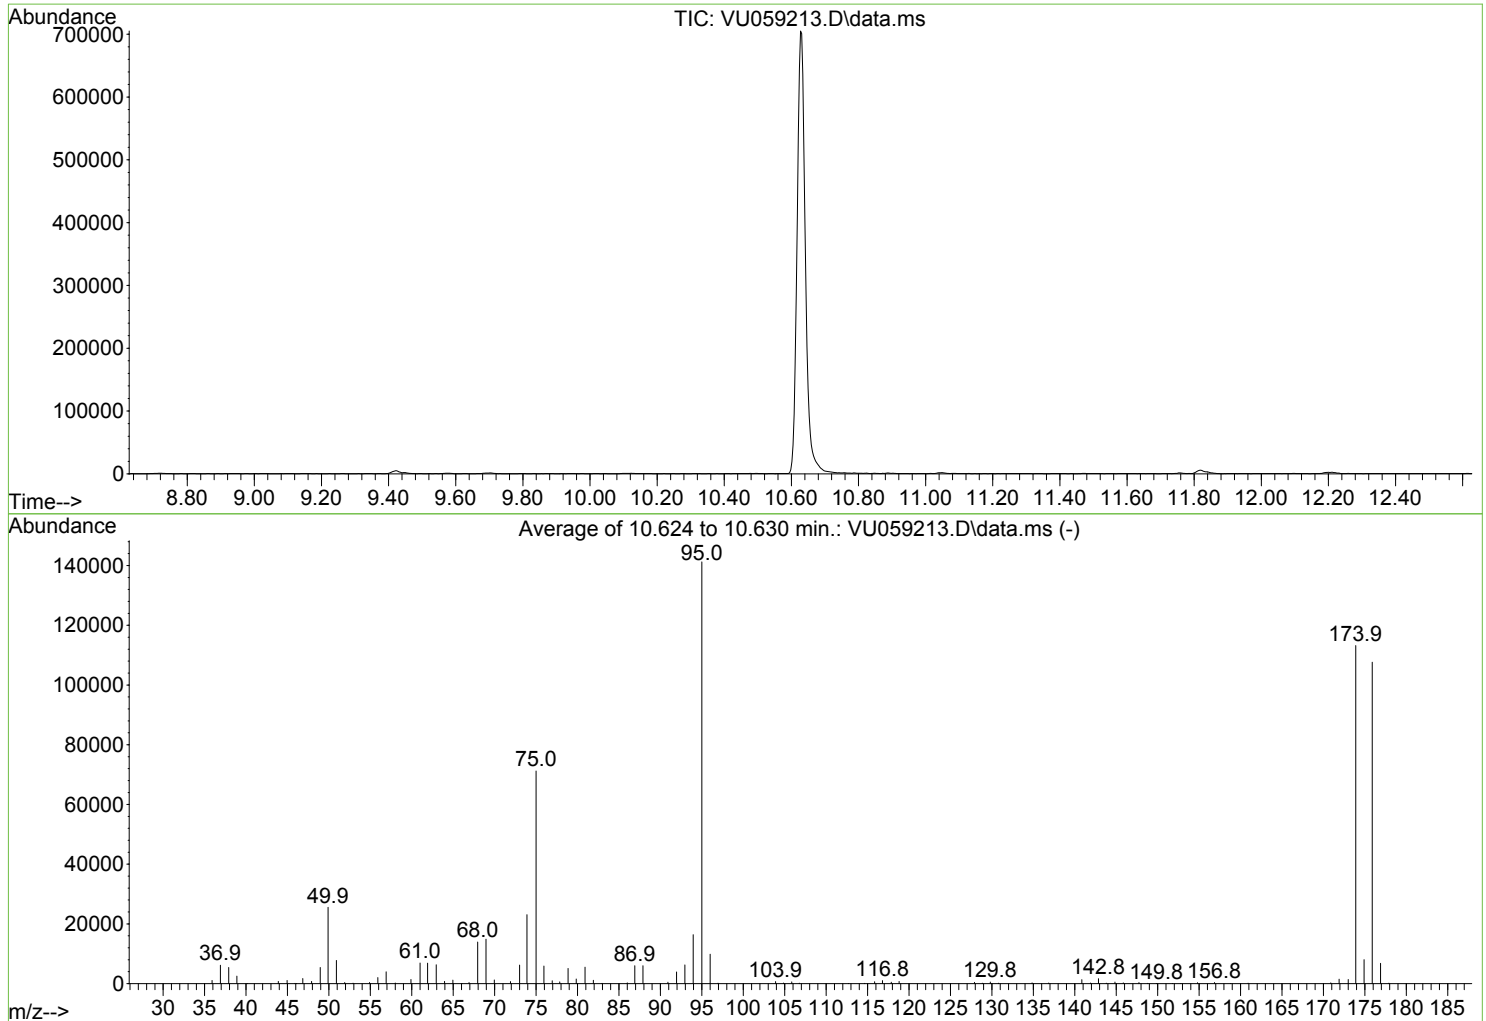

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	25549	PASS
75	95	30	60	50.4	71187	PASS
95	95	100	100	100.0	141248	PASS
96	95	5	9	7.0	9871	PASS
173	174	0.00	2	1.2	1376	PASS
174	95	50	100	80.2	113235	PASS
175	174	5	9	7.1	8038	PASS
176	174	95	101	95.0	107624	PASS
177	176	5	9	6.3	6796	PASS