




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061225\
Data File : VU063393.D
Acq On : 12 Jun 2025 11:43
Operator : MD/SY
Sample : Q2117-02
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/17/2025
Supervised By :Mahesh Dadoda 06/17/2025

Quant Time: Jun 16 08:40:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jun 16 08:39:07 2025
Response via : Initial Calibration

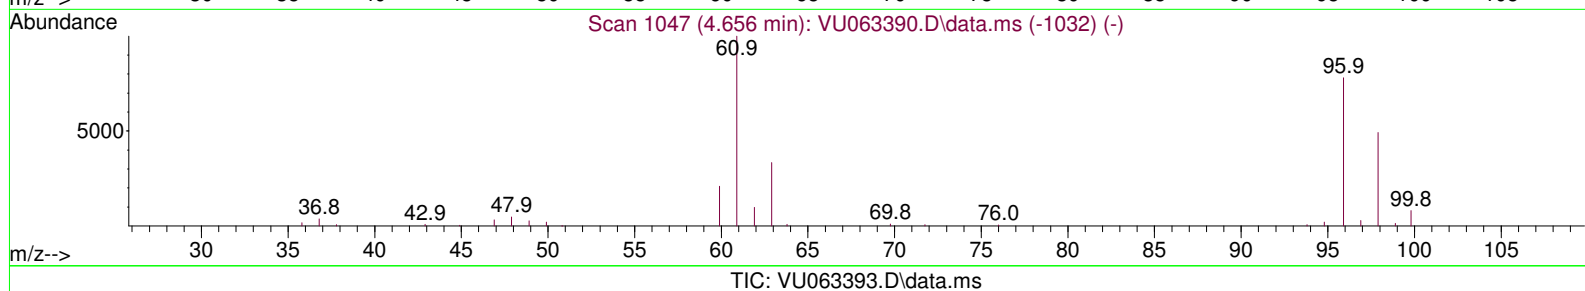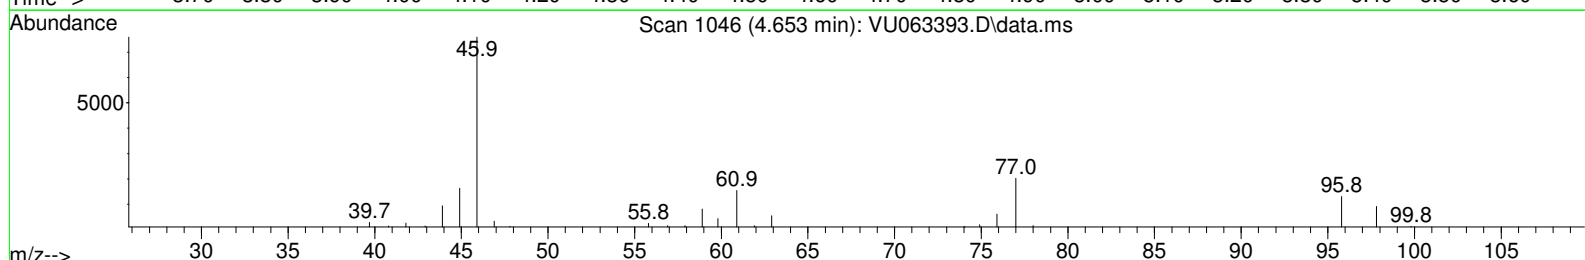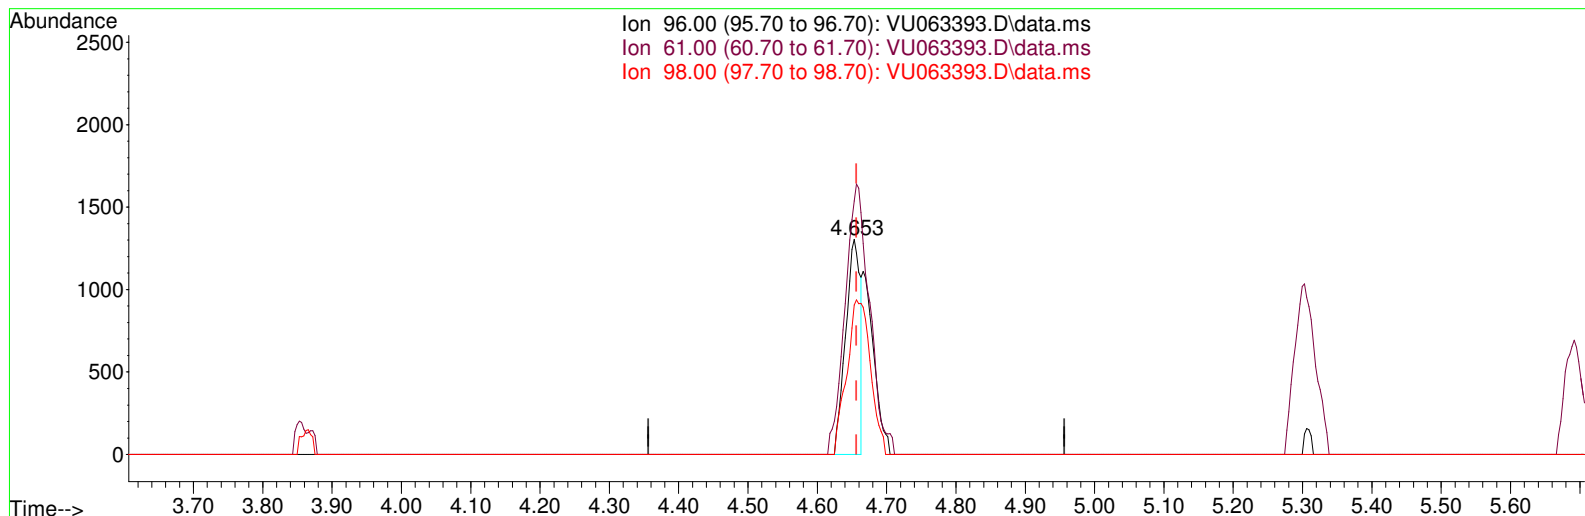

(20) cis-1,2-Dichloroethene (T)

4.653min (-0.003) 1.51 ug/L

response 1913

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	130.80	117.87
98.00	62.90	69.56
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061225\
Data File : VU063393.D
Acq On : 12 Jun 2025 11:43
Operator : MD/SY
Sample : Q2117-02
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/17/2025
Supervised By :Mahesh Dadoda 06/17/2025

Quant Time: Jun 16 08:40:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jun 16 08:39:07 2025
Response via : Initial Calibration

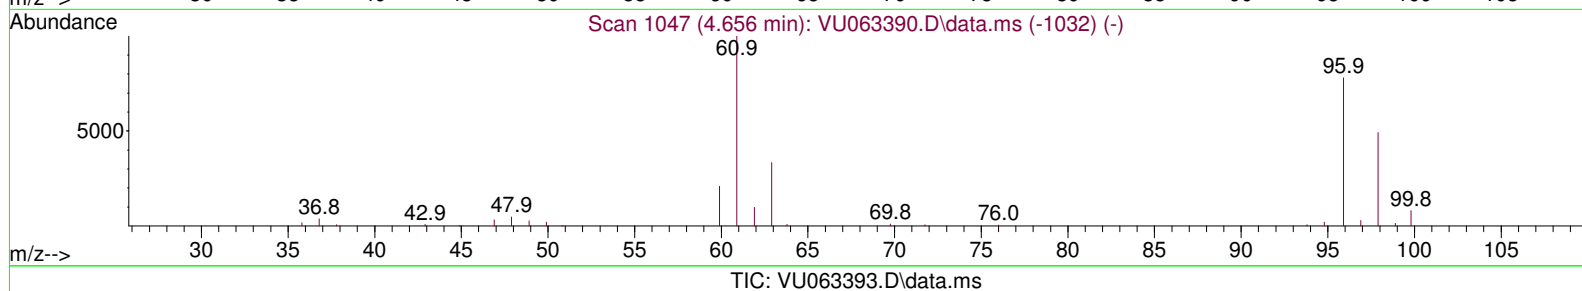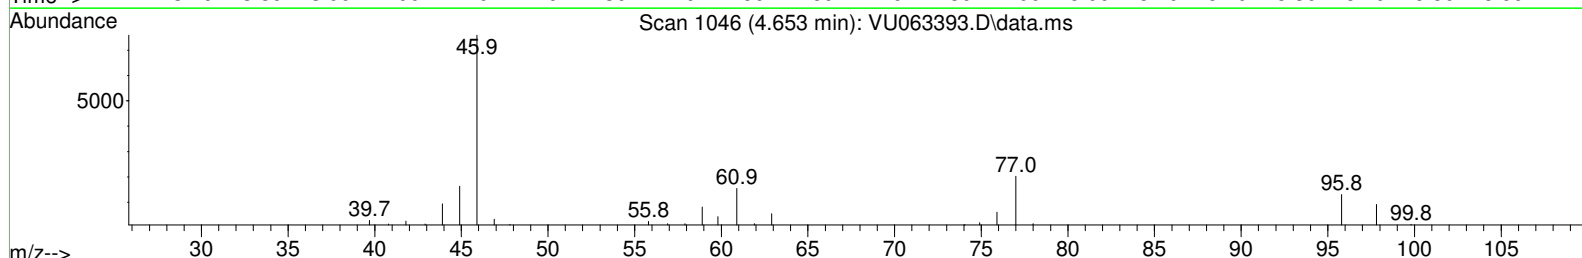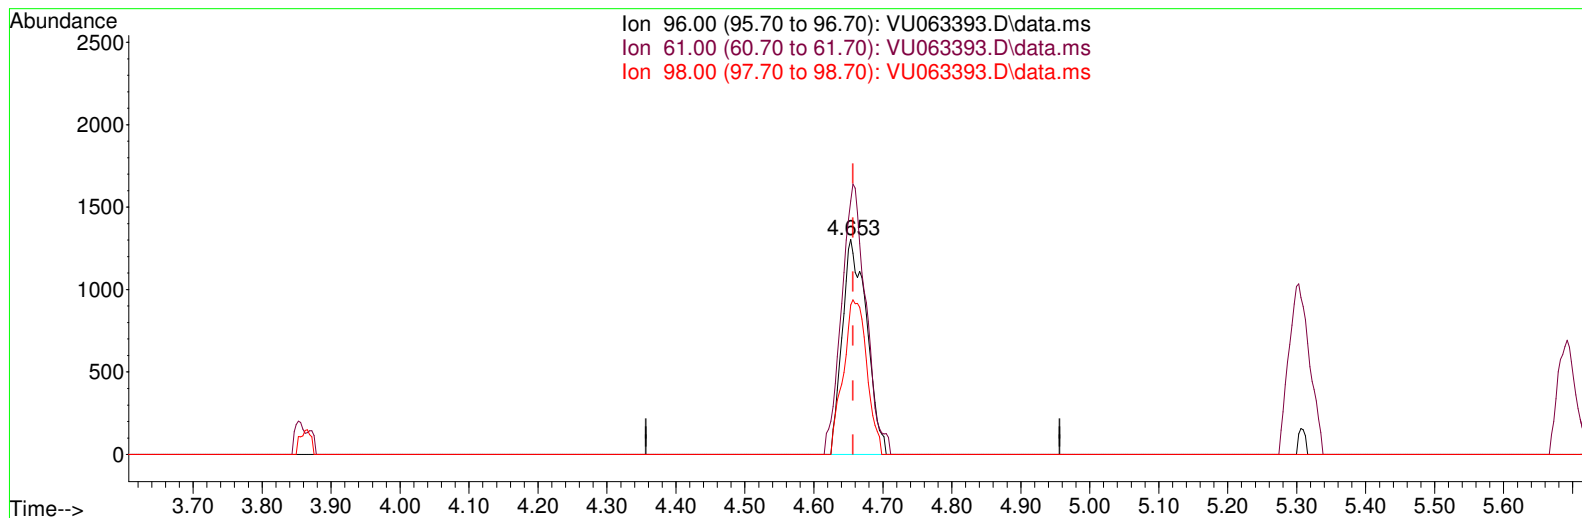

(20) cis-1,2-Dichloroethene (T)

4.653min (-0.003) 2.52 ug/L m

response 3195

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	130.80	117.87
98.00	62.90	69.56
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061225\
Data File : VU063393.D
Acq On : 12 Jun 2025 11:43
Operator : MD/SY
Sample : Q2117-02
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/17/2025
Supervised By :Mahesh Dadoda 06/17/2025

Quant Time: Jun 16 08:40:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jun 16 08:39:07 2025
Response via : Initial Calibration

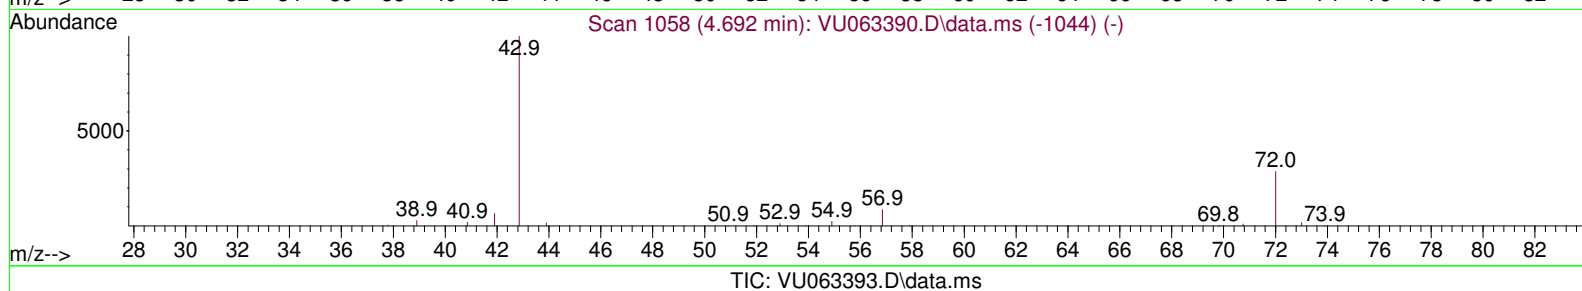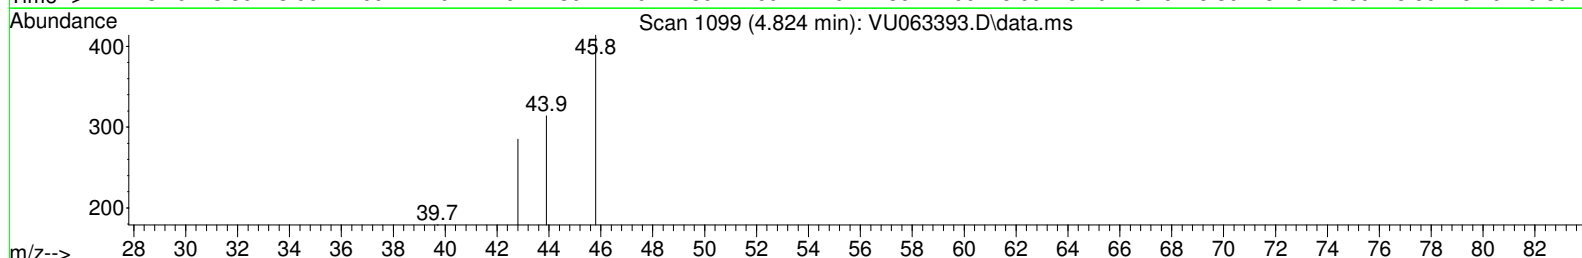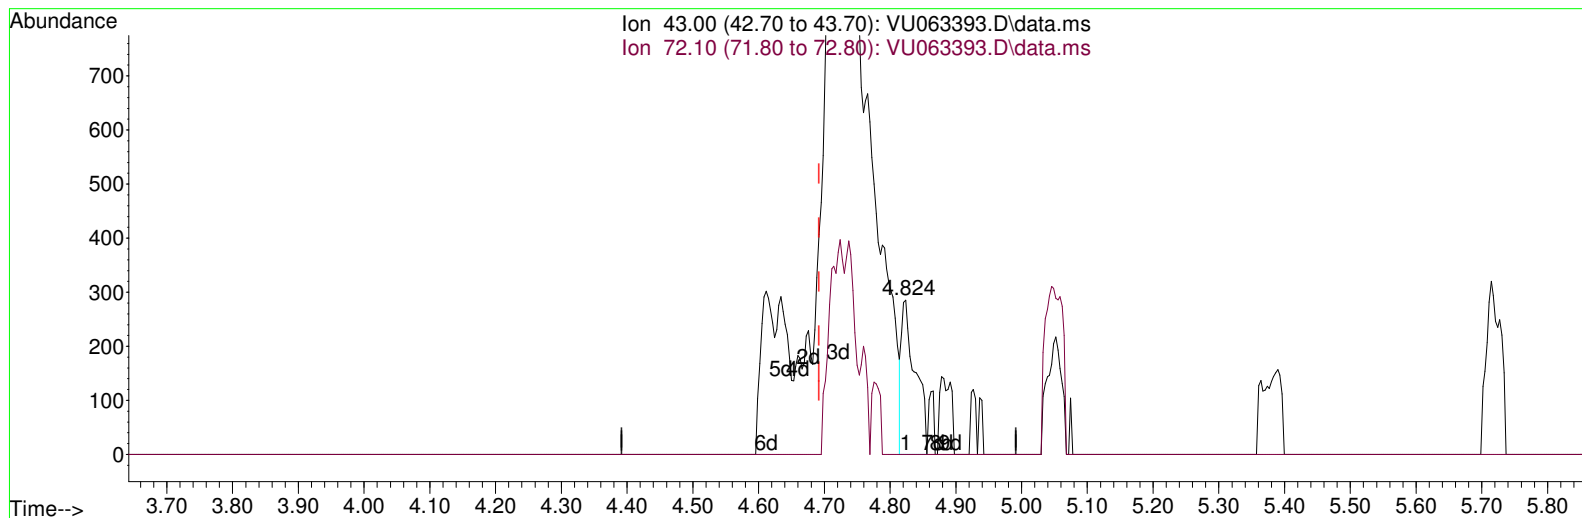

(22) 2-Butanone (T)

4.824min (+ 0.132) 0.41 ug/L

response 421

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	30.90	27.79
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061225\
Data File : VU063393.D
Acq On : 12 Jun 2025 11:43
Operator : MD/SY
Sample : Q2117-02
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/17/2025
Supervised By :Mahesh Dadoda 06/17/2025

Quant Time: Jun 16 08:40:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jun 16 08:39:07 2025
Response via : Initial Calibration

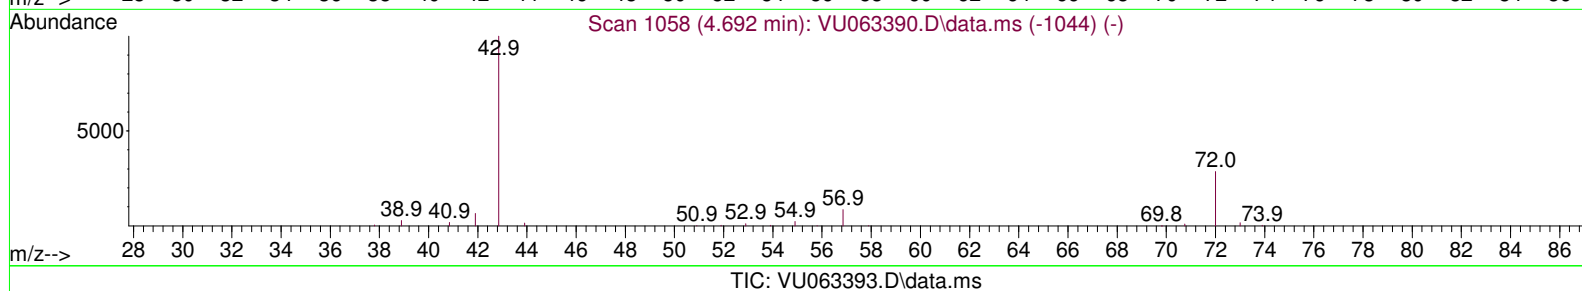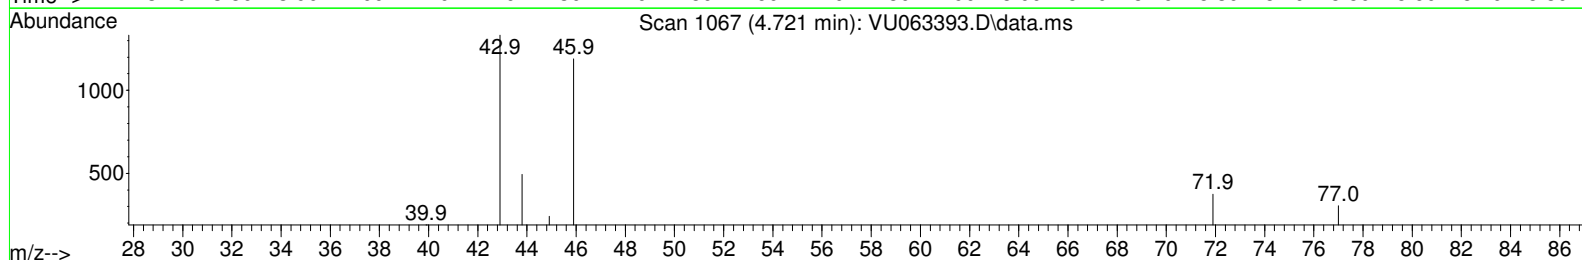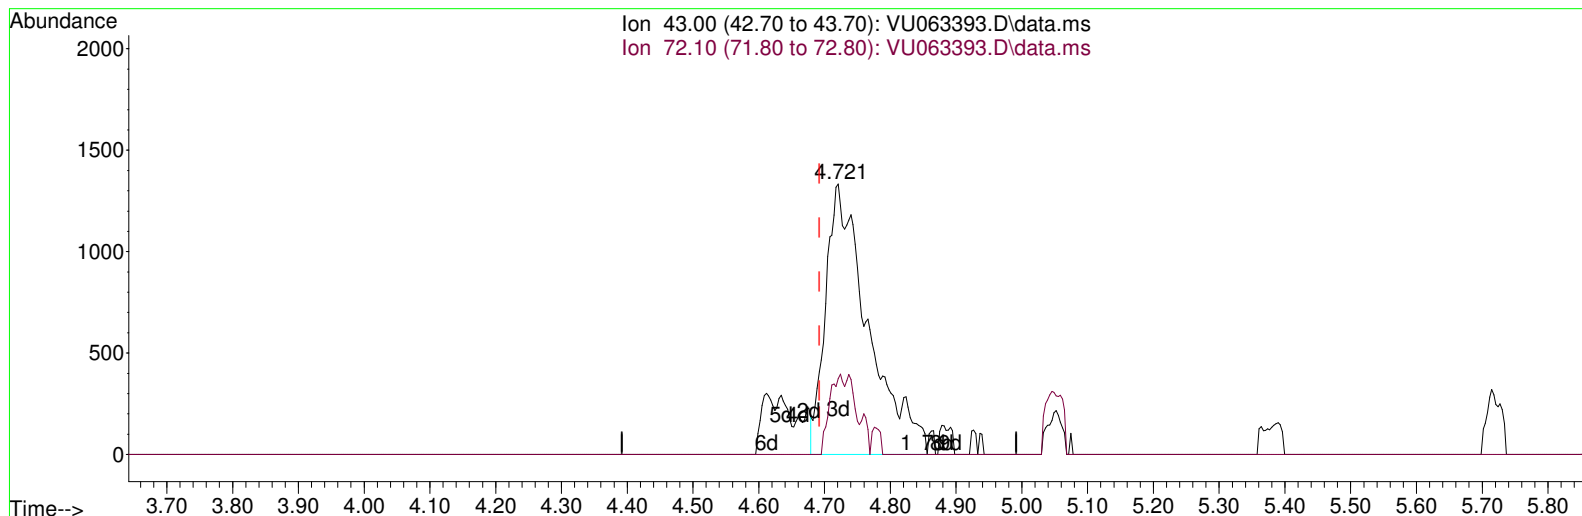

(22) 2-Butanone (T)

4.721min (+ 0.029) 5.86 ug/L m

response 5984

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	30.90	1.96#
0.00	0.00	0.00
0.00	0.00	0.00