
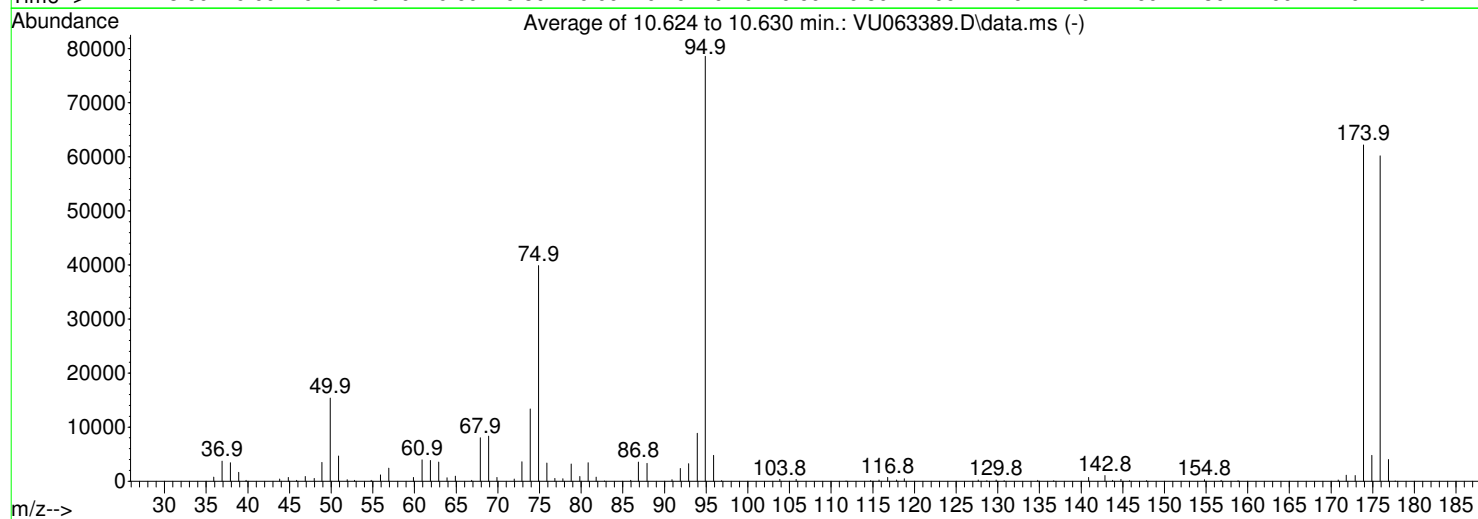


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061225\
Data File : VU063389.D
Acq On : 12 Jun 2025 09:09
Operator : MD/SY
Sample : BFB087
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB087

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Title : VOC Analysis
Last Update : Wed Jun 11 13:45:27 2025

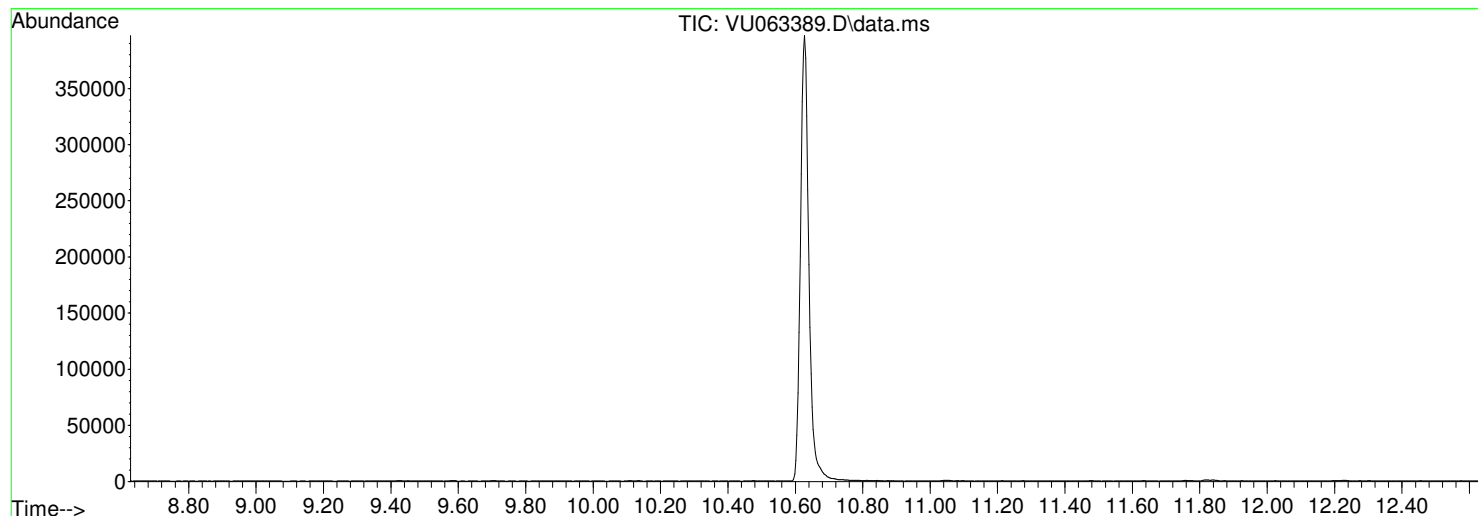

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.5	15358	PASS
75	95	30	80	50.7	39859	PASS
95	95	100	100	100.0	78611	PASS
96	95	5	9	6.1	4768	PASS
173	174	0.00	2	1.7	1062	PASS
174	95	50	120	79.1	62200	PASS
175	174	5	9	7.7	4770	PASS
176	174	95	101	96.8	60187	PASS
177	176	5	9	6.6	3994	PASS

m/z	Abundance
39.80	112.0
43.80	381.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

m/z	Abundance
35.90	861.0
36.90	3669.0
37.90	3508.0
38.90	1539.0
39.80	206.0
43.80	755.0
44.90	747.0
45.80	144.0
46.90	795.0
47.90	452.0
48.90	3519.0
49.90	15261.0
50.90	4734.0
51.90	250.0
52.80	139.0
54.80	183.0
55.90	1224.0
56.90	2411.0
59.80	758.0
60.90	4036.0
61.90	3882.0
62.90	3579.0
63.90	673.0
64.90	948.0
67.90	7913.0
68.90	8440.0
69.90	729.0
72.00	412.0
72.90	3671.0
73.90	13306.0
74.90	40032.0
75.90	3394.0
76.90	612.0
77.80	371.0
78.80	3361.0
79.80	878.0
80.90	3531.0
81.80	653.0
82.80	101.0
85.90	143.0
86.90	3559.0
87.90	3274.0
90.90	237.0
91.90	2332.0
92.90	3292.0
94.00	8908.0
94.90	78952.0
95.90	4781.0
96.80	104.0
103.80	305.0
105.80	360.0
115.80	225.0
116.80	619.0
117.80	258.0
118.80	421.0
127.70	207.0
128.70	131.0
129.80	213.0
134.80	176.0
140.90	697.0
142.80	939.0
143.80	110.0
144.80	368.0
145.80	101.0
148.00	124.0
154.80	299.0
156.80	134.0
170.80	204.0
171.80	938.0
172.90	1023.0
173.90	60440.0
174.90	4596.0
175.90	58896.0
176.90	3976.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

m/z	Abundance
35.90	788.0
36.90	3850.0
37.90	3513.0
38.90	1709.0
39.80	257.0
43.80	782.0
44.90	681.0
45.80	130.0
46.90	828.0
48.00	497.0
48.90	3594.0
49.90	15809.0
50.90	4790.0
51.90	245.0
52.80	142.0
54.80	185.0
55.90	1198.0
56.90	2474.0
59.80	656.0
60.90	3999.0
61.90	3898.0
62.90	3688.0
63.90	675.0
64.90	982.0
66.90	218.0
67.90	8309.0
68.90	8577.0
69.90	725.0
71.90	420.0
72.90	3618.0
73.90	13803.0
74.90	41000.0
75.90	3451.0
76.90	540.0
77.80	440.0
78.80	3282.0
79.90	903.0
80.80	3491.0
81.80	746.0
86.00	196.0
86.90	3577.0
87.90	3381.0
90.90	299.0
91.90	2474.0
92.90	3283.0
93.90	9108.0
94.90	81168.0
95.90	4843.0
96.90	112.0
103.90	351.0
105.80	336.0
111.80	101.0
114.70	117.0
115.80	221.0
116.80	730.0
117.90	217.0
118.80	453.0
127.70	208.0
128.70	112.0
129.80	220.0
130.80	113.0
134.80	170.0
136.70	109.0
140.90	702.0
142.80	1036.0
143.80	165.0
144.80	373.0
145.80	130.0
147.80	110.0
154.80	280.0
156.80	149.0
158.80	101.0
170.80	204.0
171.80	1111.0
172.90	1127.0
173.90	63960.0
174.90	4957.0
175.90	62024.0
176.90	4098.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

m/z	Abundance
35.90	644.0
36.90	3659.0
37.90	3261.0
38.90	1657.0
39.80	265.0
43.80	794.0
44.80	552.0
45.90	145.0
46.90	887.0
48.00	483.0
48.90	3227.0
49.90	15003.0
50.90	4508.0
51.90	225.0
52.80	160.0
54.80	164.0
55.90	1072.0
56.90	2277.0
59.90	626.0
60.90	3764.0
61.90	3717.0
62.90	3387.0
63.90	594.0
64.90	918.0
66.80	223.0
67.90	7930.0
68.90	7869.0
69.90	672.0
71.90	416.0
72.90	3386.0
73.90	12998.0
74.90	38544.0
75.90	3194.0
76.80	440.0
77.80	450.0
78.80	2874.0
79.80	890.0
80.80	3189.0
81.80	750.0
86.00	177.0
86.80	3448.0
87.90	3246.0
90.90	329.0
91.90	2308.0
92.90	3129.0
93.90	8577.0
94.90	75712.0
95.90	4679.0
96.90	115.0
103.90	348.0
105.80	282.0
114.80	110.0
115.70	215.0
116.80	725.0
117.90	212.0
118.80	480.0
127.60	198.0
129.80	207.0
130.70	108.0
134.80	123.0
136.70	104.0
140.90	622.0
142.90	1082.0
143.80	172.0
144.80	320.0
145.80	133.0
147.80	120.0
154.80	199.0
156.80	124.0
158.90	112.0
170.90	175.0
171.80	1229.0
172.90	1036.0
173.90	62200.0
174.90	4756.0
175.90	59640.0
176.90	3908.0
177.70	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087