




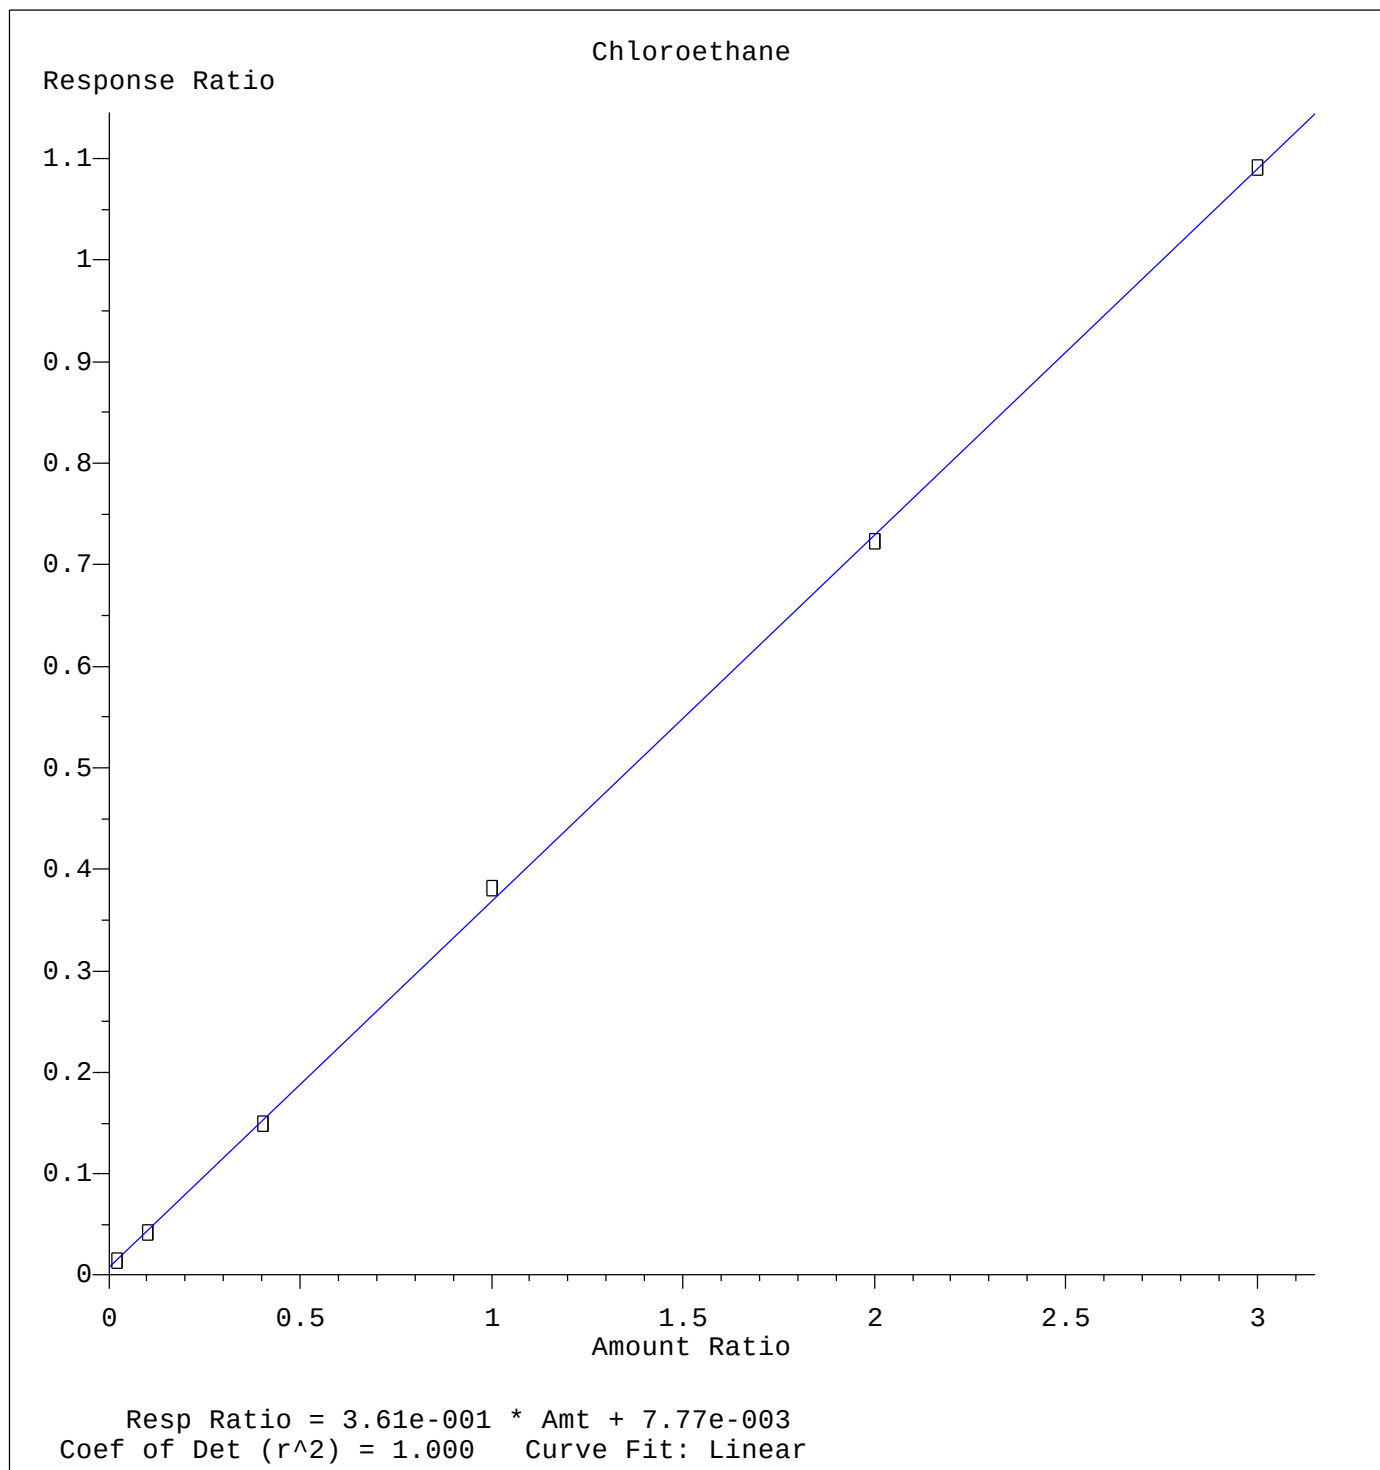


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Calibration Table Last Updated: Wed Jun 13 13:55:26 2018

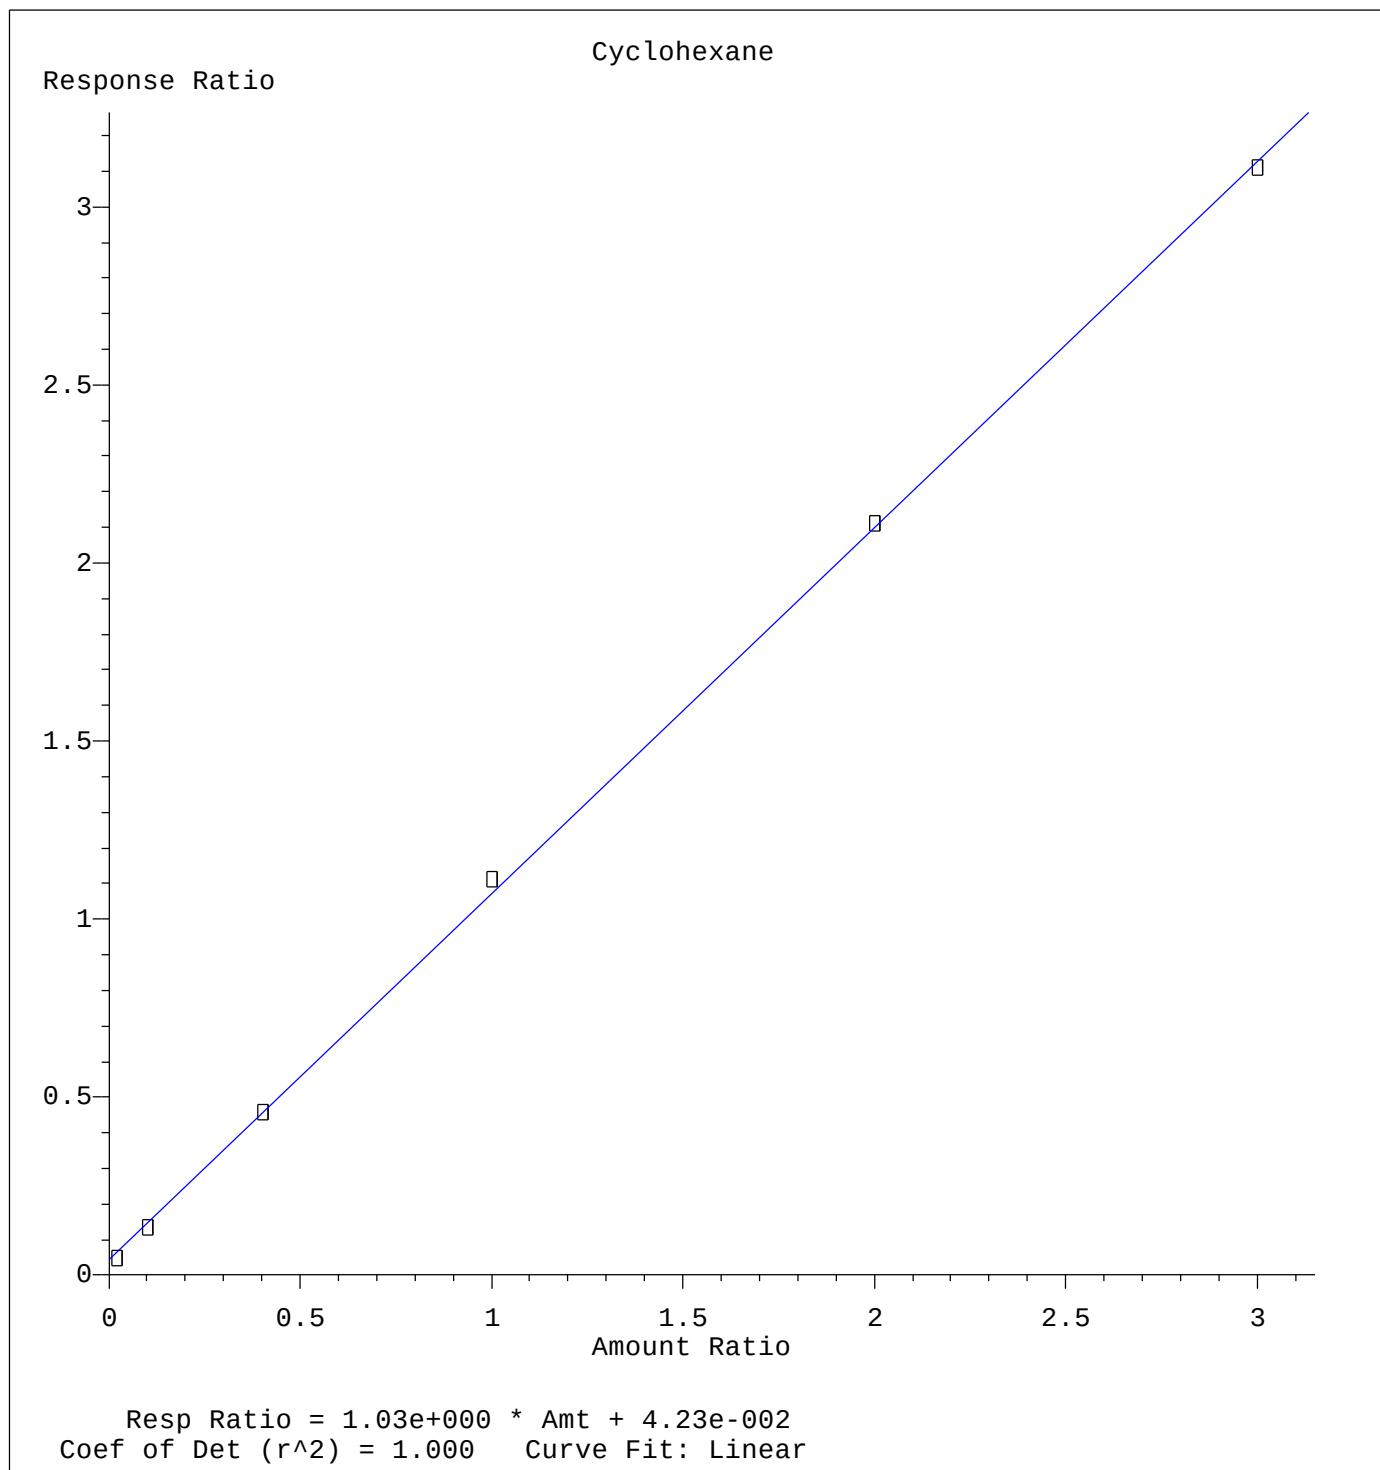

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Calibration Table Last Updated: Wed Jun 13 13:55:26 2018

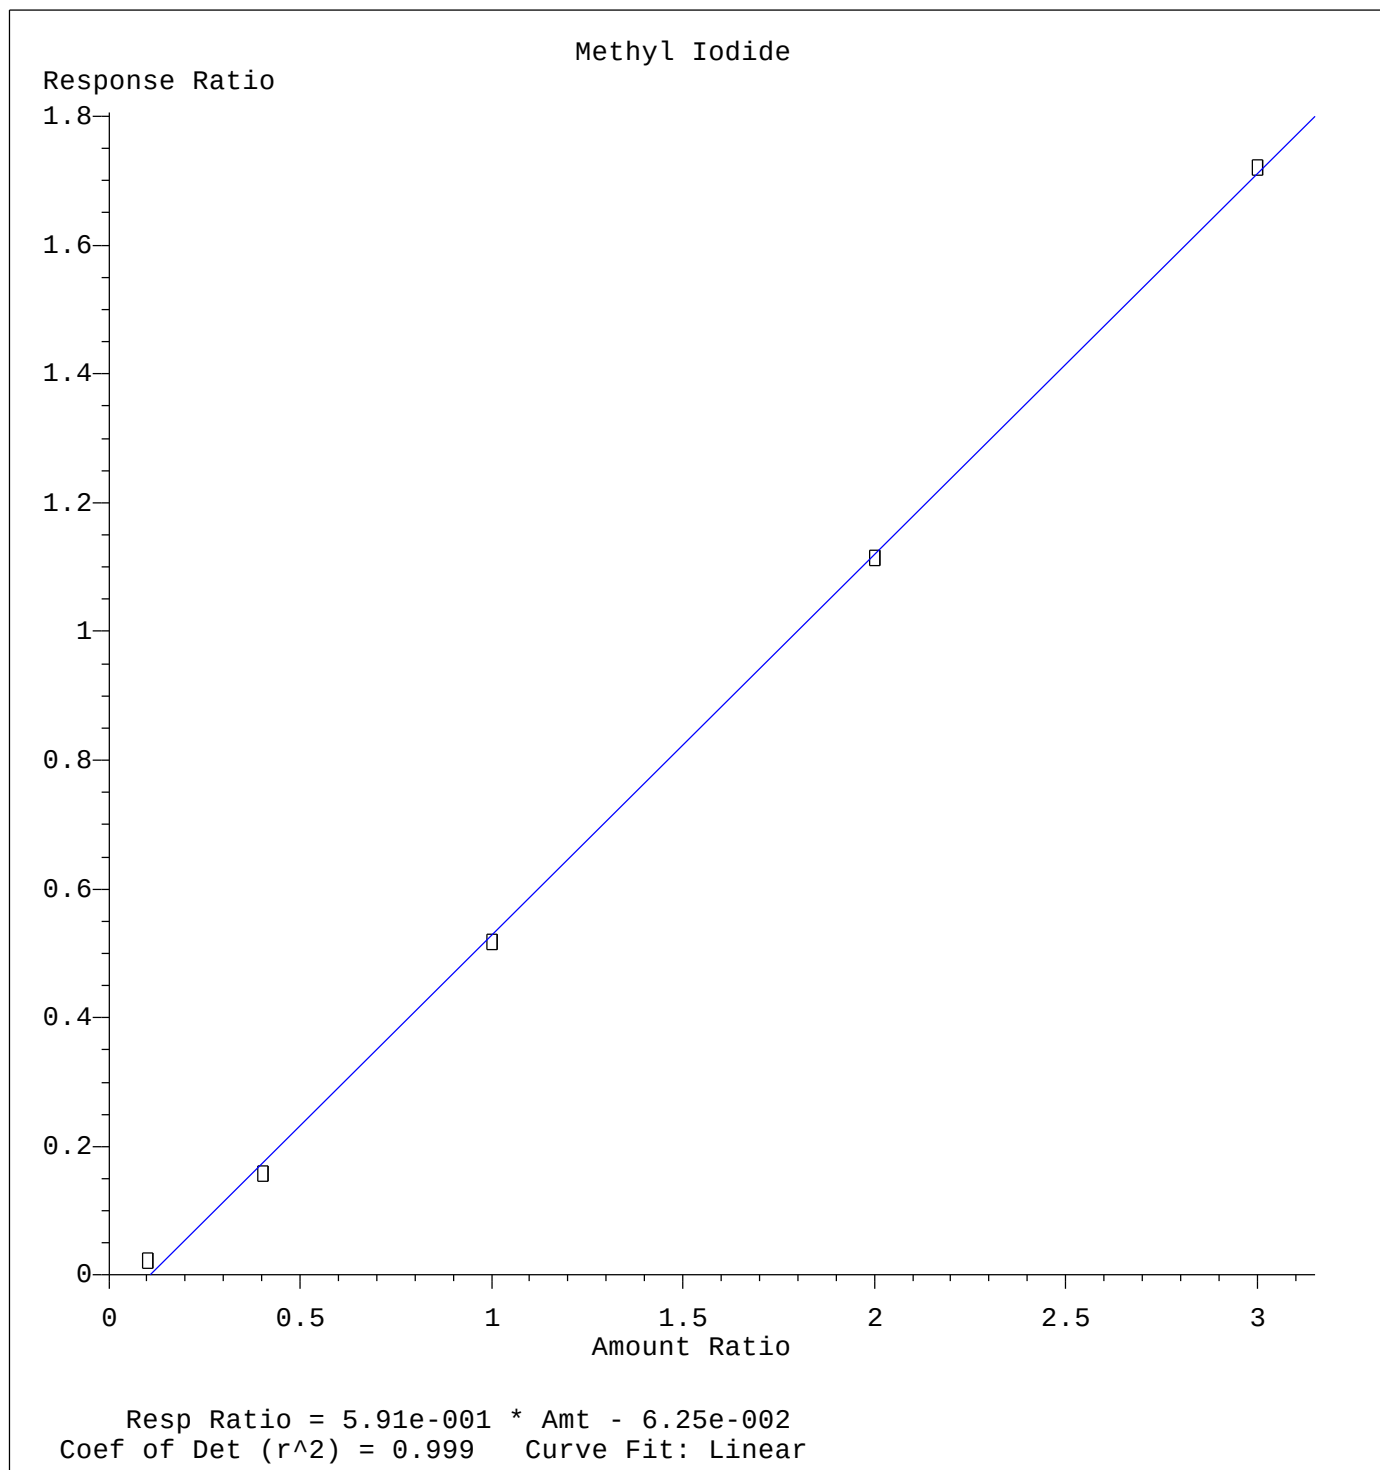


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Calibration Table Last Updated: Wed Jun 13 13:55:26 2018

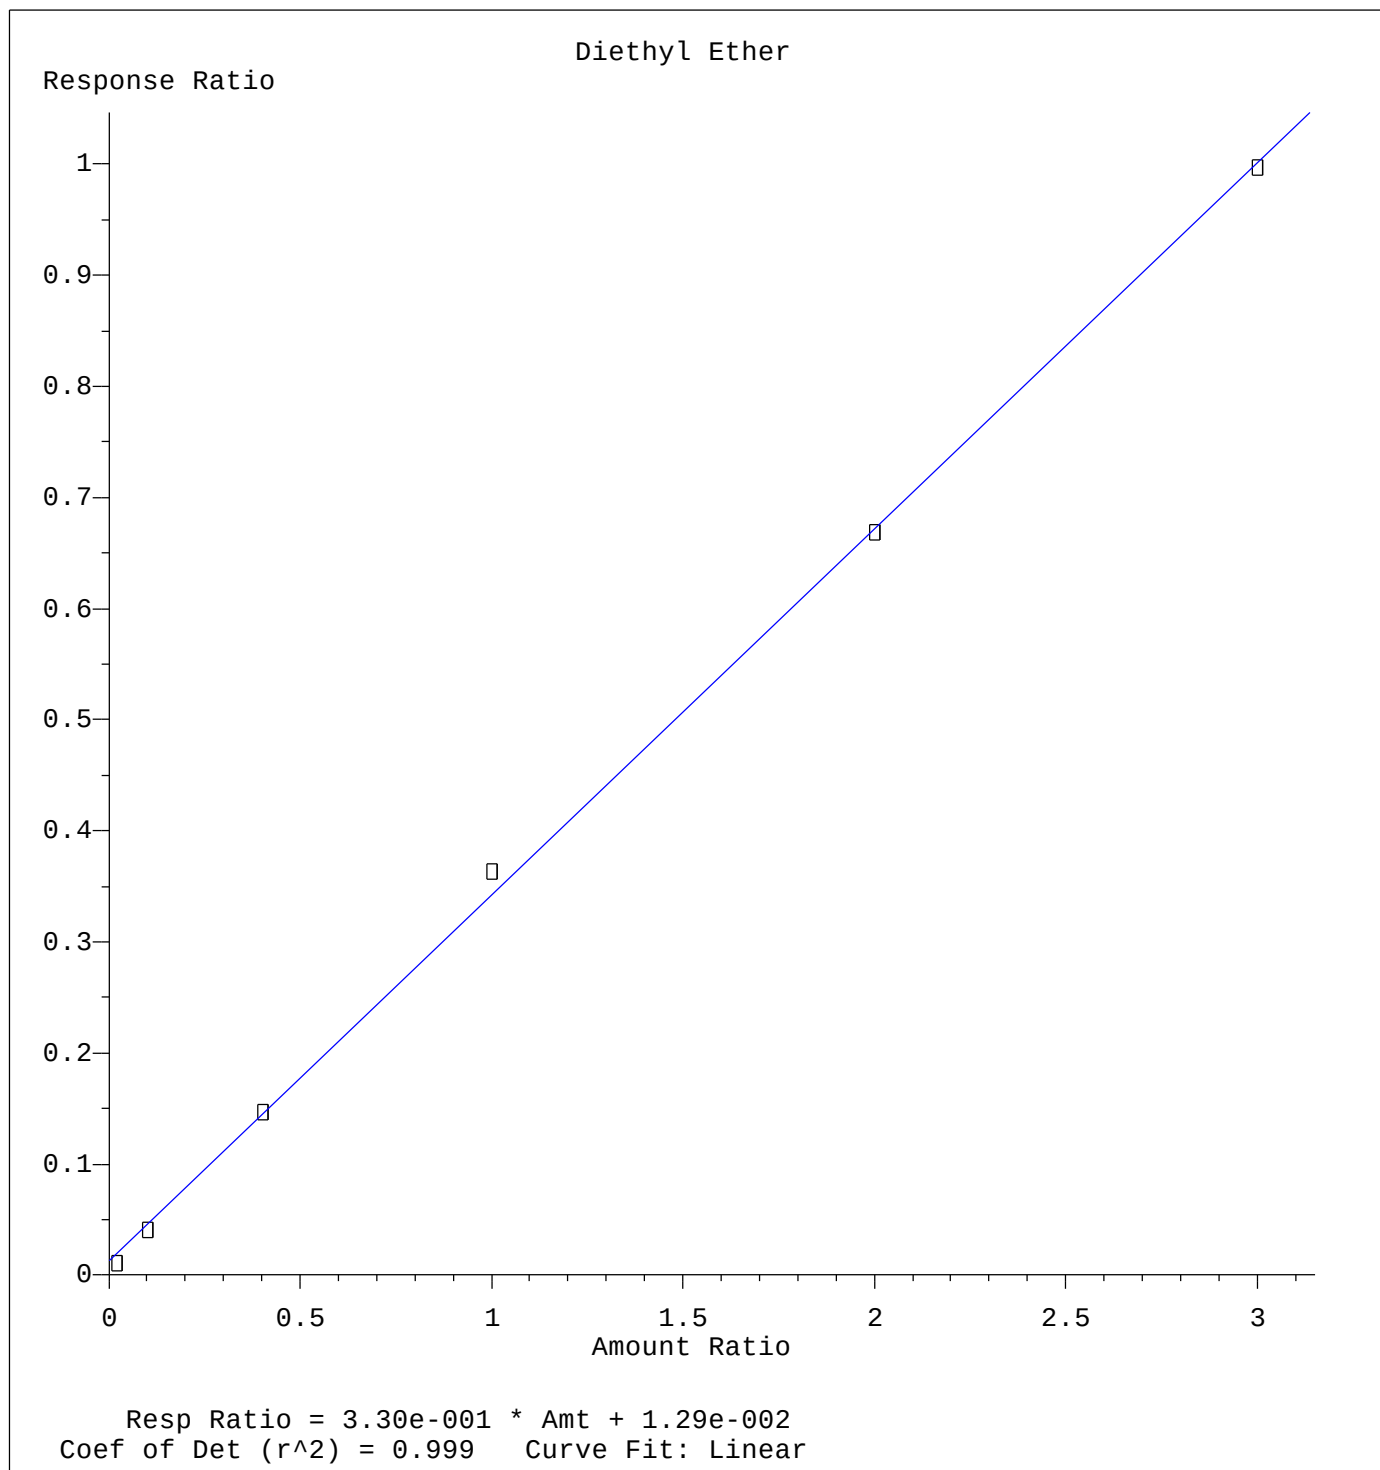

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Calibration Table Last Updated: Wed Jun 13 13:55:26 2018

Naphthalene

Response Ratio

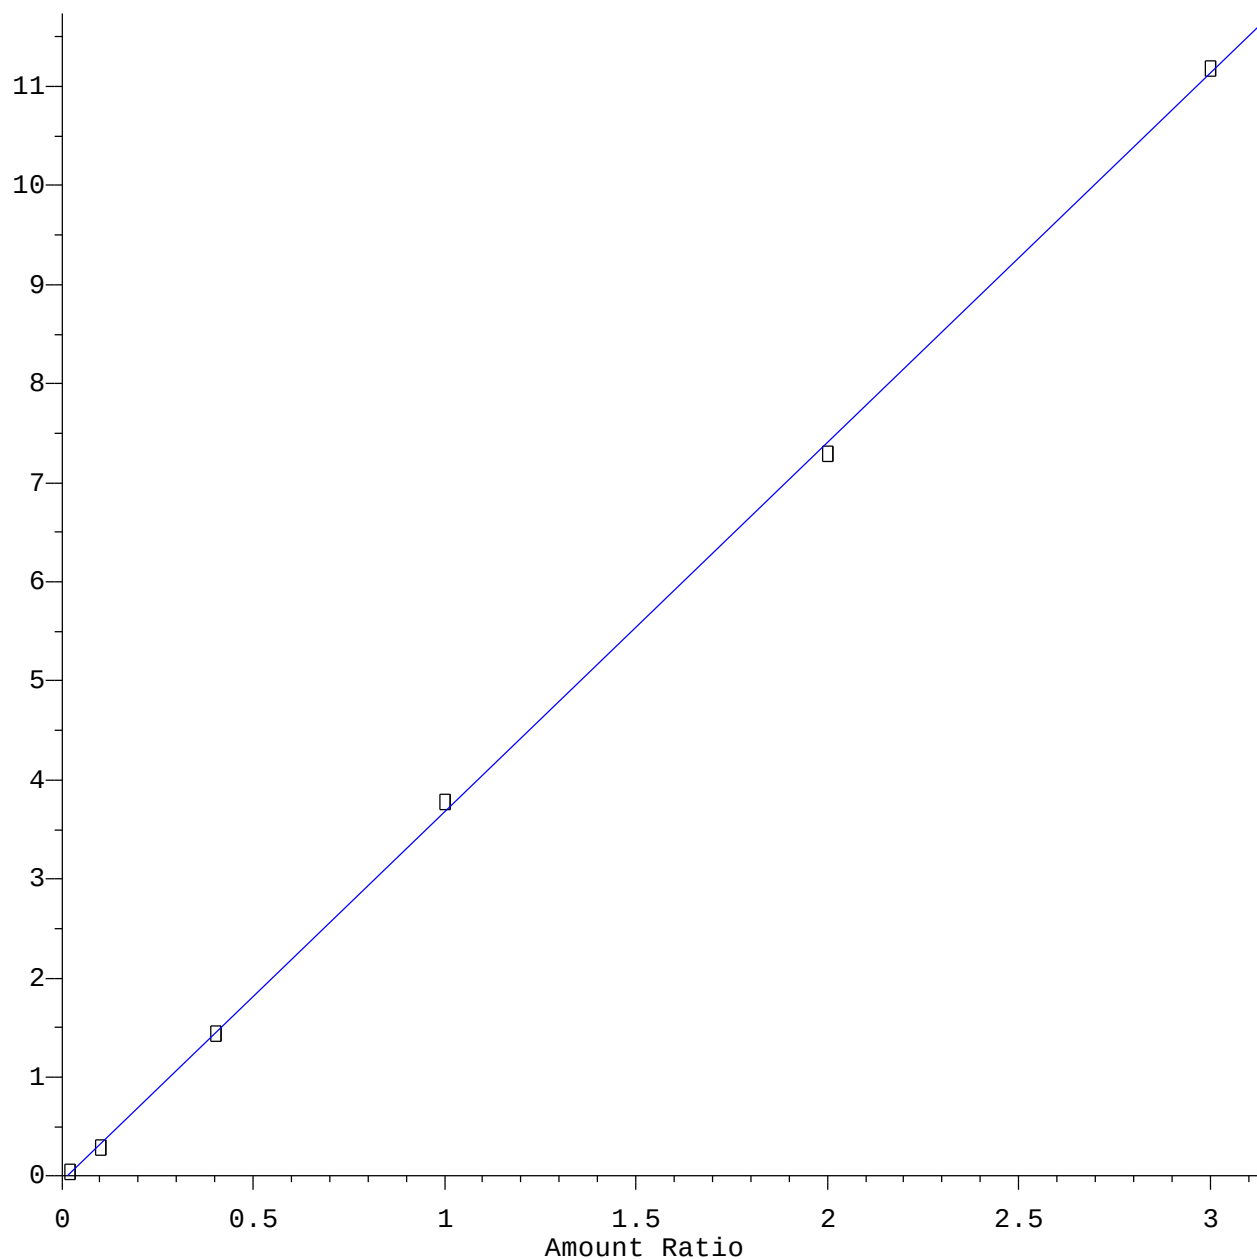

Resp Ratio = 3.73×10^0 * Amt - 5.06×10^{-2}
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Calibration Table Last Updated: Wed Jun 13 13:55:26 2018