


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU061318\
Data File : VU024498.D
Acq On : 13 Jun 2018 10:59
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Title : SW846 8260
Last Update : Wed Jun 13 13:55:26 2018

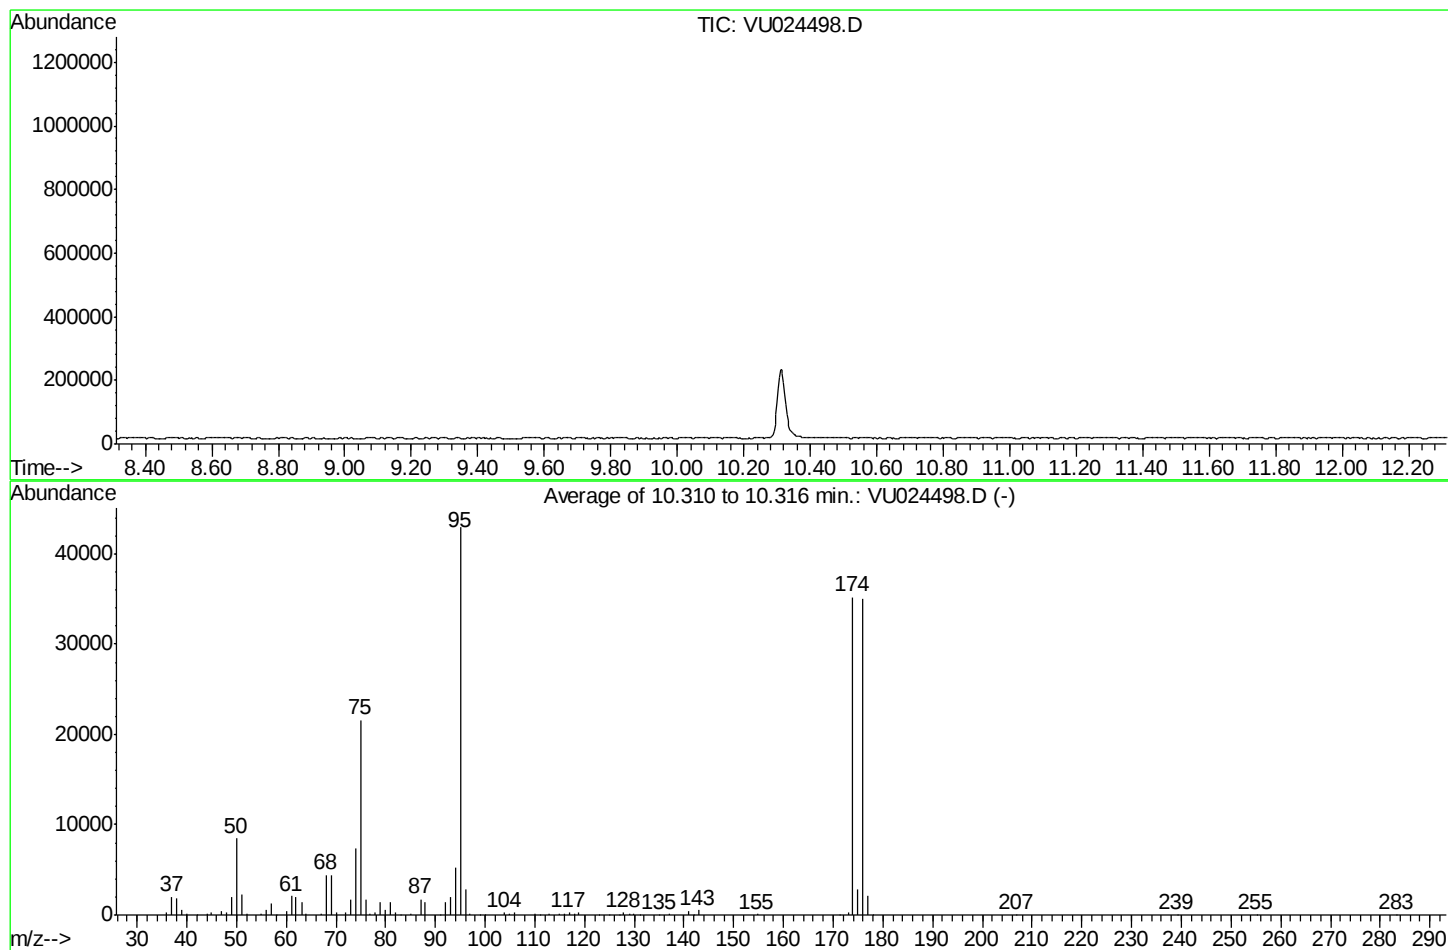

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3006

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	8496	PASS
75	95	30	60	50.2	21565	PASS
95	95	100	100	100.0	42933	PASS
96	95	5	9	6.6	2849	PASS
173	174	0.00	2	1.0	353	PASS
174	95	50	100	82.0	35224	PASS
175	174	5	9	8.0	2817	PASS
176	174	95	101	99.3	34984	PASS
177	176	5	9	6.2	2174	PASS