


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU061319\
Data File : VU032678.D
Acq On : 13 Jun 2019 08:22
Operator : JC/SP
Sample : BFB55
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB55

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Title : VOC Analysis
Last Update : Fri Jun 14 01:25:52 2019

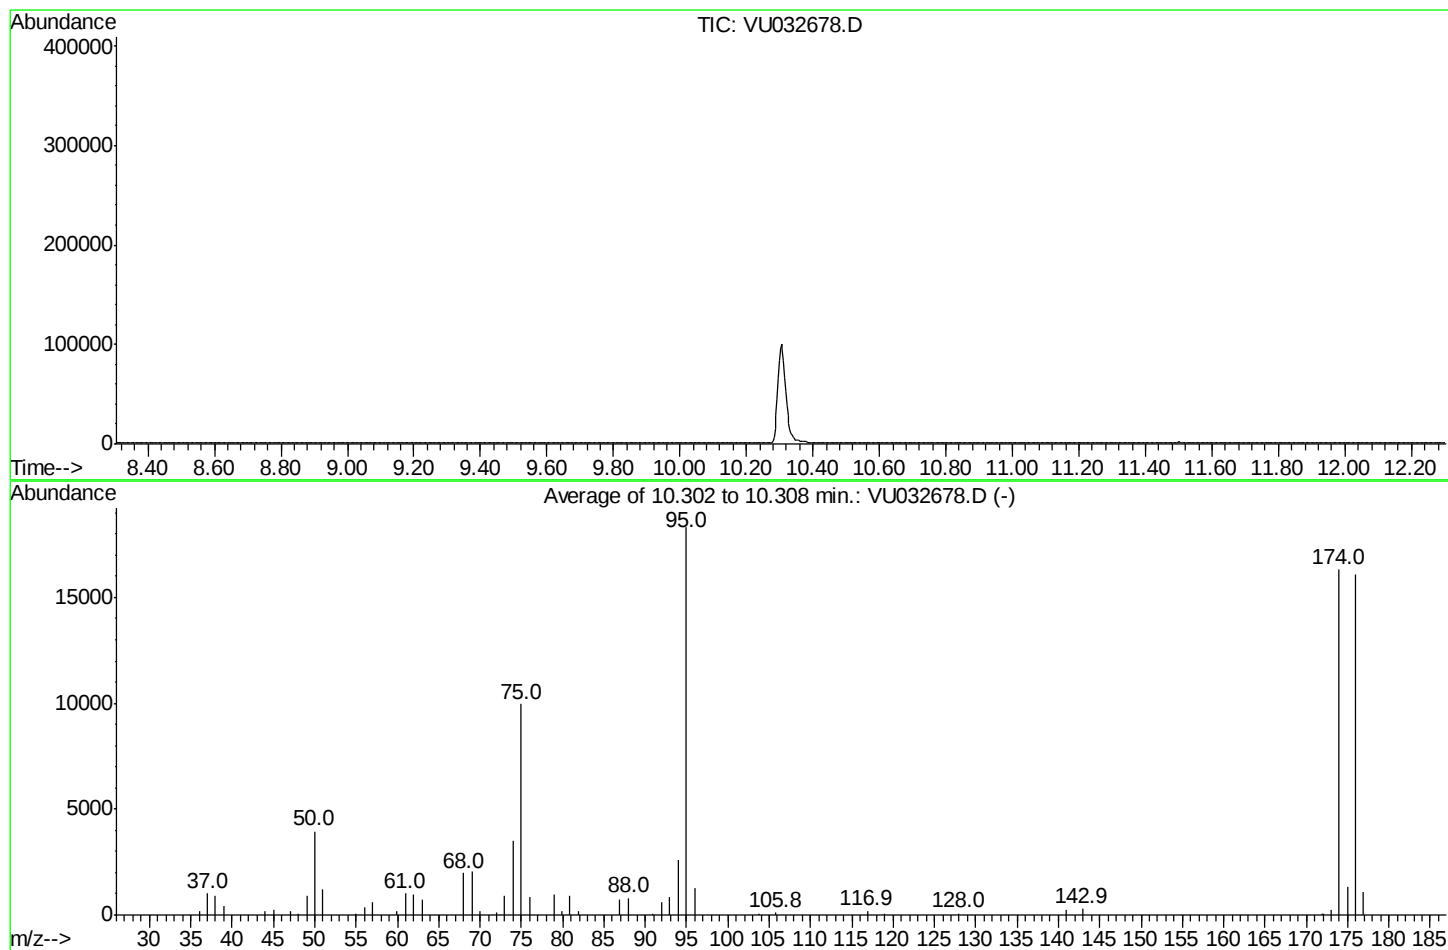

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2855

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	3942	PASS
75	95	30	80	54.3	9950	PASS
95	95	100	100	100.0	18312	PASS
96	95	5	9	6.8	1249	PASS
173	174	0.00	2	1.5	238	PASS
174	95	50	120	89.0	16302	PASS
175	174	5	9	8.0	1311	PASS
176	174	95	101	98.5	16058	PASS
177	176	5	9	7.0	1118	PASS

Scan 2855 (10.270 min): VU032678.D
BFB55

m/z	Abundance
39.90	665.0
43.90	262.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
36.00	205.0
37.00	1052.0
38.00	905.0
38.90	464.0
40.00	623.0
43.90	475.0
45.00	187.0
47.10	211.0
47.90	117.0
49.00	877.0
50.00	4012.0
51.00	1232.0
55.00	111.0
56.00	427.0
57.00	615.0
59.90	205.0
61.00	962.0
62.00	927.0
63.00	677.0
68.00	2054.0
69.00	2052.0
70.10	152.0
72.00	160.0
73.00	892.0
74.00	3477.0
75.00	9840.0
76.00	918.0
78.90	924.0
79.80	208.0
80.90	862.0
81.90	158.0
86.90	736.0
88.00	838.0
91.90	559.0
92.90	891.0
94.00	2534.0
95.00	18456.0
96.00	1272.0
103.80	145.0
105.80	114.0
116.90	152.0
140.90	272.0
142.90	275.0
171.90	114.0
173.00	238.0
174.00	15735.0
175.00	1265.0
176.00	15952.0
177.00	1016.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
36.00	195.0
37.00	1023.0
38.00	921.0
38.90	433.0
40.00	648.0
43.90	481.0
45.00	227.0
47.00	211.0
48.00	100.0
49.00	926.0
50.00	4066.0
51.00	1254.0
56.00	398.0
57.00	635.0
60.00	201.0
61.00	1008.0
62.00	982.0
63.00	713.0
68.00	2019.0
69.00	2104.0
70.00	174.0
72.00	138.0
73.00	940.0
74.00	3594.0
75.00	10306.0
76.00	864.0
78.90	985.0
79.90	202.0
80.90	936.0
81.80	193.0
86.90	765.0
88.00	819.0
92.00	588.0
92.90	891.0
94.00	2692.0
95.00	18864.0
96.00	1287.0
103.80	109.0
105.80	120.0
116.90	205.0
118.90	121.0
128.00	109.0
140.90	274.0
142.90	306.0
172.10	124.0
173.00	250.0
174.00	16832.0
175.00	1350.0
176.00	16520.0
177.00	1162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
36.00	187.0
37.00	992.0
38.00	872.0
39.00	372.0
39.90	676.0
43.90	449.0
45.00	236.0
47.00	204.0
49.00	914.0
50.00	3748.0
51.00	1185.0
56.00	324.0
57.00	608.0
60.00	194.0
61.00	1034.0
62.00	948.0
63.10	721.0
68.00	1867.0
69.00	1963.0
70.00	176.0
72.10	113.0
73.00	880.0
74.00	3396.0
75.00	9705.0
76.00	786.0
78.90	917.0
79.90	182.0
80.80	882.0
81.80	214.0
86.90	681.0
88.00	738.0
90.90	108.0
92.00	616.0
93.00	807.0
94.00	2554.0
95.00	17616.0
96.00	1188.0
105.80	119.0
116.90	203.0
118.90	135.0
128.00	105.0
140.90	239.0
142.90	303.0
172.10	129.0
173.00	227.0
174.00	16339.0
175.00	1320.0
176.00	15702.0
176.90	1177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55