

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061320\
 Data File : VU038878.D
 Acq On : 13 Jun 2020 03:13
 Operator : SY/MD
 Sample : L2985-05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFT73

Quant Time: Jun 13 04:20:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 13 02:52:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	261293	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	267105	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	122344	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	59098	4.15	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.00%
7) Chloroethane-d5	1.93	69	62112	5.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.60%
11) 1,1-Dichloroethene-d2	2.59	63	72765	2.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	45.00%#
20) 2-Butanone-d5	4.68	46	313016	70.03	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	140.06%#
24) Chloroform-d	5.10	84	172902	5.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.60%
26) 1,2-Dichloroethane-d4	5.74	65	107708	6.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	120.80%
32) Benzene-d6	5.76	84	325846	5.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.40%
36) 1,2-Dichloropropane-d6	6.72	67	106757	5.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	114.40%
41) Toluene-d8	7.92	98	260265	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
43) trans-1,3-Dichloropropene-	8.20	79	37283	4.49	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.80%
46) 2-Hexanone-d5	8.65	63	260393	70.67	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	141.34%#
57) 1,1,2,2-Tetrachloroethane-	10.77	84	97398	5.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	119.20%
64) 1,2-Dichlorobenzene-d4	12.20	152	110100	5.53	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.60%

Target Compounds


					Ovalue
2) Dichlorodifluoromethane	1.39	85	9690	0.381 ug/L	98
9) Trichlorofluoromethane	2.16	101	7648	0.231 ug/L	99
17) Methyl tert-butyl Ether	3.40	73	51660	1.096 ug/L	99
18) trans-1,2-Dichloroethene	3.39	96	2021	0.103 ug/L #	78
22) cis-1,2-Dichloroethene	4.71	96	22417	1.095 ug/L	96
34) Trichloroethene	6.57	95	683232	32.417 ug/L	98
47) Tetrachloroethene	8.57	164	141642	8.729 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061320\
Data File : VU038878.D
Acq On : 13 Jun 2020 03:13
Operator : SY/MD
Sample : L2985-05
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT73

Quant Time: Jun 13 04:20:12 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 13 02:52:53 2020
Response via : Initial Calibration

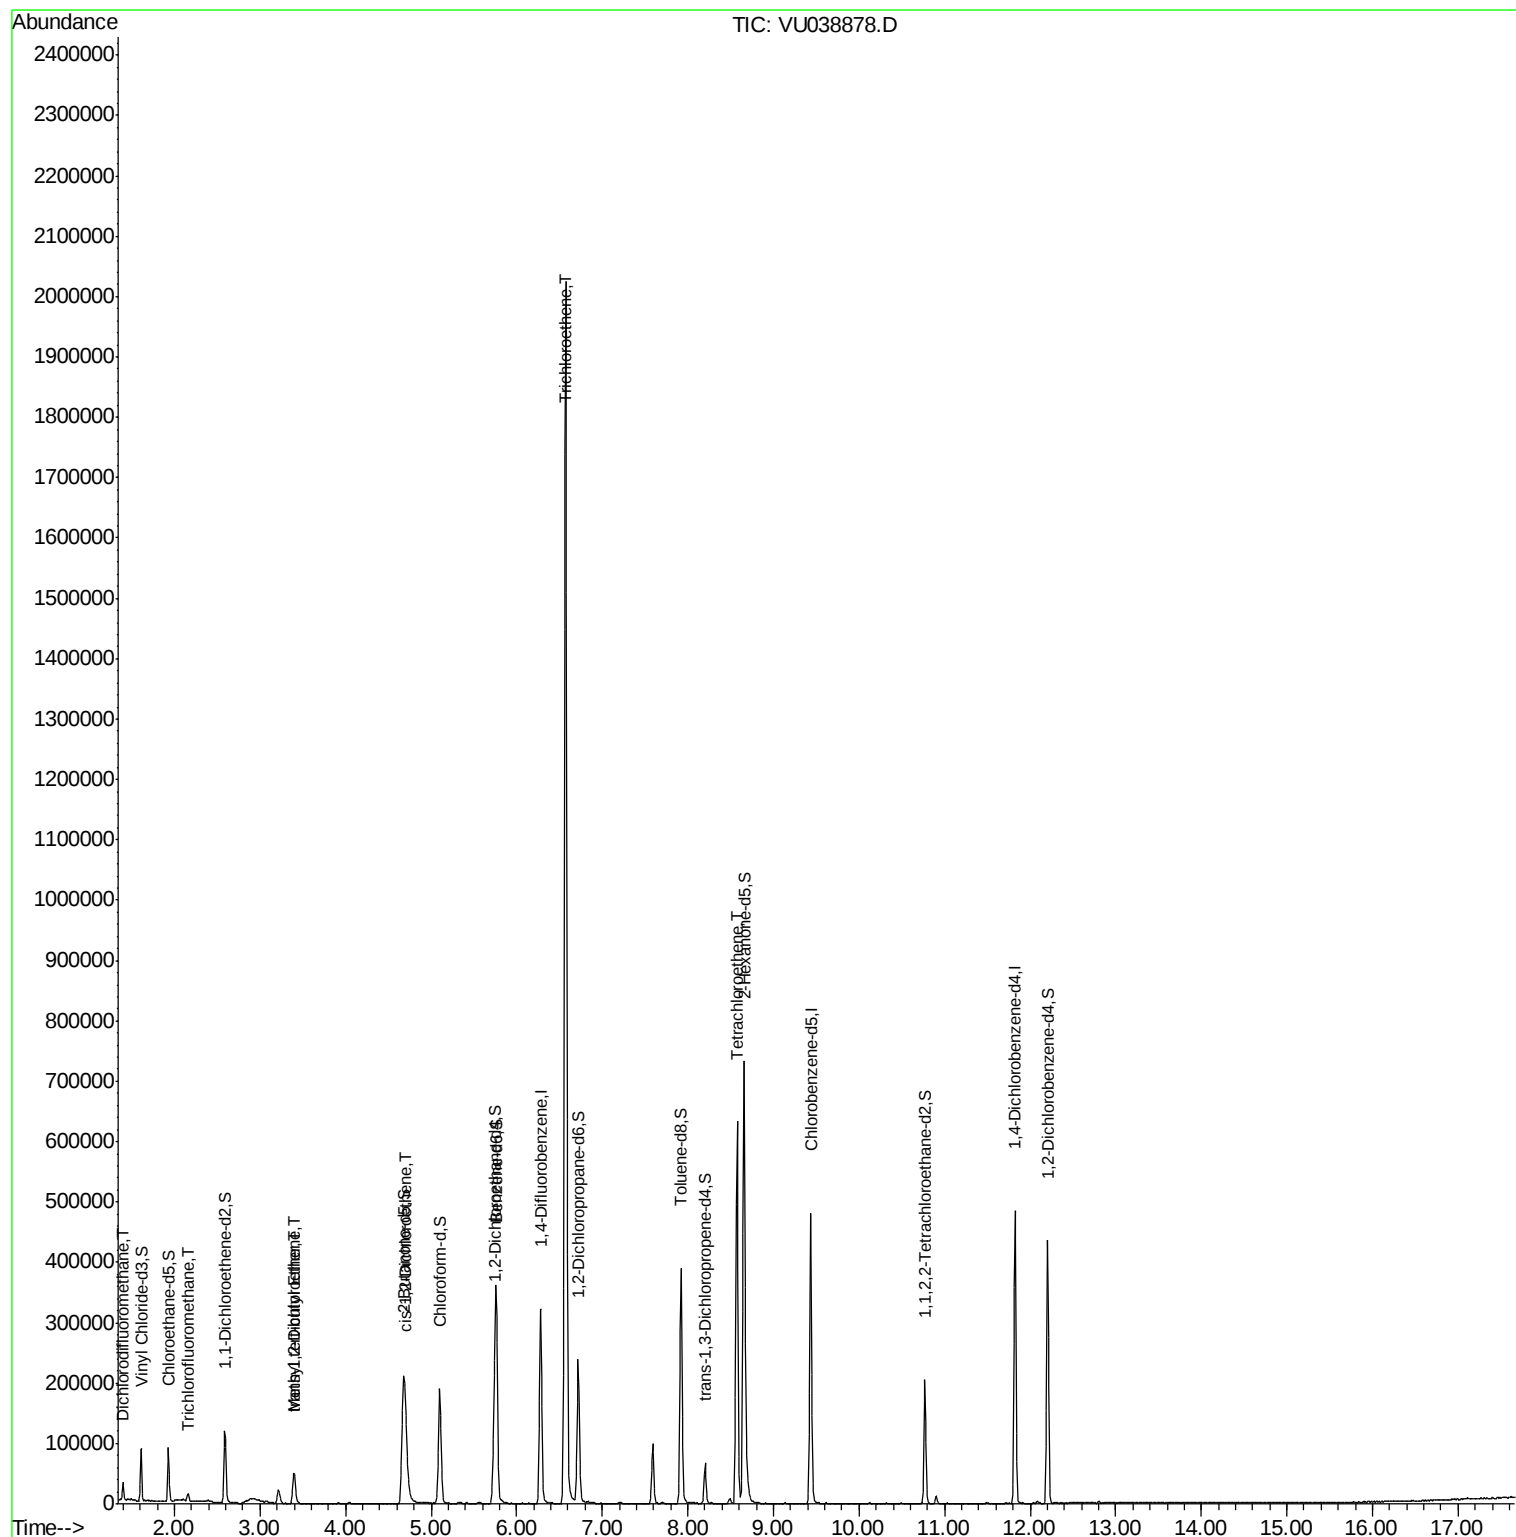

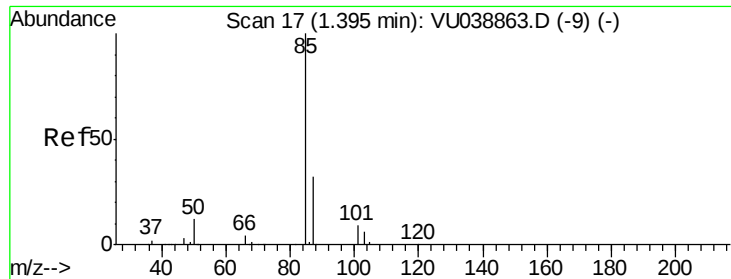

#2

Dichlorodifluoromethane

Concen: 0.381 ug/L

RT: 1.39 min Scan# 17

Delta R.T. -0.00 min

Lab File: VU038878.D

Acq: 13 Jun 2020 03:13

Instrument :

MSVOA_U

ClientSampleId :


BFT73

Tot Ion: 85 Resp: 9690

Ion Ratio Lower Upper

85 100

87 31.3 25.9 38.9

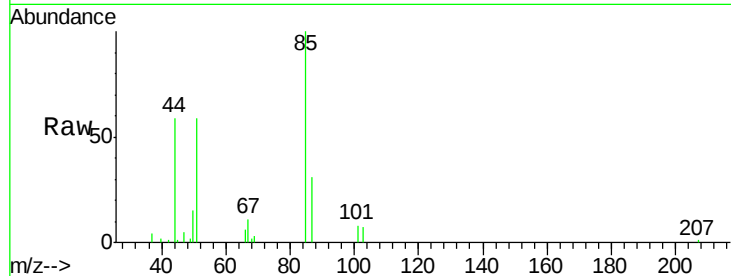


Abundance Ion 85.00 (84.70 to 85.70): VU038863.D (-9) (-)

Ion 87.00 (86.70 to 87.70): VU038863.D (-9) (-)

1.39

Time-->

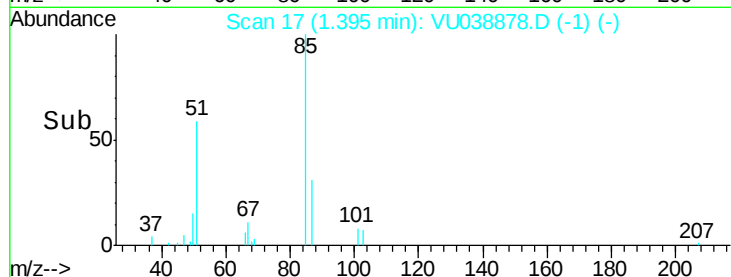


Abundance

Ion 85.00 (84.70 to 85.70): VU038878.D (-1) (-)

Ion 87.00 (86.70 to 87.70): VU038878.D (-1) (-)

1.39

Time-->

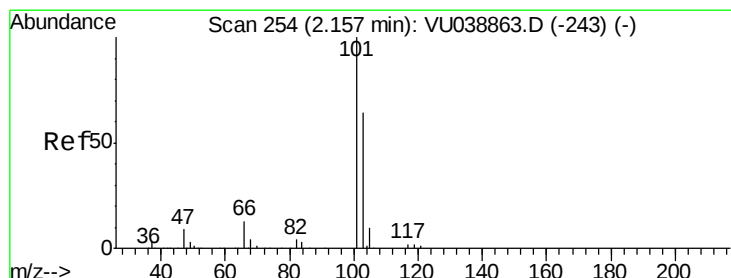

#9

Trichlorofluoromethane

Concen: 0.231 ug/L

RT: 2.16 min Scan# 254

Delta R.T. -0.00 min

Lab File: VU038878.D


Acq: 13 Jun 2020 03:13

Tgt Ion: 101 Resp: 7648

Ion Ratio Lower Upper

101 100

103 63.2 51.5 77.3

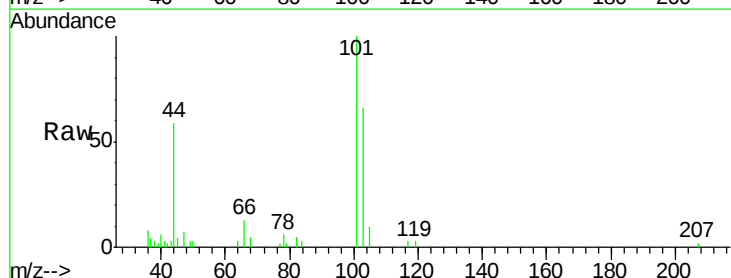


Abundance Ion 101.00 (100.70 to 101.70): VU038863.D (-243) (-)

Ion 103.00 (102.70 to 103.70): VU038863.D (-243) (-)

2.16

Time-->

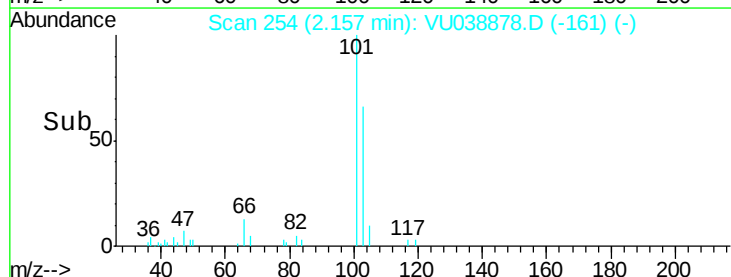


Abundance

Ion 101.00 (100.70 to 101.70): VU038878.D (-161) (-)

Ion 103.00 (102.70 to 103.70): VU038878.D (-161) (-)

2.16


Time-->

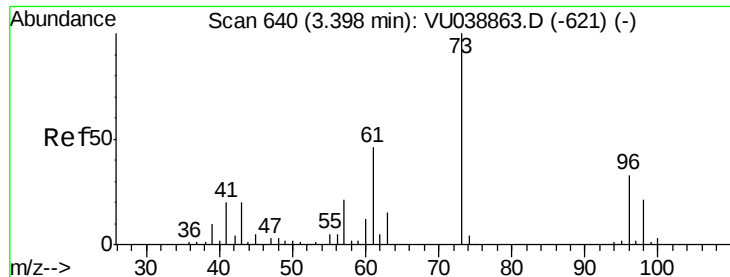




#17
Methvl tert-butvl Ether
Concen: 1.096 ug/L
RT: 3.40 min Scan# 641
Delta R.T. 0.00 min
Lab File: VU038878.D
Acq: 13 Jun 2020 03:13

Instrument :
MSVOA_U
ClientSampleId :
BFT73

Tot Ion: 73 Resp: 51660
Ion Ratio Lower Upper
73 100
43 20.5 15.9 23.9
57 22.6 17.5 26.3

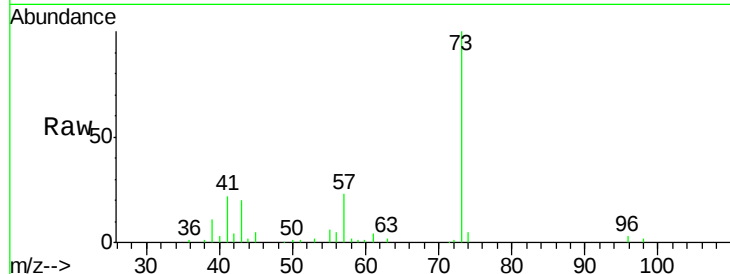


Abundance Ion 73.10 (72.80 to 73.80): VU0
Ion 43.05 (42.75 to 43.75): VU0
Ion 57.10 (56.80 to 57.80): VU0

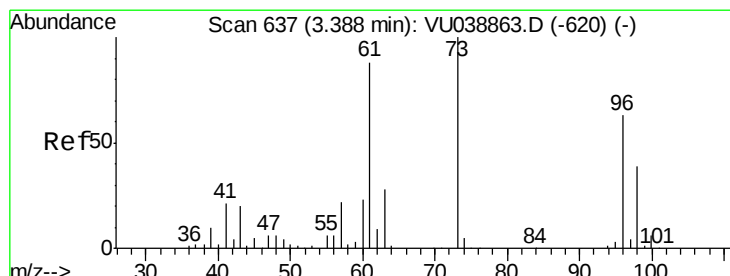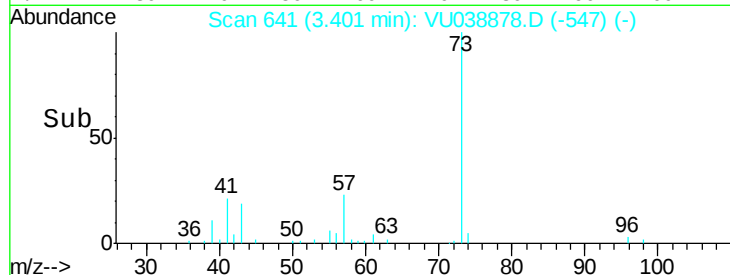
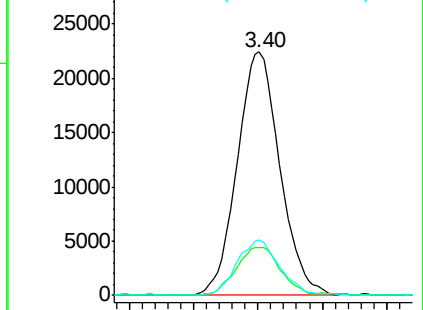



#18
trans-1,2-Dichloroethene
Concen: 0.103 ug/L
RT: 3.39 min Scan# 637
Delta R.T. -0.00 min
Lab File: VU038878.D
Acq: 13 Jun 2020 03:13

Tgt Ion: 96 Resp: 2021
Ion Ratio Lower Upper
96 100
61 165.1 99.3 184.5
98 85.7 43.9 81.5#

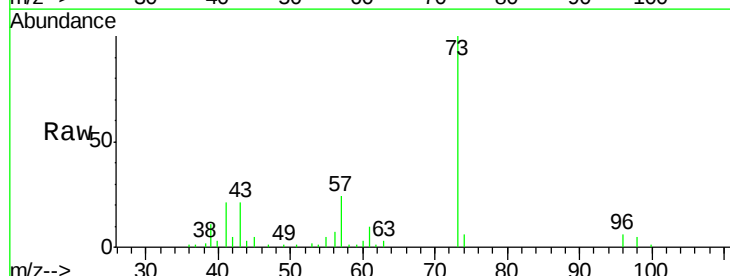

Abundance Ion 96.00 (95.70 to 96.70): VU0
Ion 61.05 (60.75 to 61.75): VU0
Ion 97.95 (97.65 to 98.65): VU0

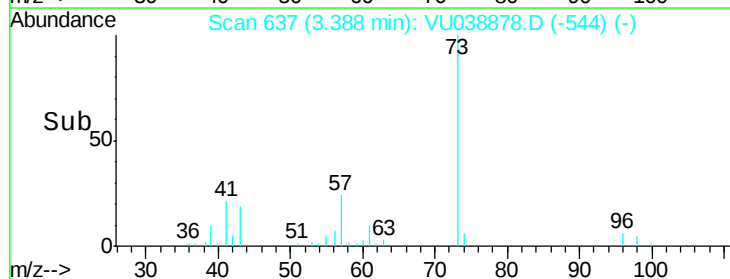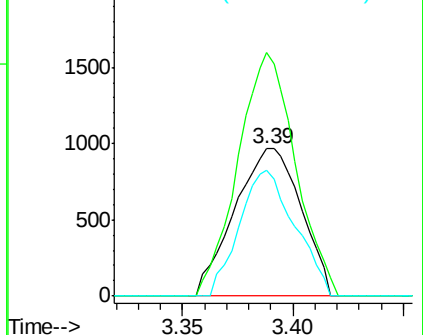

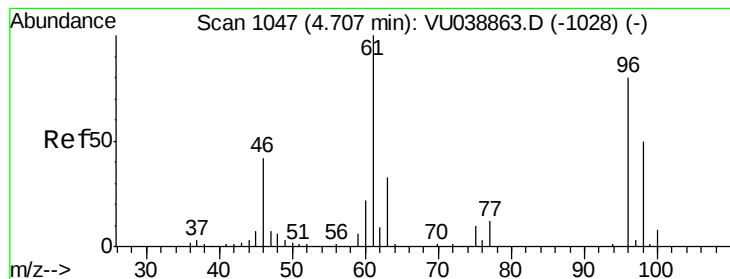

#22

cis-1,2-Dichloroethene

Concen: 1.095 ug/L

RT: 4.71 min Scan# 1047

Delta R.T. -0.00 min

Lab File: VU038878.D

Acq: 13 Jun 2020 03:13

Instrument :

MSVOA_U

ClientSampleId :

BFT73


Tot Ion: 96 Resp: 22417

Ion Ratio Lower Upper

96 100

61 133.3 89.7 166.7




68 0.0 0.0 0.0

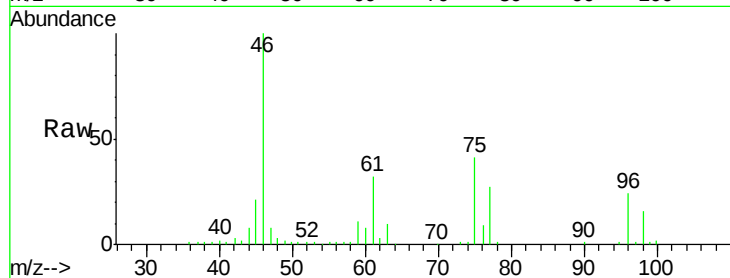

Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.05 (60.75 to 61.75): VU0

Ion 68.15 (67.85 to 68.85): VU0

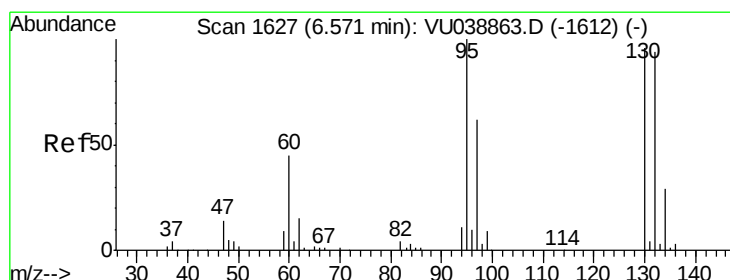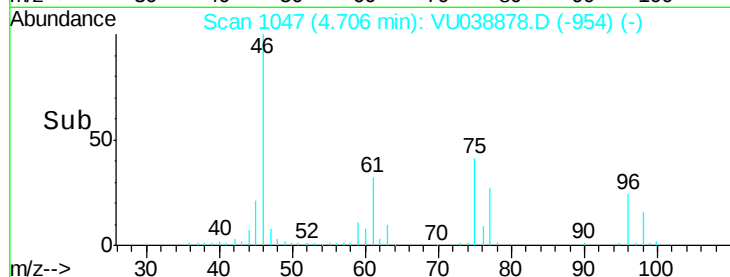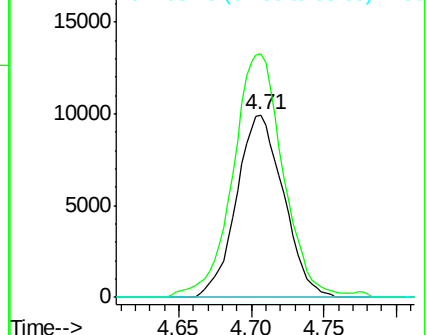

#34

Trichloroethene

Concen: 32.417 ug/L

RT: 6.57 min Scan# 1627

Delta R.T. -0.00 min

Lab File: VU038878.D

Acq: 13 Jun 2020 03:13

Tgt Ion: 95 Resp: 683232


Ion Ratio Lower Upper

95 100

97 64.7 46.1 85.5

132 95.9 67.5 125.3

130 99.3 66.7 123.9


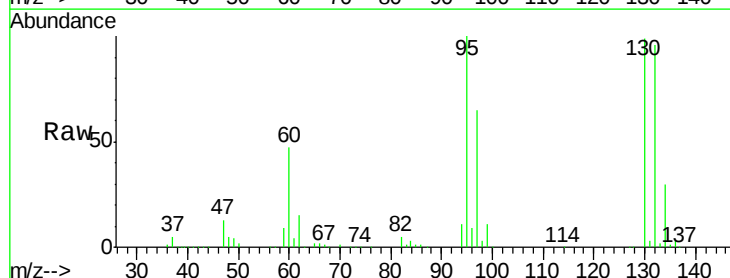



Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

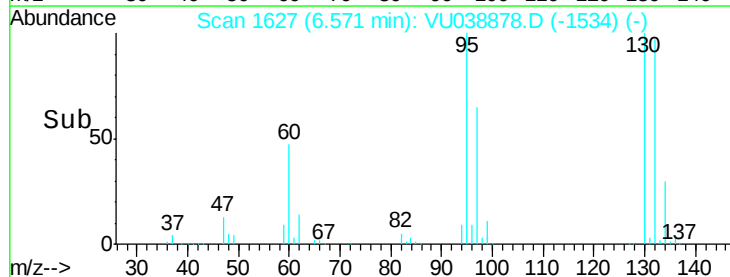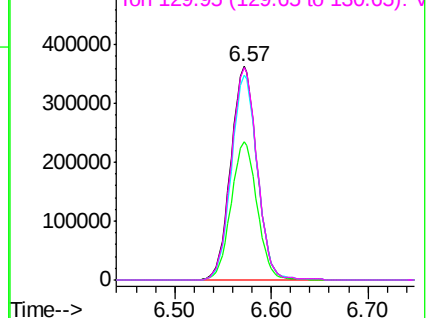

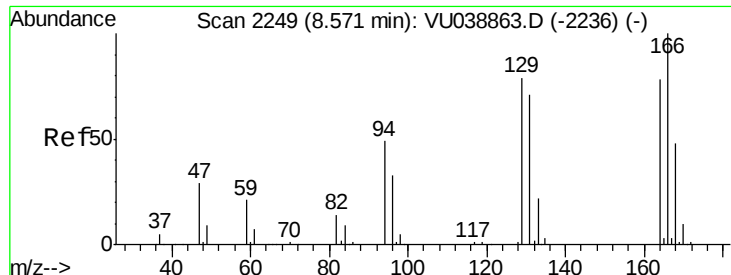

#47

Tetrachloroethene

Concen: 8.729 ug/L

RT: 8.57 min Scan# 2250

Delta R.T. 0.00 min

Lab File: VU038878.D


Acq: 13 Jun 2020 03:13

Instrument :

MSVOA_U

ClientSampleId :

BFT73

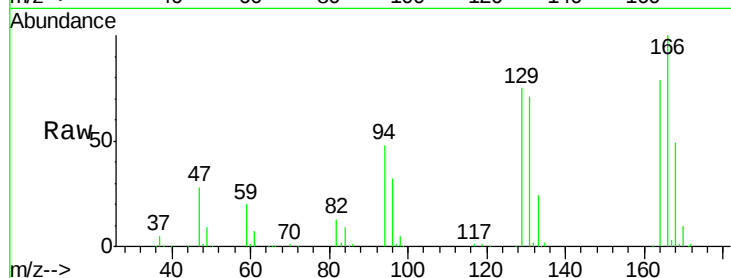

Tot Ion:164 Resp: 141642

Ion Ratio Lower Upper

164 100

129 94.4 67.3 124.9

131 89.2 65.0 120.6

166 125.8 91.0 169.0

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

