


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061320\
 Data File : VU038837.D
 Acq On : 12 Jun 2020 08:30
 Operator : SY/MD
 Sample : BFB12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB12

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jun 12 10:00:03 2020

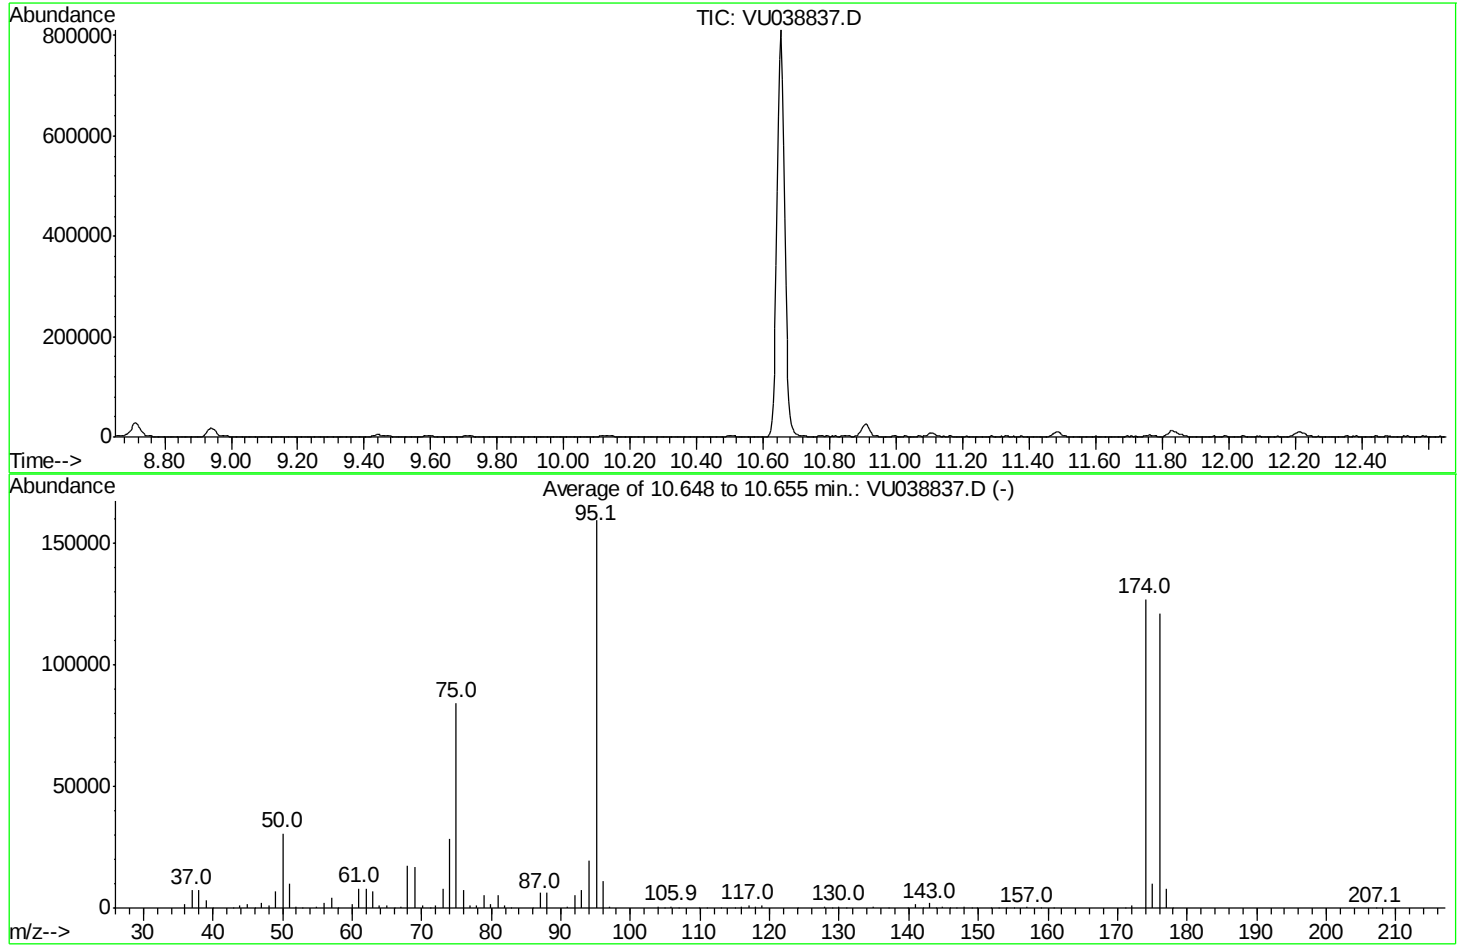

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	30562	PASS
75	95	30	80	53.0	84501	PASS
95	95	100	100	100.0	159573	PASS
96	95	5	9	7.0	11148	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.6	127066	PASS
175	174	5	9	7.8	9937	PASS
176	174	95	101	95.5	121328	PASS
177	176	5	9	6.5	7894	PASS

m/z	Abundance
36.00	1450.0
37.00	7488.0
38.00	7110.0
39.00	3016.0
40.00	274.0
42.90	122.0
44.00	1345.0
44.90	1409.0
46.00	208.0
47.00	1737.0
48.10	895.0
49.00	6304.0
50.00	30016.0
51.00	9683.0
51.90	419.0
54.90	429.0
56.00	2246.0
57.00	4203.0
57.90	160.0
60.00	1404.0
61.00	7680.0
62.00	7647.0
63.00	6380.0
64.00	888.0
65.00	1208.0
66.00	122.0
67.00	561.0
68.00	16928.0
69.00	16648.0
70.00	1243.0
72.00	813.0
73.00	7379.0
74.00	27528.0
75.00	82712.0
76.00	6927.0
77.00	1033.0
77.90	803.0
78.90	5011.0
79.90	1451.0
80.90	5138.0
81.90	1428.0
82.90	143.0
87.00	6246.0
88.00	6107.0
90.90	585.0
92.00	5116.0
93.00	7340.0
94.00	18976.0
95.10	151104.0
96.10	11098.0
97.10	297.0
103.90	744.0
104.90	156.0
105.90	773.0
106.80	155.0
109.70	130.0
110.90	134.0
113.00	149.0
115.00	136.0
115.90	486.0
116.90	1167.0
117.90	729.0
119.00	840.0
128.00	411.0
129.00	227.0
130.00	565.0
131.00	257.0
134.90	256.0
137.00	251.0
139.90	101.0
140.90	1548.0
142.10	294.0
143.00	1941.0
143.90	148.0
144.90	483.0
145.80	273.0
147.90	350.0
149.00	124.0
151.80	145.0
152.90	236.0
155.00	243.0
157.00	296.0
159.00	203.0
160.70	113.0
172.00	1102.0
174.00	120320.0
175.00	9538.0
176.00	113736.0
177.10	7729.0
178.00	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	1581.0
37.00	7614.0
38.00	7461.0
39.00	3057.0
39.90	275.0
40.10	267.0
44.00	1433.0
44.90	1439.0
46.10	244.0
47.00	2063.0
48.10	970.0
49.00	6951.0
50.00	31600.0
51.00	10758.0
52.00	525.0
52.90	129.0
54.90	427.0
56.00	2364.0
57.00	4436.0
58.00	157.0
60.00	1517.0
61.00	8517.0
62.00	7960.0
63.00	6923.0
64.00	855.0
65.00	1225.0
66.00	139.0
67.10	710.0
68.00	18216.0
69.00	17360.0
70.00	1341.0
71.20	105.0
72.10	930.0
73.00	8032.0
74.00	29000.0
75.00	87024.0
76.10	7394.0
77.00	1263.0
77.90	847.0
78.90	5608.0
79.90	1676.0
80.90	5779.0
81.90	1286.0
82.90	106.0
87.00	6341.0
88.00	6604.0
90.90	657.0
92.00	5360.0
93.00	7584.0
94.00	19496.0
95.10	164480.0
96.10	11512.0
97.00	309.0
103.90	775.0
104.90	177.0
105.90	803.0
106.90	206.0
109.80	136.0
110.90	134.0
112.90	160.0
115.00	149.0
115.80	553.0
116.90	1290.0
117.90	719.0
119.00	895.0
124.00	122.0
128.00	434.0
129.00	275.0
130.00	566.0
131.00	249.0
134.80	306.0
137.00	261.0
139.90	160.0
140.90	1568.0
142.10	295.0
143.00	2150.0
143.90	156.0
144.90	523.0
145.90	258.0
146.80	100.0
147.90	437.0
149.00	135.0
151.80	119.0
152.90	189.0
154.00	118.0
155.10	261.0
157.00	344.0
159.00	255.0
160.70	141.0
171.20	188.0
172.00	1139.0
174.00	131136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

175.00	10253.0
176.00	124800.0
177.00	8017.0
178.00	188.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	1612.0
37.00	7316.0
38.00	7180.0
39.00	2731.0
39.80	255.0
40.10	256.0
43.90	1394.0
45.00	1324.0
46.10	211.0
47.00	2129.0
48.10	930.0
49.00	6943.0
50.00	30072.0
51.00	10339.0
52.00	570.0
52.90	110.0
54.90	389.0
56.00	2355.0
57.00	4419.0
58.00	145.0
59.90	1462.0
61.00	8350.0
62.00	7743.0
63.00	6747.0
63.90	778.0
65.00	1143.0
66.00	108.0
67.10	802.0
68.00	17184.0
69.00	16784.0
70.10	1403.0
71.10	108.0
72.10	860.0
73.00	7908.0
74.00	28192.0
75.00	83768.0
76.10	7104.0
77.00	1207.0
77.90	861.0
78.90	5576.0
80.00	1712.0
80.90	5670.0
81.90	1176.0
86.00	288.0
87.00	5907.0
88.00	6623.0
90.90	664.0
92.00	4941.0
93.00	7271.0
94.10	19344.0
95.10	163136.0
96.10	10834.0
97.00	273.0
103.90	723.0
105.00	215.0
105.90	771.0
106.80	232.0
109.90	139.0
111.00	125.0
112.80	174.0
115.80	597.0
117.00	1236.0
117.90	592.0
118.90	952.0
123.90	117.0
127.90	456.0
129.00	308.0
130.00	511.0
131.00	216.0
134.80	331.0
137.00	263.0
139.90	170.0
140.90	1548.0
142.10	248.0
143.00	2118.0
143.90	127.0
144.80	428.0
145.90	229.0
146.80	109.0
147.90	514.0
149.00	151.0
149.80	103.0
153.00	107.0
154.00	108.0
155.10	297.0
157.00	361.0
159.00	252.0
160.80	175.0
171.20	204.0
172.00	1158.0
174.00	129744.0
175.10	10022.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

176.00	125448.0
177.00	7936.0
178.00	155.0
207.10	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

Scan 2882 (10.607 min): VU038837.D
BFB12

m/z	Abundance
36.10	154.0
39.80	192.0
43.80	507.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12