

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061323\
 Data File : VU054499.D
 Acq On : 13 Jun 2023 10:24
 Operator : MD/SY
 Sample : VU0613WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	114	rBV	105174	126032	13.09%	1.585%
2	1.914	186	194	209	rBV	113484	154209	16.01%	1.939%
3	2.566	384	397	416	rBV	178274	295368	30.67%	3.715%
4	3.046	536	546	563	rVB5	7669	15314	1.59%	0.193%
5	4.637	1028	1041	1080	rBV	118802	398034	41.33%	5.006%
6	5.058	1153	1172	1191	rBV2	178686	410755	42.65%	5.166%
7	5.721	1357	1378	1409	rBV2	364430	963107	100.00%	12.113%
8	6.245	1529	1541	1566	rBV	348333	679895	70.59%	8.551%
9	6.685	1665	1678	1699	rBV	237017	473677	49.18%	5.957%
10	7.563	1939	1951	1978	rBV2	93922	178439	18.53%	2.244%
11	7.894	2041	2054	2089	rBV	413226	748767	77.74%	9.417%
12	8.177	2131	2142	2158	rBV	59303	102083	10.60%	1.284%
13	8.634	2272	2284	2320	rBV2	434895	903223	93.78%	11.360%
14	9.415	2513	2527	2552	rBV	477493	830311	86.21%	10.443%
15	10.753	2931	2943	2962	rBV	162243	265668	27.58%	3.341%
16	11.807	3260	3271	3293	rVV	458088	754007	78.29%	9.483%
17	12.190	3377	3390	3411	rBV	360980	611202	63.46%	7.687%
18	13.846	3896	3905	3917	rBV5	8846	15411	1.60%	0.194%
19	14.100	3975	3984	3995	rBV5	5310	10316	1.07%	0.130%
20	14.331	4048	4056	4069	rVB5	8487	15167	1.57%	0.191%




Sum of corrected areas: 7950985

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061323\
Data File : VU054499.D
Acq On : 13 Jun 2023 10:24
Operator : MD/SY
Sample : VU0613WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

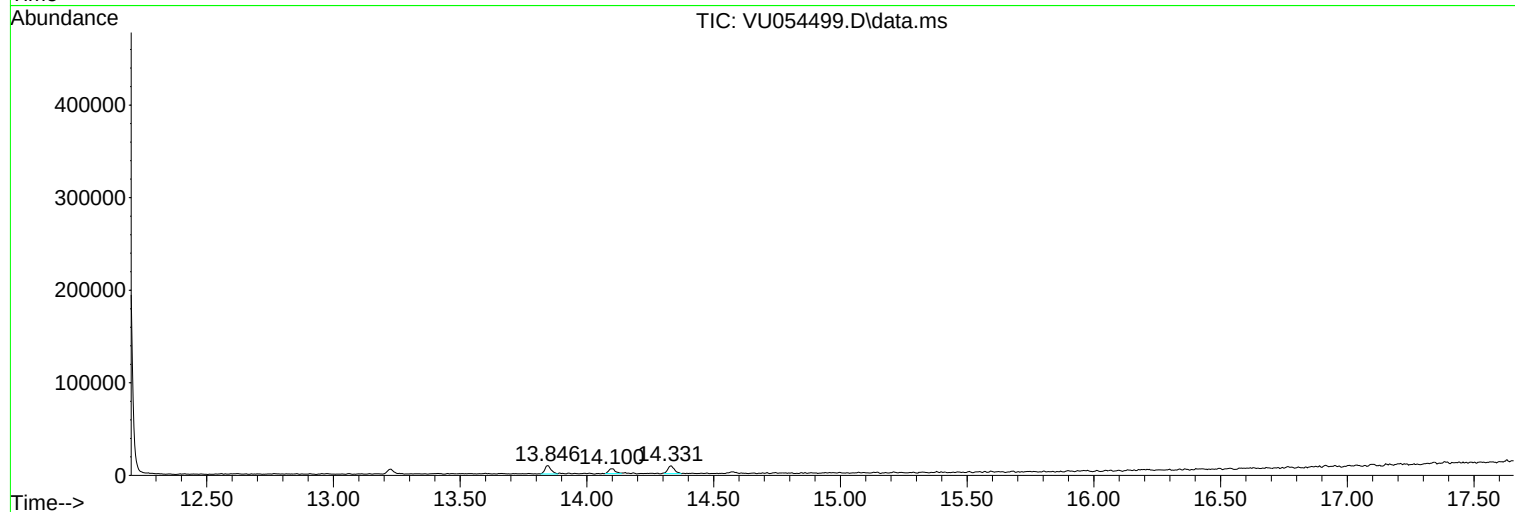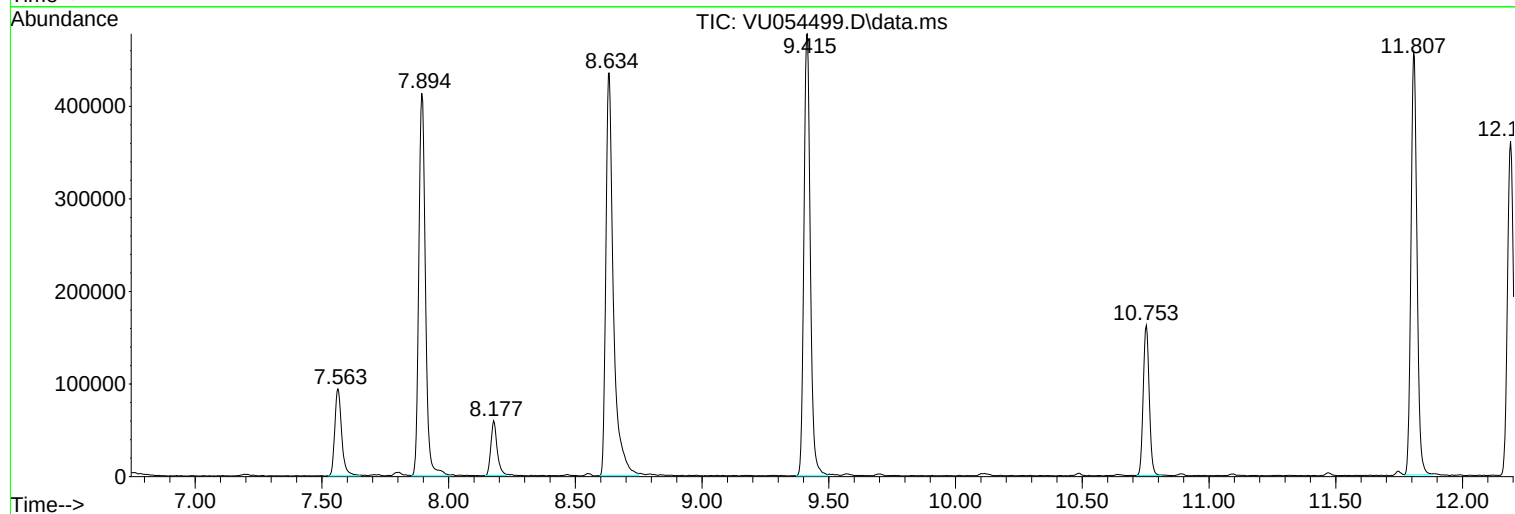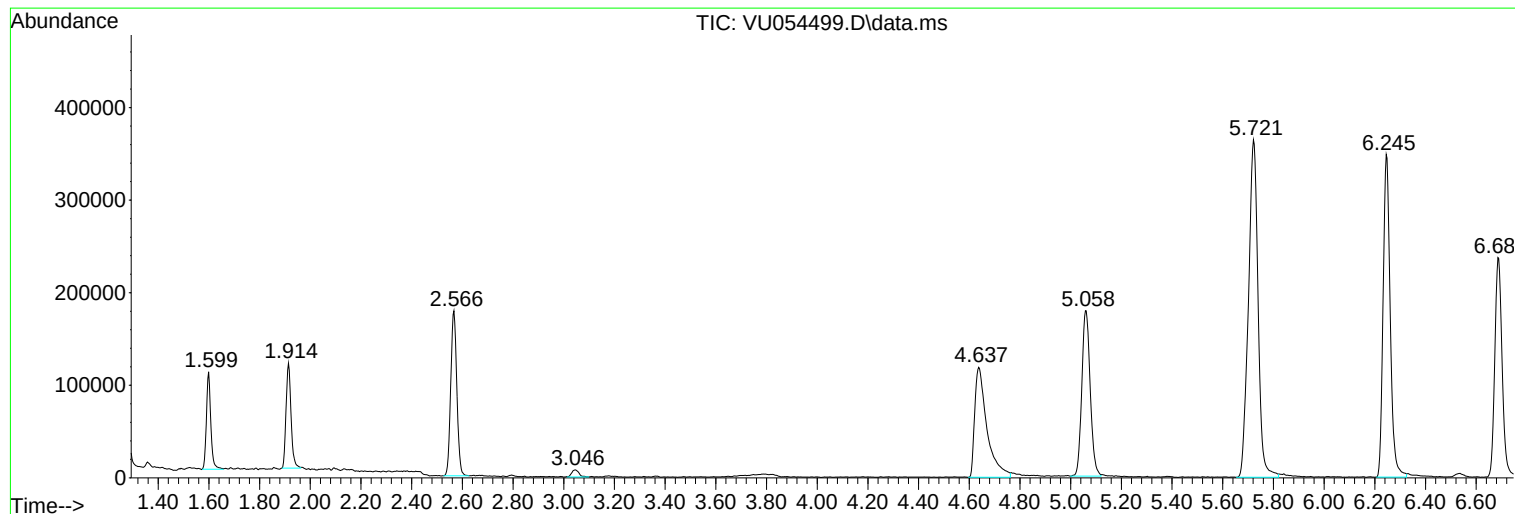

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061323\
Data File : VU054499.D
Acq On : 13 Jun 2023 10:24
Operator : MD/SY
Sample : VU0613WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061323\
Data File : VU054499.D
Acq On : 13 Jun 2023 10:24
Operator : MD/SY
Sample : VU0613WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
