


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061323\
 Data File : VU054497.D
 Acq On : 13 Jun 2023 09:04
 Operator : MD/SY
 Sample : BFB018
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB018

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jun 14 00:05:43 2023

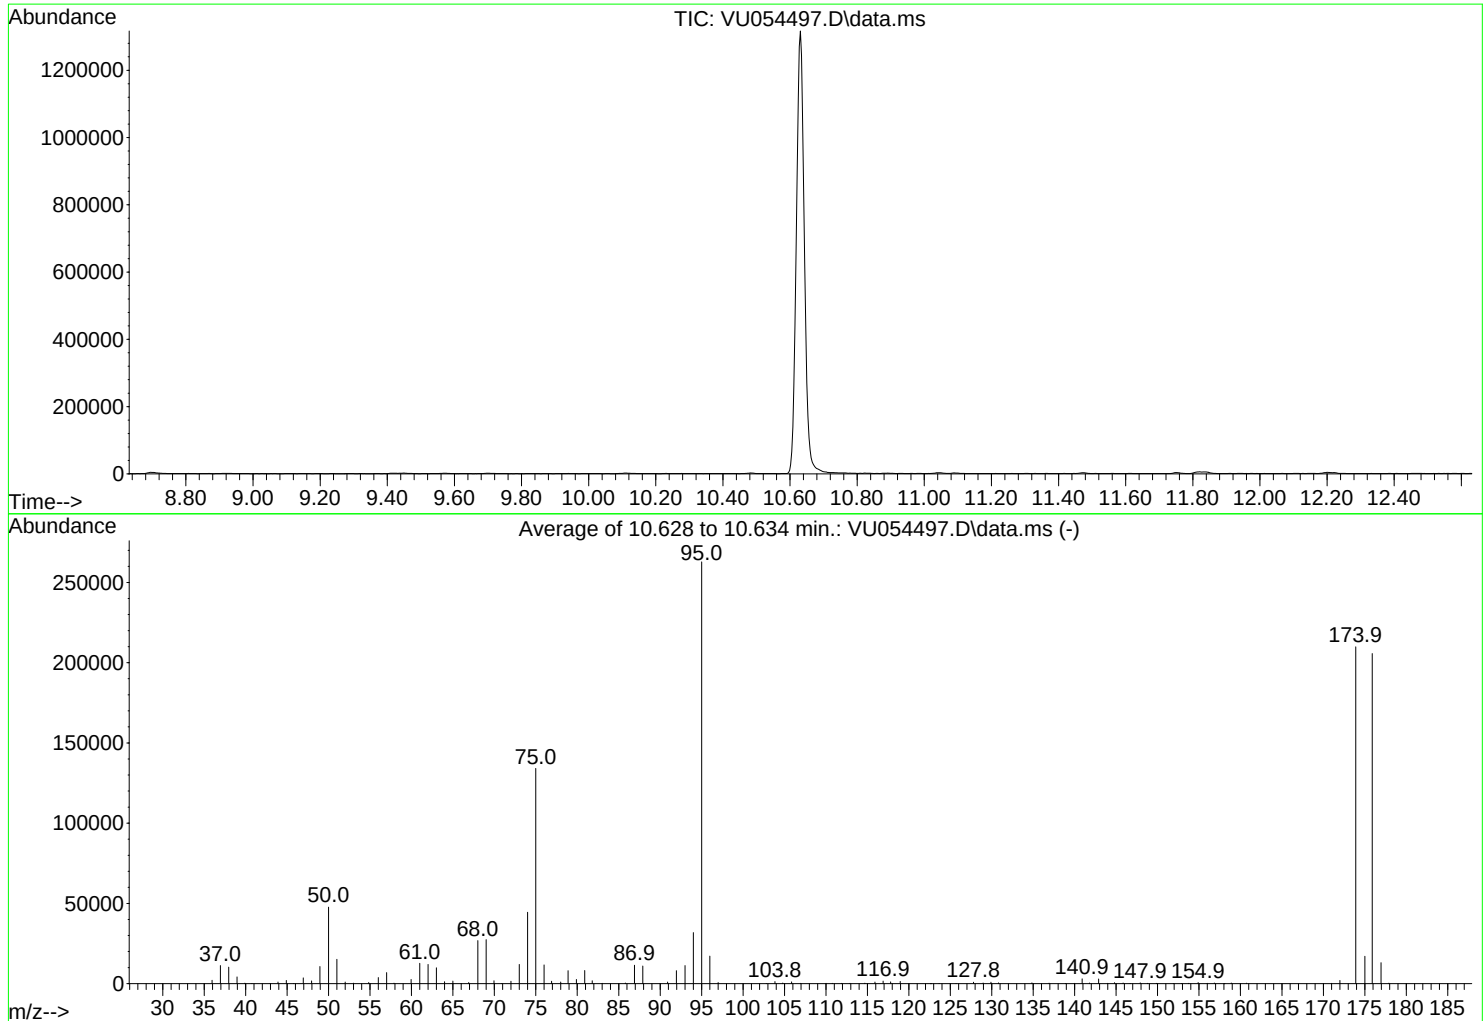

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	47653	PASS
75	95	30	80	51.0	134077	PASS
95	95	100	100	100.0	262848	PASS
96	95	5	9	6.5	17178	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.9	209899	PASS
175	174	5	9	8.1	17010	PASS
176	174	95	101	98.0	205675	PASS
177	176	5	9	6.4	13108	PASS

Scan 2890 (10.583 min): VU054497.D\data.ms
BFB018

m/z	Abundance
39.80	163.0
44.00	767.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
35.90	2129.0
36.90	11660.0
37.90	10522.0
39.00	4091.0
40.00	473.0
40.70	120.0
43.00	206.0
43.90	1673.0
44.90	1923.0
45.80	159.0
47.00	3697.0
47.90	1724.0
48.90	10604.0
50.00	49296.0
51.00	15555.0
52.00	934.0
53.00	275.0
54.90	672.0
56.00	3863.0
57.00	6706.0
57.90	303.0
60.00	2534.0
61.00	12683.0
62.00	12507.0
63.00	10109.0
64.00	1423.0
65.00	1494.0
66.90	726.0
68.00	26120.0
69.00	27056.0
69.90	1903.0
70.90	167.0
72.00	1551.0
73.00	12104.0
74.00	46112.0
75.00	134528.0
76.00	12455.0
76.90	1395.0
78.00	1002.0
78.90	7974.0
79.90	2663.0
80.90	8042.0
81.80	1735.0
83.00	266.0
85.80	560.0
86.90	11104.0
87.90	10724.0
90.90	948.0
92.00	7995.0
93.00	11551.0
94.00	31072.0
95.00	262976.0
96.00	17560.0
97.00	599.0
103.80	1410.0
104.90	455.0
105.90	1119.0
106.90	130.0
110.00	202.0
110.70	292.0
111.90	174.0
112.90	203.0
114.70	225.0
115.90	972.0
116.90	1616.0
117.80	1143.0
119.00	1414.0
123.70	122.0
127.80	901.0
129.00	421.0
129.90	878.0
130.80	516.0
134.90	576.0
136.90	357.0
138.90	119.0
139.90	104.0
140.90	3089.0
141.80	413.0
142.90	2937.0
144.00	190.0
144.80	628.0
145.80	404.0
146.70	207.0
147.90	509.0
148.80	181.0
149.90	241.0
151.90	139.0
153.70	199.0
154.90	651.0
156.00	199.0
156.80	340.0
158.90	363.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

160.80	312.0
171.00	296.0
172.00	1989.0
173.90	204096.0
175.00	16327.0
175.90	201216.0
176.90	13282.0
177.90	323.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
36.00	2191.0
37.00	11568.0
38.00	10526.0
39.00	4339.0
39.90	501.0
40.80	111.0
42.90	153.0
43.90	1840.0
44.90	2004.0
45.80	148.0
47.00	3762.0
48.00	1758.0
49.00	11195.0
50.00	49280.0
51.00	15636.0
52.00	1006.0
53.00	270.0
54.80	702.0
56.00	4047.0
57.00	7116.0
57.90	367.0
60.00	2604.0
61.00	13094.0
62.00	12208.0
63.00	10255.0
64.00	1262.0
65.00	1609.0
66.00	122.0
66.90	750.0
68.00	27752.0
69.00	28464.0
69.90	1899.0
70.90	130.0
72.00	1528.0
73.00	12316.0
74.00	45696.0
75.00	138304.0
76.00	11936.0
76.90	1542.0
78.00	1038.0
78.90	8369.0
79.90	2668.0
80.90	8402.0
81.80	1849.0
83.00	268.0
85.80	453.0
86.90	11893.0
87.90	11325.0
90.90	995.0
91.90	8424.0
93.00	11472.0
94.00	32936.0
95.00	270272.0
96.00	17664.0
97.00	722.0
102.80	118.0
103.90	1351.0
104.80	415.0
105.90	1090.0
107.00	154.0
110.00	232.0
110.70	247.0
111.80	227.0
112.90	242.0
114.70	279.0
115.90	1041.0
116.90	1660.0
117.80	1214.0
118.90	1460.0
123.60	158.0
125.70	123.0
127.80	933.0
128.90	466.0
129.90	901.0
130.80	554.0
134.80	535.0
136.90	375.0
138.90	125.0
140.00	204.0
140.90	3155.0
141.80	386.0
142.90	2994.0
144.00	167.0
144.80	598.0
145.90	446.0
146.70	158.0
147.90	495.0
148.80	182.0
149.90	260.0
151.90	132.0
152.90	111.0
153.80	191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

154.90	744.0
156.00	196.0
156.80	424.0
158.90	393.0
160.70	345.0
171.00	280.0
172.00	1958.0
173.90	216448.0
175.00	17488.0
175.90	212416.0
176.90	13388.0
177.90	389.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
36.00	2042.0
37.00	10498.0
38.00	9801.0
38.90	4148.0
39.90	491.0
43.00	114.0
43.90	1842.0
44.90	1933.0
45.80	151.0
46.90	3470.0
48.00	1536.0
49.00	10402.0
50.00	44384.0
51.00	14225.0
52.00	982.0
53.00	281.0
54.90	674.0
56.00	3611.0
57.00	6796.0
57.90	391.0
59.90	2548.0
61.00	12098.0
62.00	11106.0
63.00	9378.0
64.00	1069.0
65.00	1621.0
66.00	155.0
66.90	651.0
68.00	26712.0
69.00	26624.0
70.00	1695.0
72.00	1320.0
73.00	11415.0
74.00	41616.0
75.00	129400.0
76.00	10571.0
76.90	1522.0
78.00	1049.0
78.90	7909.0
79.90	2399.0
80.90	8065.0
81.80	1760.0
83.00	230.0
85.70	313.0
86.90	11488.0
87.90	10767.0
90.90	1062.0
91.90	7878.0
93.00	10736.0
94.00	31544.0
95.00	255296.0
96.00	16310.0
97.00	692.0
102.80	158.0
103.80	1130.0
104.70	379.0
105.80	1089.0
107.00	223.0
110.00	210.0
110.80	185.0
111.80	271.0
112.90	277.0
114.70	325.0
115.90	912.0
116.90	1628.0
117.80	1096.0
118.90	1377.0
122.60	111.0
123.60	173.0
125.70	130.0
127.80	912.0
128.90	442.0
129.90	858.0
130.80	444.0
134.80	461.0
136.90	361.0
140.00	243.0
140.90	2791.0
141.80	313.0
142.90	2815.0
144.00	175.0
144.80	529.0
145.90	386.0
146.70	112.0
147.90	450.0
148.80	206.0
149.80	244.0
151.90	102.0
152.90	167.0
153.80	159.0
154.90	738.0
156.00	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

156.90	559.0
158.00	122.0
158.90	348.0
160.80	318.0
172.00	1919.0
173.90	209152.0
175.00	17216.0
175.90	203392.0
177.00	12654.0
177.90	371.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018