

Data File : VU032737.D
Acq On : 14 Jun 2019 21:21
Operator : JC/SP
Sample : K3365-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM62

Quant Time: Jun 14 23:54:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 23:49:20 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	101341	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	95118	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	46287	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	28579	4.34	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.80%
7) Chloroethane-d5	1.67	69	24642	4.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.60%
11) 1,1-Dichloroethene-d2	2.27	63	83039	6.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	124.20%
20) 2-Butanone-d5	4.18	46	96280	52.36	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.72%
24) Chloroform-d	4.64	84	59967	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
26) 1,2-Dichloroethane-d4	5.30	65	34574	5.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.20%
32) Benzene-d6	5.33	84	112679	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
36) 1,2-Dichloropropane-d6	6.32	67	38678	5.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.20%
41) Toluene-d8	7.56	98	98399	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.00%
43) trans-1,3-Dichloropropene-	7.85	79	13571	4.36	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.20%
46) 2-Hexanone-d5	8.31	63	75056	48.09	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.18%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	33364	5.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	40767	4.90	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.00%

Target Compounds

					Qvalue
3) Chloromethane	1.33	50	3187	0.353 ug/L	99
12) 1,1-Dichloroethene	2.28	96	68050	10.569 ug/L	88
13) Acetone	2.32	43	5069	3.552 ug/L	98
15) Methyl Acetate	2.61	43	593	0.151 ug/L #	60
18) trans-1,2-Dichloroethene	2.98	96	453	0.065 ug/L #	70
19) 1,1-Dichloroethane	3.43	63	5721	0.460 ug/L	91
22) cis-1,2-Dichloroethene	4.22	96	81263	10.336 ug/L	86
25) Chloroform	4.66	83	2396	0.189 ug/L	88
29) 1,1,1-Trichloroethane	4.90	97	84228	7.267 ug/L	97
31) Carbon tetrachloride	4.90	117	10869	1.031 ug/L	100
34) Trichloroethene	6.18	95	1245741	154.431 ug/L	98
35) Methylcyclohexane	6.32	83	8484	0.654 ug/L #	19
37) 1,2-Dichloropropane	6.32	63	4024	0.555 ug/L #	89
45) 1,1,2-Trichloroethane	8.06	97	933	0.177 ug/L	88
48) 2-Hexanone	8.31	43	10629	2.880 ug/L #	73
59) 1,2,3-Trichloropropane	11.48	75	5969	1.253 ug/L #	87

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061419\
Quantitation Report (Not Reviewed)

Data File : VU032737.D
Acq On : 14 Jun 2019 21:21
Operator : JC/SP
Sample : K3365-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM62

Quant Time: Jun 14 23:54:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 23:49:20 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU032737.D
Acq On : 14 Jun 2019 21:21
Operator : JC/SP
Sample : K3365-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM62

Quant Time: Jun 14 23:54:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 23:49:20 2019
Response via : Initial Calibration

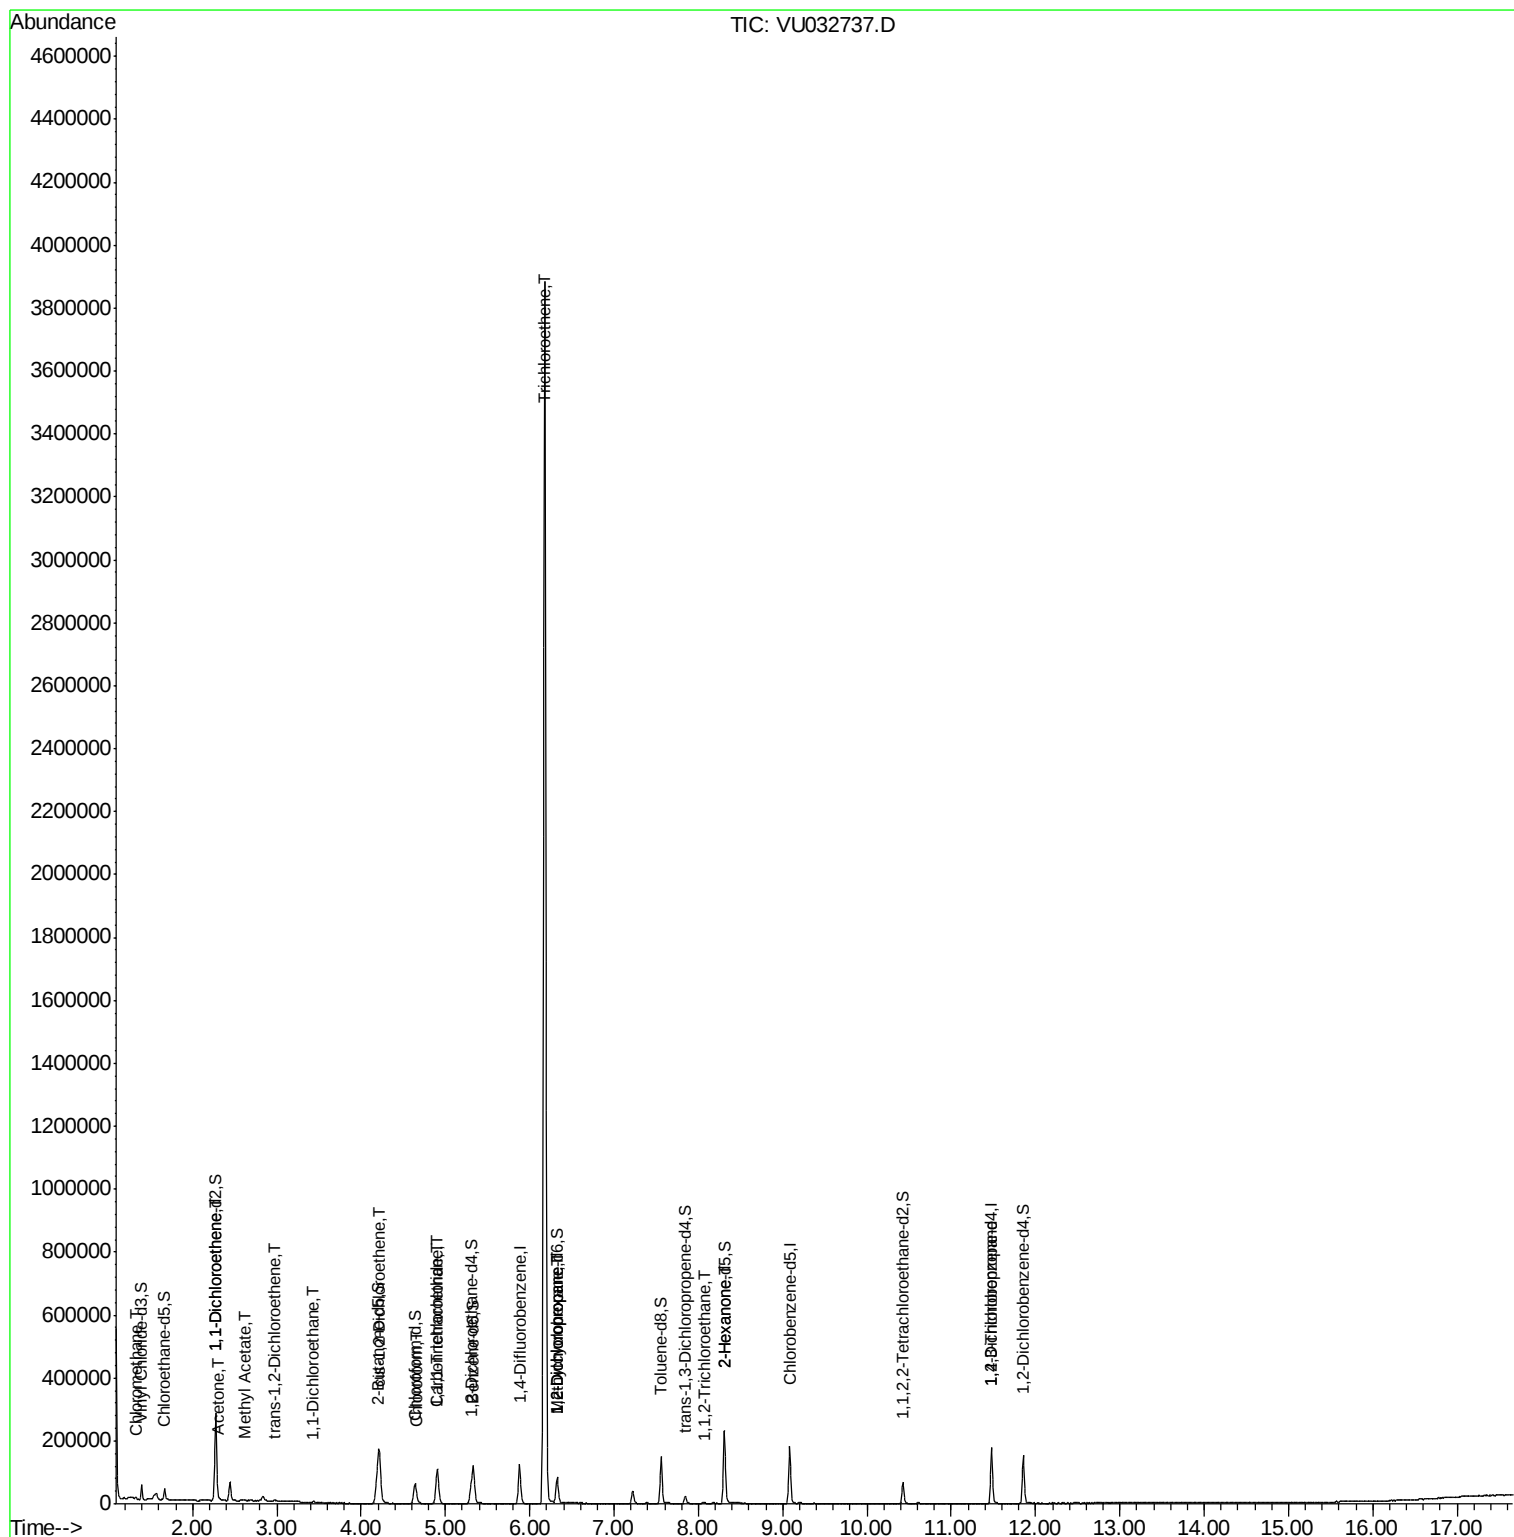

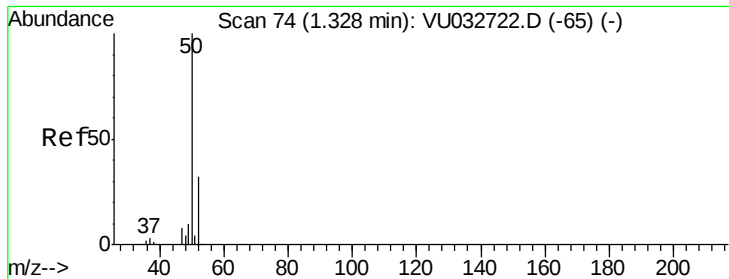

#3

Chloromethane

Concen: 0.353 ug/L

RT: 1.33 min Scan# 74

Delta R.T. 0.00 min

Lab File: VU032737.D

Acq: 14 Jun 2019 21:21

Instrument :

MSVOA_U

ClientSampleId :





COM62

Tgt Ion: 50 Resp: 3187

Ion Ratio Lower Upper

50 100

52 32.5 23.2 43.2

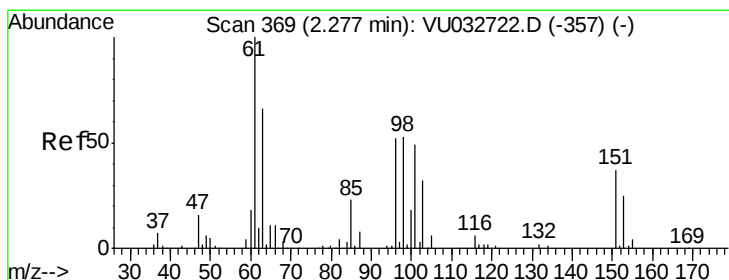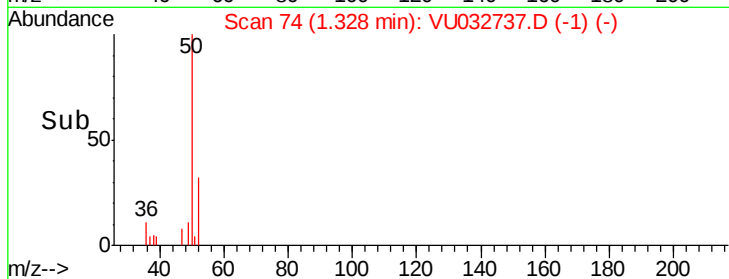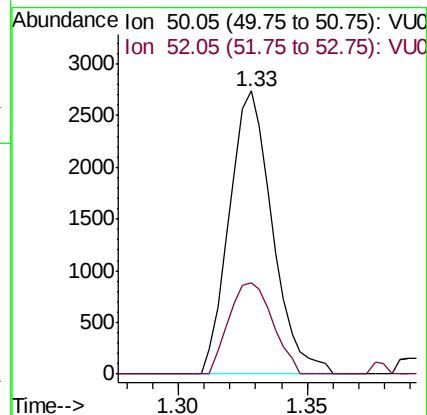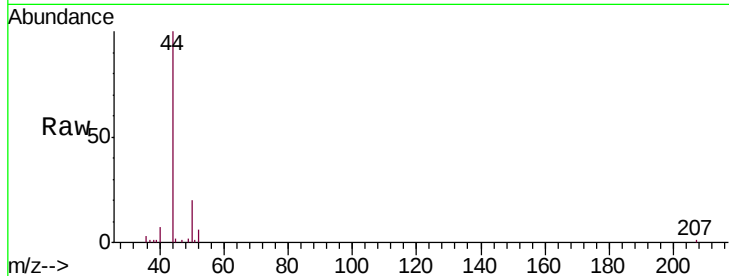

#12

1,1-Dichloroethene

Concen: 10.569 ug/L

RT: 2.28 min Scan# 369

Delta R.T. 0.00 min

Lab File: VU032737.D

Acq: 14 Jun 2019 21:21




Tgt Ion: 96 Resp: 68050


Ion Ratio Lower Upper

96 100

61 188.6 131.8 244.8

63 96.0 90.1 167.3

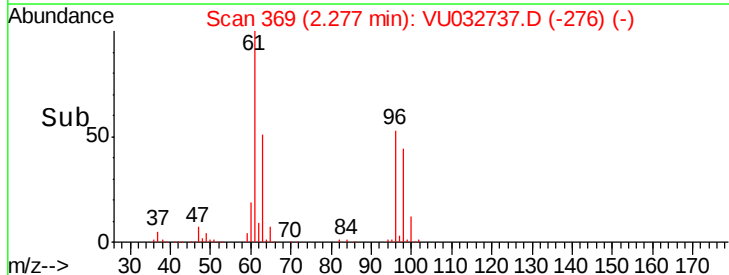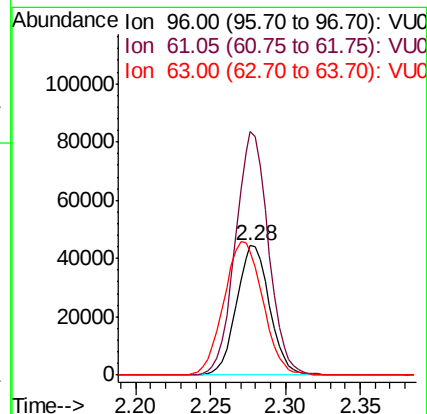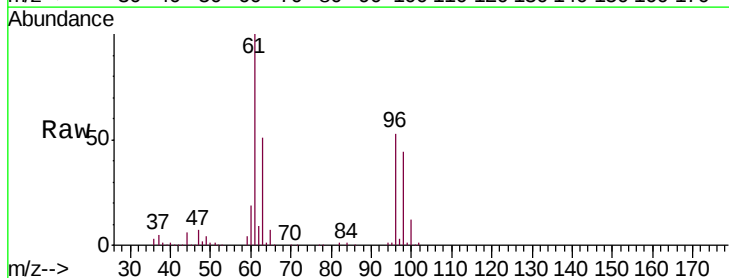



#13

Acetone

Concen: 3.552 ug/L

RT: 2.32 min Scan# 381

Delta R.T. 0.00 min

Lab File: VU032737.D

Acq: 14 Jun 2019 21:21

Instrument :

MSVOA_U

ClientSampleId :


C0M62

Tgt Ion: 43 Resp: 5069

Ion Ratio Lower Upper

43 100

58 31.4 0.0 60.8



Abundance Ion 43.05 (42.75 to 43.75): VU032722.D (-355) (-)

Ion 58.05 (57.75 to 58.75): VU032722.D (-355) (-)

2.32



3000

2000

1000

0

Time--> 2.25 2.30 2.35



#15

Methyl Acetate

Concen: 0.151 ug/L

RT: 2.61 min Scan# 474

Delta R.T. 0.00 min

Lab File: VU032737.D


Acq: 14 Jun 2019 21:21

Tgt Ion: 43 Resp: 593

Ion Ratio Lower Upper

43 100

74 3.2 17.8 26.8#



Abundance Ion 43.05 (42.75 to 43.75): VU032722.D (-458) (-)

Ion 74.05 (73.75 to 74.75): VU032722.D (-458) (-)

2.61

600

500

400


300


200

100

0

Time--> 2.55 2.60 2.65



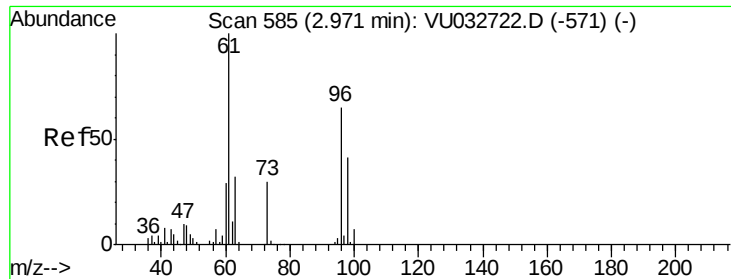

#18

trans-1,2-Dichloroethene

Concen: 0.065 ug/L

RT: 2.98 min Scan# 587

Delta R.T. 0.01 min

Lab File: VU032737.D

Acq: 14 Jun 2019 21:21

Instrument :

MSVOA_U

ClientSampled :

C0M62


Tgt Ion: 96 Resp: 453

Ion Ratio Lower Upper

96 100

61 100.0 103.1 191.5#




98 54.5 43.7 81.1

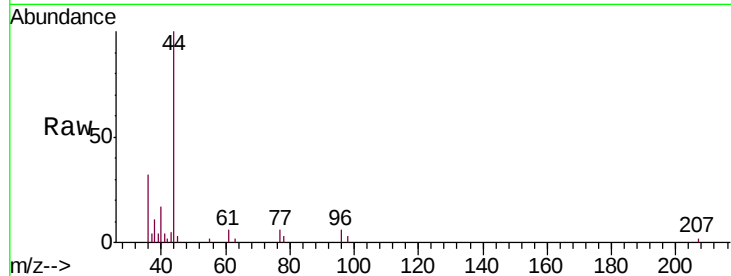

Abundance Ion 96.00 (95.70 to 96.70): VU032737.D (-587) (-)

Ion 61.05 (60.75 to 61.75): VU032737.D (-587) (-)

Ion 97.95 (97.65 to 98.65): VU032737.D (-587) (-)

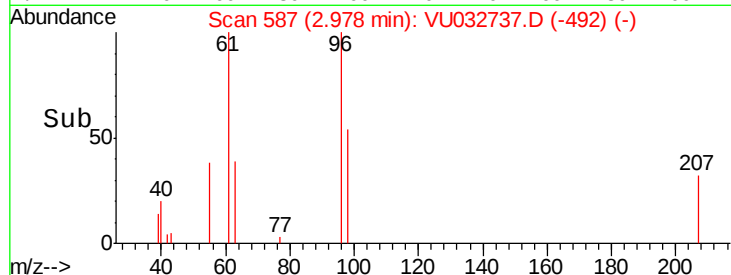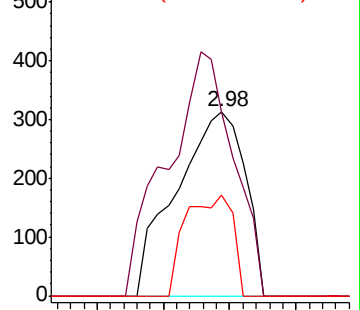

#19

1,1-Dichloroethane

Concen: 0.460 ug/L

RT: 3.43 min Scan# 729

Delta R.T. 0.00 min

Lab File: VU032737.D

Acq: 14 Jun 2019 21:21


Tgt Ion: 63 Resp: 5721

Ion Ratio Lower Upper

63 100

65 37.2 21.3 39.6



83 13.7 10.1 18.7




Abundance Ion 63.10 (62.80 to 63.80): VU032737.D (-729) (-)

Ion 65.10 (64.80 to 65.80): VU032737.D (-729) (-)

Ion 83.05 (82.75 to 83.75): VU032737.D (-729) (-)

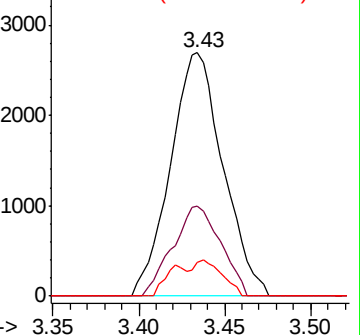




#22




cis-1,2-Dichloroethene
 Concen: 10.336 ug/L
 RT: 4.22 min Scan# 972
 Delta R.T. 0.00 min
 Lab File: VU032737.D
 Acq: 14 Jun 2019 21:21

Instrument :
 MSVOA_U
 ClientSampleId :
 COM62

Tgt Ion: 96 Resp: 81263
 Ion Ratio Lower Upper
 96 100
 61 139.7 86.6 160.8
 68 0.0 0.0 0.0

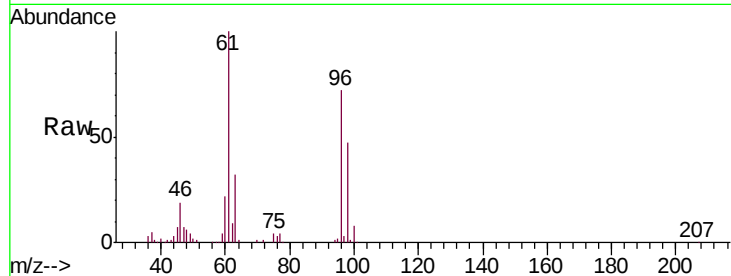


Abundance Ion 96.00 (95.70 to 96.70): VU0
 Ion 61.05 (60.75 to 61.75): VU0
 Ion 68.15 (67.85 to 68.85): VU0

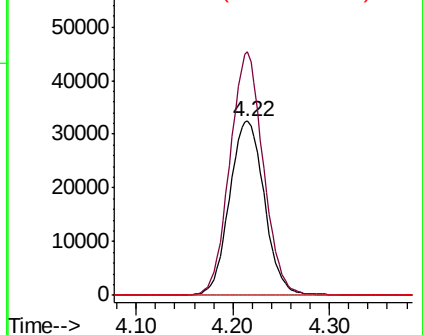



#25


Chloroform
 Concen: 0.189 ug/L
 RT: 4.66 min Scan# 1111
 Delta R.T. 0.00 min
 Lab File: VU032737.D
 Acq: 14 Jun 2019 21:21

Tgt Ion: 83 Resp: 2396
 Ion Ratio Lower Upper
 83 100
 85 71.7 43.8 81.3



Abundance Ion 83.05 (82.75 to 83.75): VU0
 Ion 85.00 (84.70 to 85.70): VU0

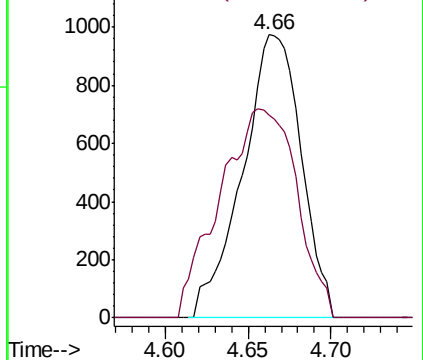



#29

1,1,1-Trichloroethane

Concen: 7.267 ug/L

RT: 4.90 min Scan# 1186

Delta R.T. 0.00 min

Lab File: VU032737.D

Acq: 14 Jun 2019 21:21

Instrument :

MSVOA_U

ClientSampleId :

C0M62


Tgt Ion: 97 Resp: 84228

Ion Ratio Lower Upper

97 100

99 62.4 51.8 77.6




61 45.8 34.7 52.1

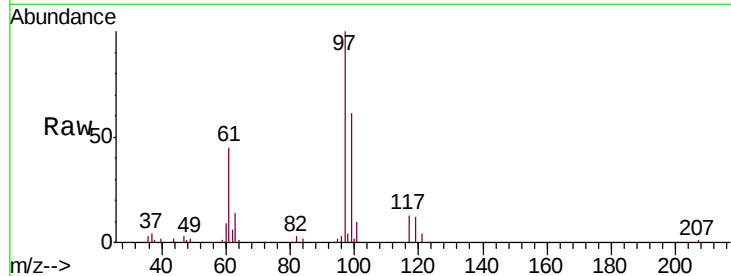

Abundance Ion 96.95 (96.65 to 97.65): VU032722.D (-1168) (-)

Ion 99.05 (98.75 to 99.75): VU032722.D (-1168) (-)

Ion 61.05 (60.75 to 61.75): VU032722.D (-1168) (-)

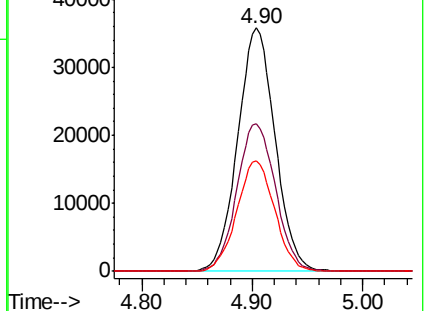

#31

Carbon tetrachloride

Concen: 1.031 ug/L

RT: 4.90 min Scan# 1186

Delta R.T. -0.22 min

Lab File: VU032737.D


Acq: 14 Jun 2019 21:21

Tgt Ion: 117 Resp: 10869

Ion Ratio Lower Upper



117 100


119 97.0 77.8 116.6

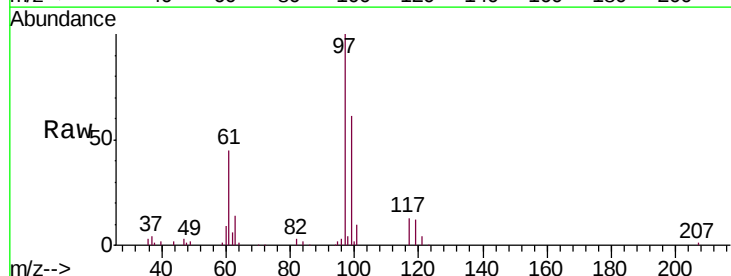

Abundance Ion 116.90 (116.60 to 117.60): VU032722.D (-1237) (-)

Ion 118.90 (118.60 to 119.60): VU032722.D (-1237) (-)

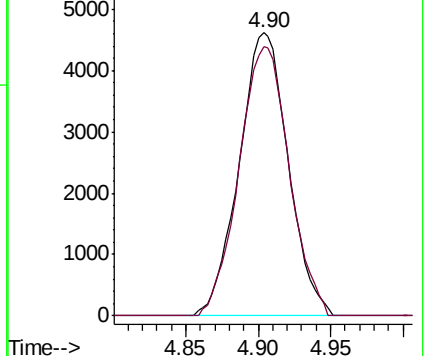

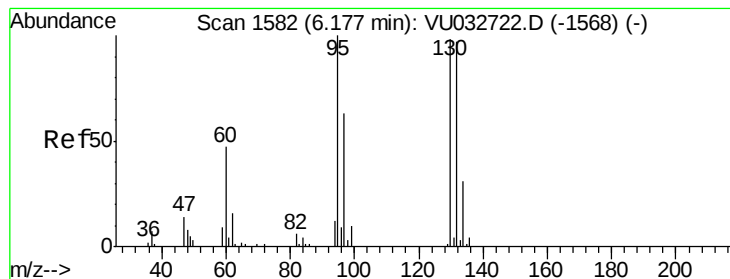

#34

Trichloroethene

Concen: 154.431 ug/L

RT: 6.18 min Scan# 1582

Delta R.T. 0.00 min

Lab File: VU032737.D

Acq: 14 Jun 2019 21:21

Instrument :

MSVOA_U

ClientSampleId :

COM62

Tgt Ion: 95 Resp: 1245741





Ion Ratio Lower Upper

95 100

97 65.0 44.1 81.9

132 96.8 68.8 127.8

130 100.4 71.0 131.8

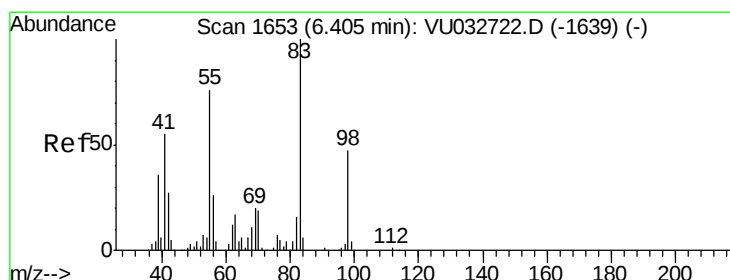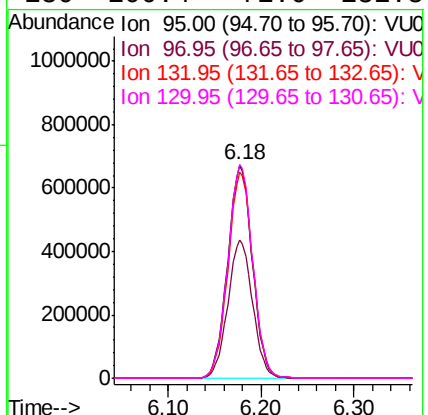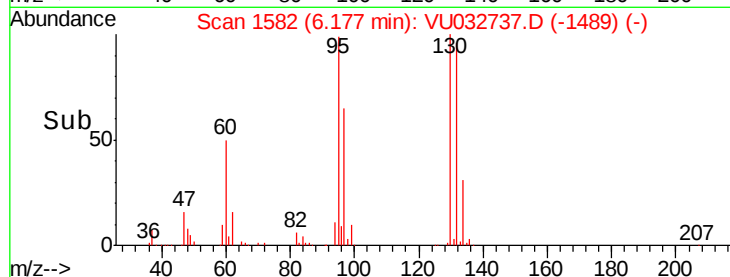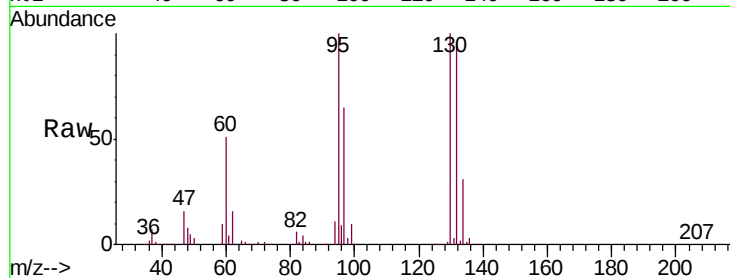

#35

Methylcyclohexane

Concen: 0.654 ug/L

RT: 6.32 min Scan# 1628

Delta R.T. -0.08 min

Lab File: VU032737.D

Acq: 14 Jun 2019 21:21




Tgt Ion: 83 Resp: 8484


Ion Ratio Lower Upper

83 100

55 0.0 60.0 90.0#

98 0.0 37.8 56.8#


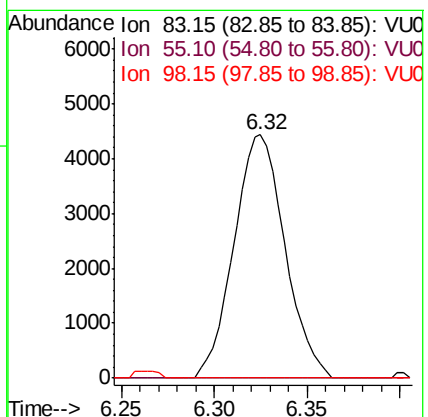
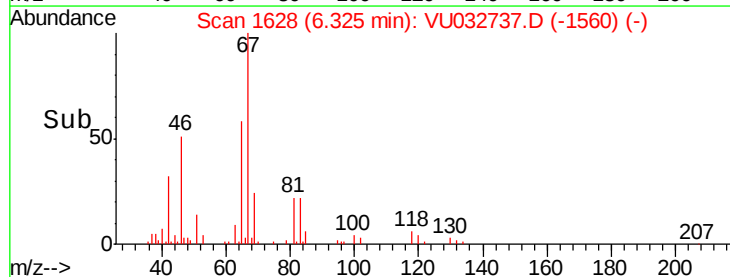
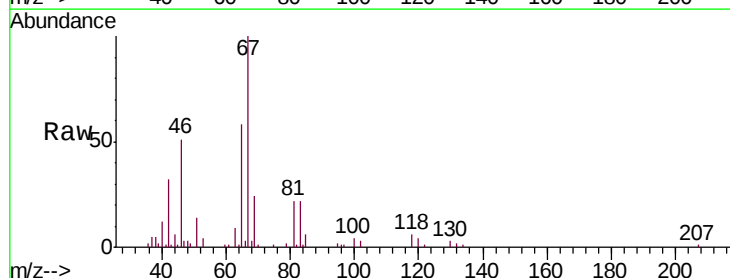


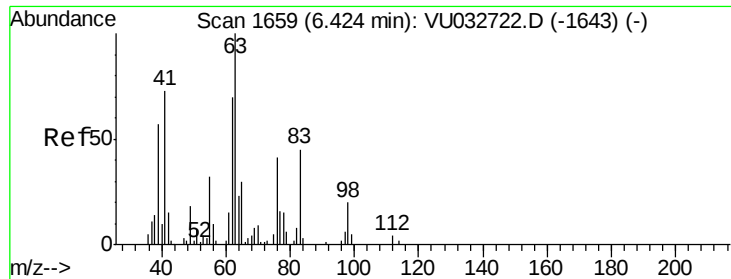

#37
 1,2-Dichloropropane
 Concen: 0.555 ug/L
 RT: 6.32 min Scan# 1627
 Delta R.T. -0.10 min
 Lab File: VU032737.D
 Acq: 14 Jun 2019 21:21




Instrument :
 MSVOA_U
 ClientSampleId :
 COM62


Tgt Ion: 63 Resp: 4024
 Ion Ratio Lower Upper
 63 100
 112 0.0 2.9 4.3#

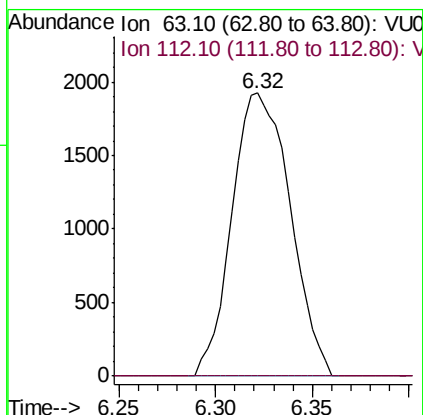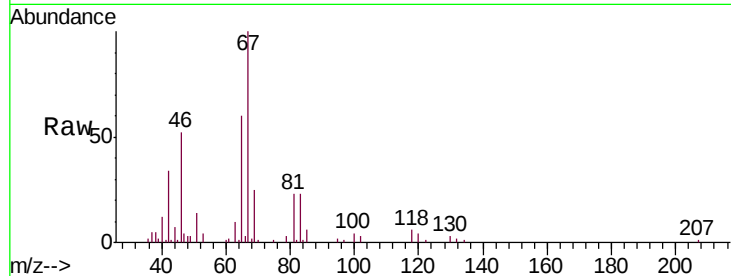

#45
 1,1,2-Trichloroethane
 Concen: 0.177 ug/L
 RT: 8.06 min Scan# 2169
 Delta R.T. 0.00 min
 Lab File: VU032737.D
 Acq: 14 Jun 2019 21:21

Tgt Ion: 97 Resp: 933
 Ion Ratio Lower Upper
 97 100
 99 50.1 44.9 83.3
 83 70.9 58.7 108.9
 85 52.0 37.9 70.5



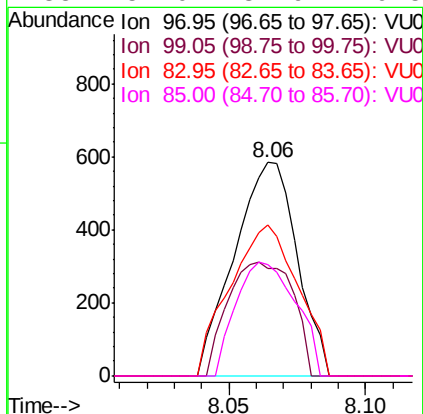





#48
2-Hexanone
Concen: 2.880 ug/L
RT: 8.31 min Scan# 2244
Delta R.T. -0.05 min
Lab File: VU032737.D
Acq: 14 Jun 2019 21:21

Instrument :
MSVOA_U
ClientSampleId :
COM62

Tgt Ion: 43 Resp: 10629
Ion Ratio Lower Upper
43 100
58 30.0 41.9 62.9#
57 23.5 15.1 22.7#
100 0.0 9.0 13.6#

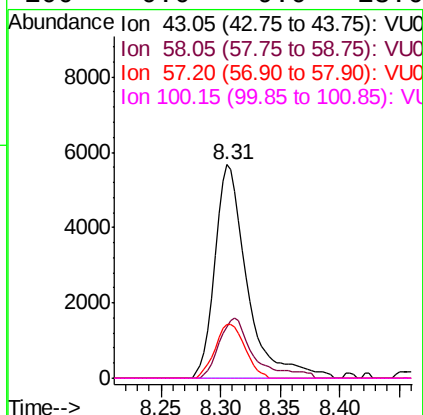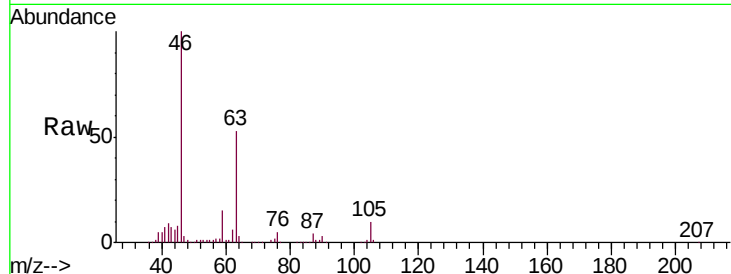

#59
1,2,3-Trichloropropane
Concen: 1.253 ug/L
RT: 11.48 min Scan# 3231
Delta R.T. 0.99 min
Lab File: VU032737.D
Acq: 14 Jun 2019 21:21

Tgt Ion: 75 Resp: 5969
Ion Ratio Lower Upper
75 100
77 38.7 25.3 37.9#

