

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
 Data File : VU032714.D
 Acq On : 13 Jun 2019 23:25
 Operator : JC/SP
 Sample : K3364-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM35

Quant Time: Jun 14 08:59:55 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 14 07:38:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	91246	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	87410	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	40068	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	28253	4.76	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.20%
7) Chloroethane-d5	1.67	69	23791	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.80%
11) 1,1-Dichloroethene-d2	2.27	63	43640	3.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.60%
20) 2-Butanone-d5	4.18	46	90006	54.36	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.72%
24) Chloroform-d	4.64	84	57098	5.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.40%
26) 1,2-Dichloroethane-d4	5.30	65	33202	5.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	119.60%
32) Benzene-d6	5.33	84	110886	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.00%
36) 1,2-Dichloropropane-d6	6.32	67	36213	5.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.20%
41) Toluene-d8	7.56	98	95528	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.00%
43) trans-1,3-Dichloropropene-	7.85	79	11735	4.10	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.00%
46) 2-Hexanone-d5	8.31	63	43955	30.65	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	61.30%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	26246	4.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	38898	5.40	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.00%


Target Compounds					Ovalue
13) Acetone	2.32	43	4743	3.691 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032714.D
Acq On : 13 Jun 2019 23:25
Operator : JC/SP
Sample : K3364-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM35

Quant Time: Jun 14 08:59:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 07:38:22 2019
Response via : Initial Calibration

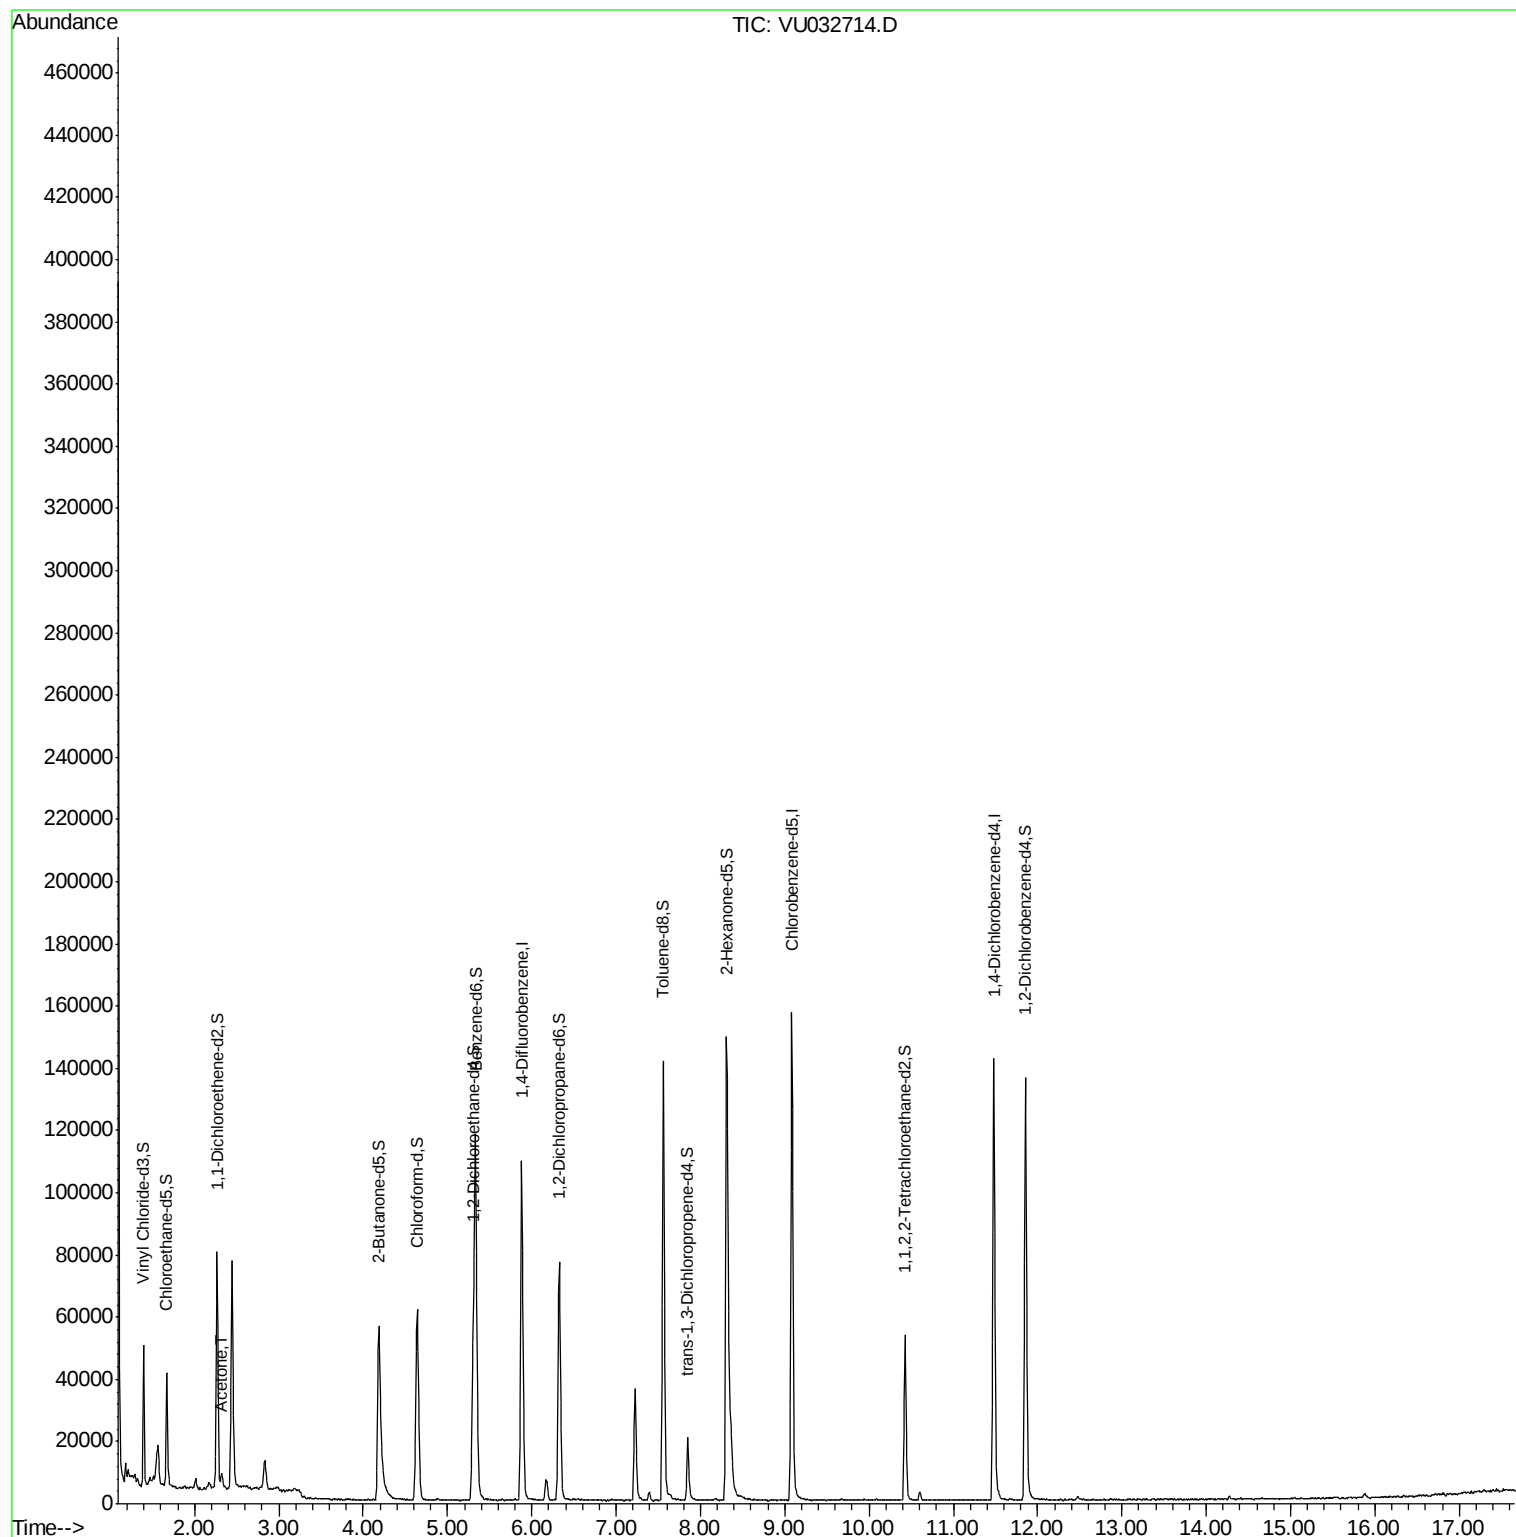

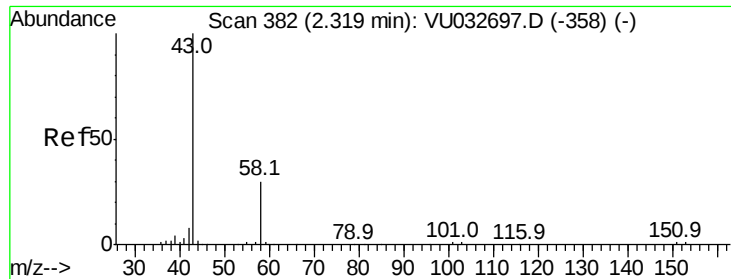

#13

Acetone

Concen: 3.691 ug/L

RT: 2.32 min Scan# 382

Delta R.T. -0.00 min

Lab File: VU032714.D

Acq: 13 Jun 2019 23:25

Instrument :

MSVOA_U

ClientSampleId :

COM35

Tot Ion: 43 Resp: 4743

Ion Ratio Lower Upper

43 100

58 27.3 0.0 60.8

