

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
 Data File : VU032716.D
 Acq On : 14 Jun 2019 00:14
 Operator : JC/SP
 Sample : K3364-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM37

Quant Time: Jun 17 16:01:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 14 07:38:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	91394	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	88319	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	40773	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	26574	4.47	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.40%
7) Chloroethane-d5	1.67	69	23684	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.20%
11) 1,1-Dichloroethene-d2	2.27	63	42649	3.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.80%
20) 2-Butanone-d5	4.18	46	91268	55.03	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.06%
24) Chloroform-d	4.64	84	56776	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.60%
26) 1,2-Dichloroethane-d4	5.31	65	33160	5.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	119.20%
32) Benzene-d6	5.33	84	109265	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
36) 1,2-Dichloropropane-d6	6.32	67	35222	5.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.20%
41) Toluene-d8	7.56	98	93709	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
43) trans-1,3-Dichloropropene-	7.85	79	11743	4.06	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.20%
46) 2-Hexanone-d5	8.31	63	46443	32.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	64.10%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	26612	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	38567	5.26	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.20%


Target Compounds					Ovalue
13) Acetone	2.32	43	3176	2.468 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032716.D
Acq On : 14 Jun 2019 00:14
Operator : JC/SP
Sample : K3364-16
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM37

Quant Time: Jun 17 16:01:08 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 07:38:22 2019
Response via : Initial Calibration

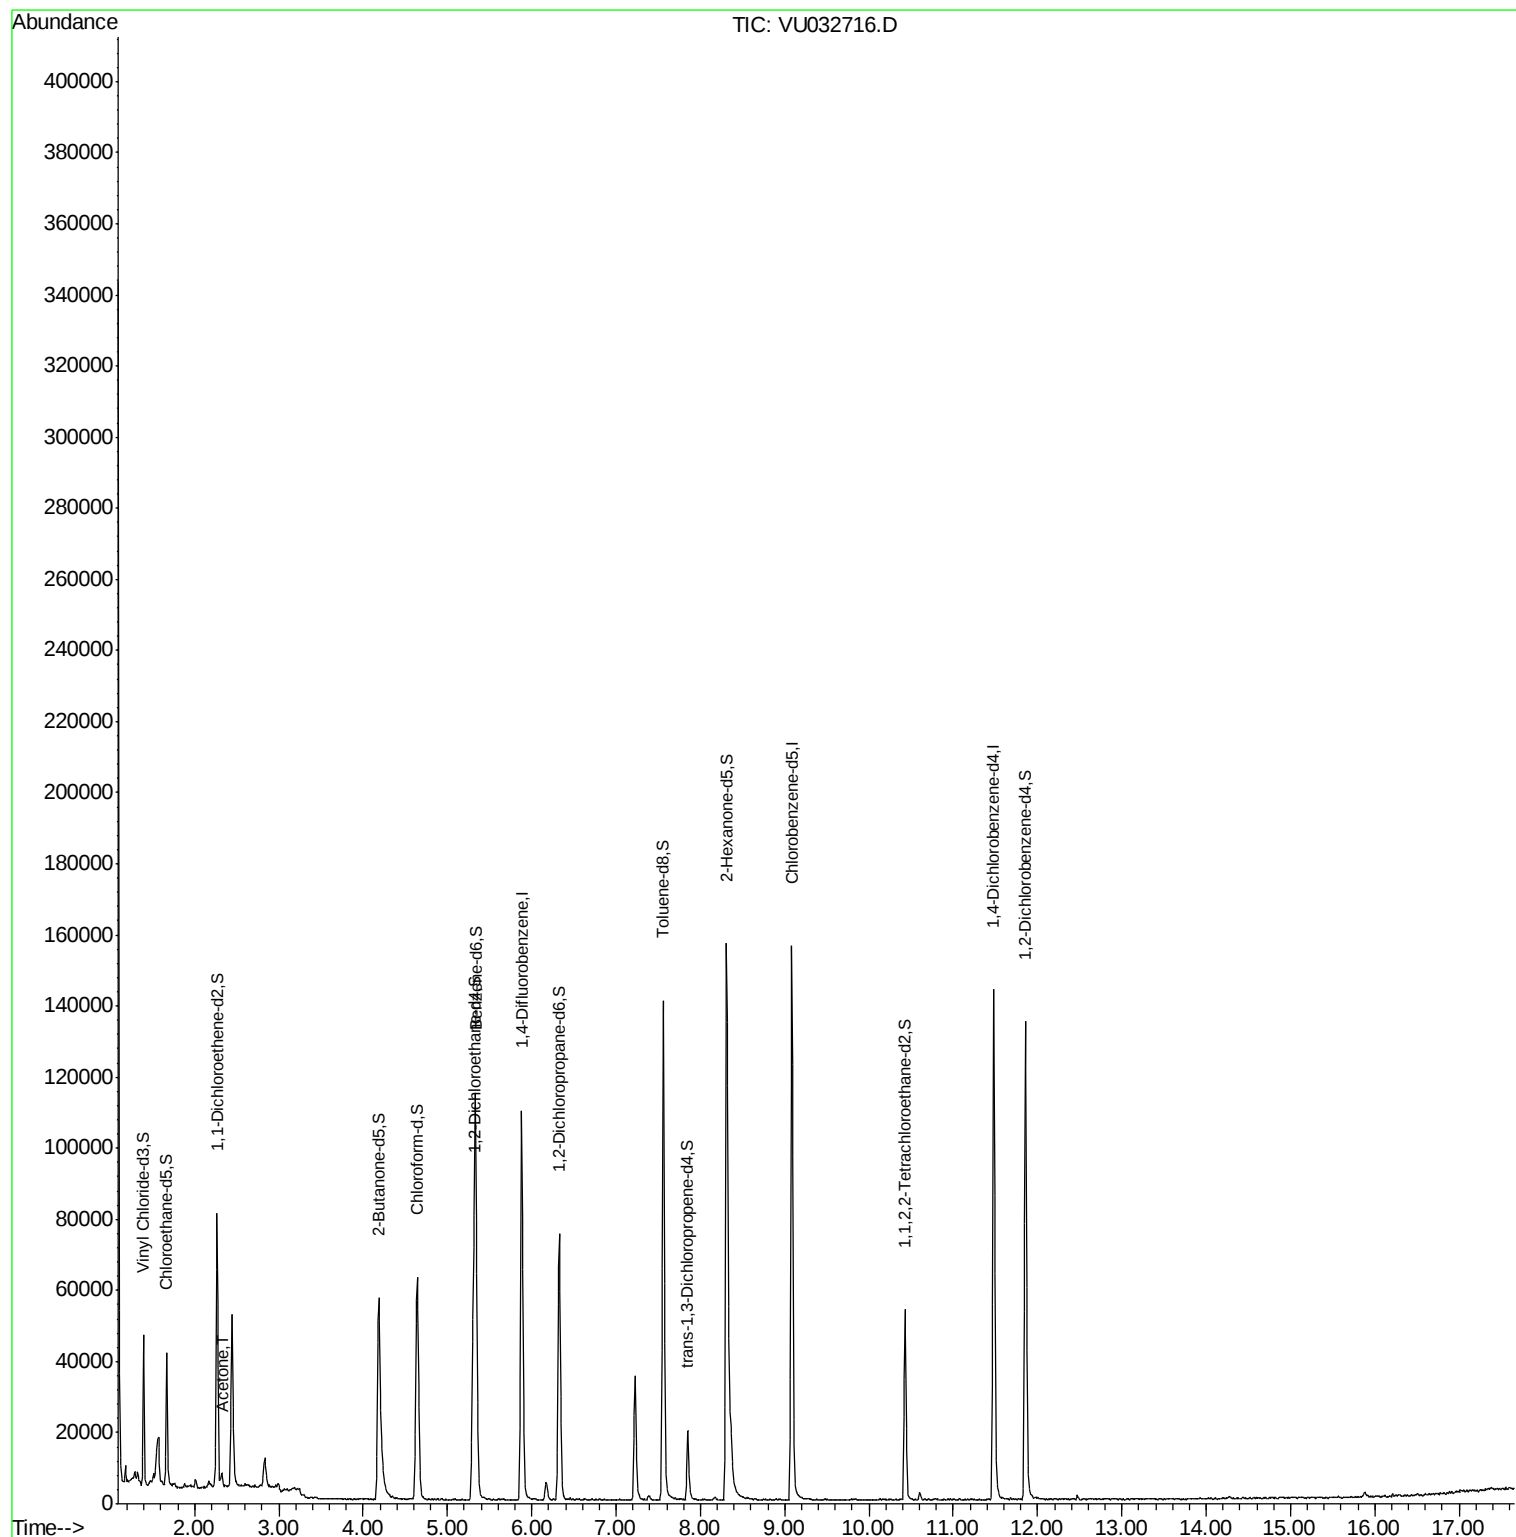

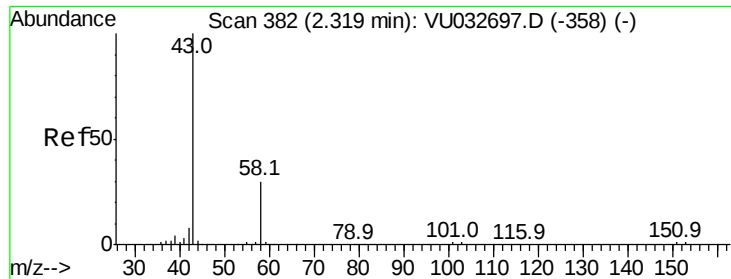

#13

Acetone

Concen: 2.468 ug/L

RT: 2.32 min Scan# 383

Delta R.T. 0.00 min

Lab File: VU032716.D

Acq: 14 Jun 2019 00:14

Instrument :

MSVOA_U

ClientSampleId :

COM37

Tot Ion: 43 Resp: 3176

Ion Ratio Lower Upper

43 100

58 27.6 0.0 60.8

