

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
 Data File : VU032732.D
 Acq On : 14 Jun 2019 19:17
 Operator : JC/SP
 Sample : K3383-09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XK8

Quant Time: Jun 15 00:27:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 14 23:49:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	102618	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	95941	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	48410	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	27882	4.18	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.60%
7) Chloroethane-d5	1.67	69	25014	4.39	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.80%
11) 1,1-Dichloroethene-d2	2.27	63	45408	3.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.00%
20) 2-Butanone-d5	4.18	46	99085	53.21	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.42%
24) Chloroform-d	4.64	84	62130	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.00%
26) 1,2-Dichloroethane-d4	5.30	65	35403	5.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.40%
32) Benzene-d6	5.33	84	116771	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	6.32	67	39055	5.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.20%
41) Toluene-d8	7.56	98	103598	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.00%
43) trans-1,3-Dichloropropene-	7.85	79	15902	5.06	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.20%
46) 2-Hexanone-d5	8.31	63	79651	50.60	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.20%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	35829	5.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	115.60%
64) 1,2-Dichlorobenzene-d4	11.85	152	44522	5.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.20%


Target Compounds					Ovalue
13) Acetone	2.32	43	7076	4.896 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032732.D
Acq On : 14 Jun 2019 19:17
Operator : JC/SP
Sample : K3383-09
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XK8

Quant Time: Jun 15 00:27:43 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 23:49:20 2019
Response via : Initial Calibration

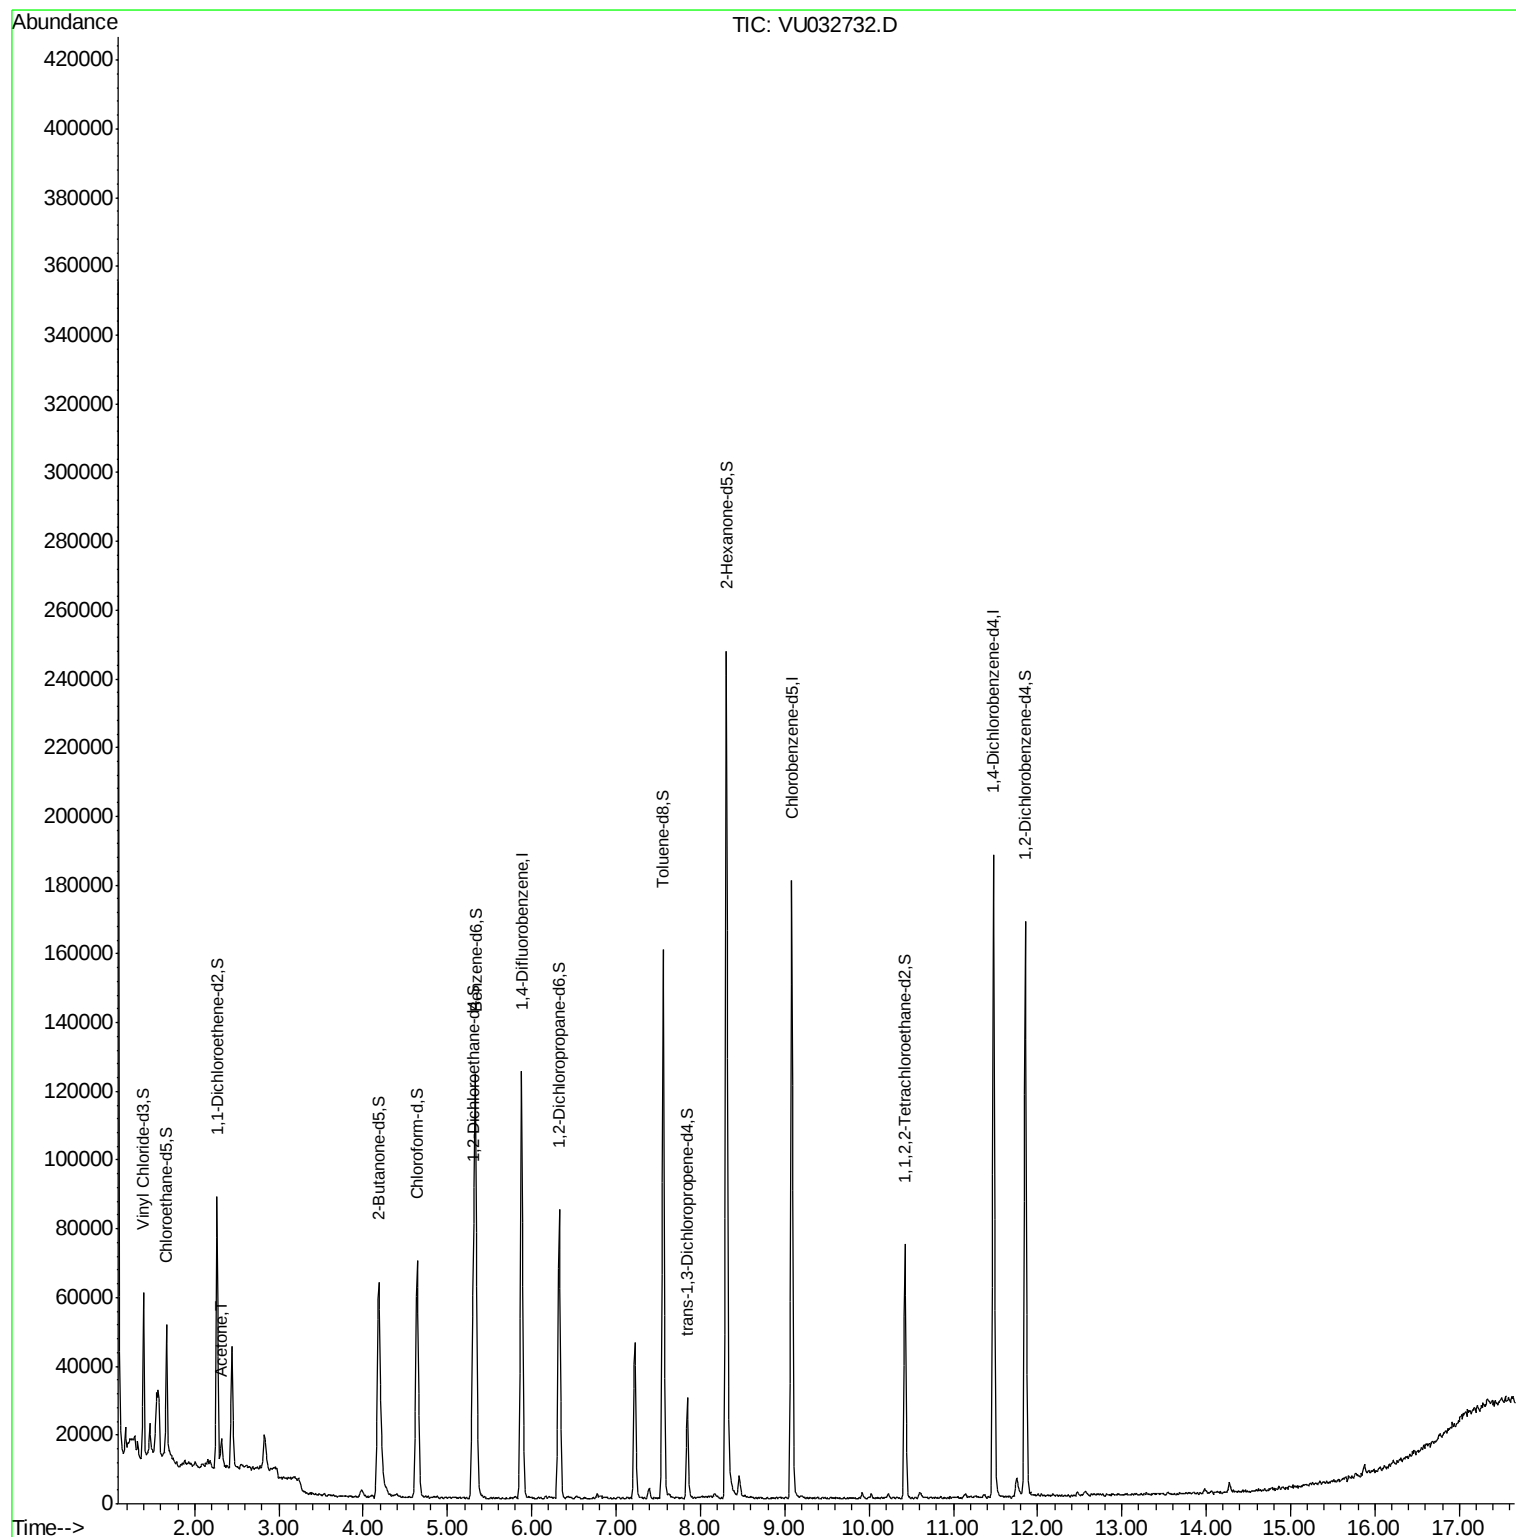

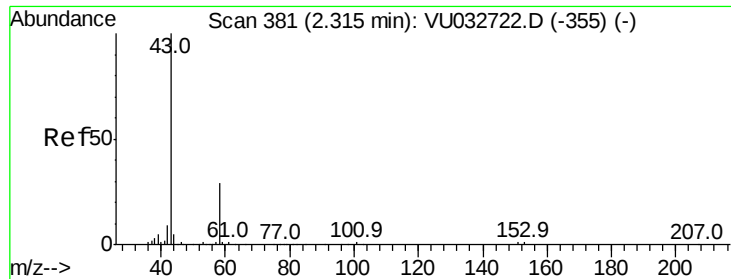

#13

Acetone

Concen: 4.896 ug/L

RT: 2.32 min Scan# 382

Delta R.T. 0.00 min

Lab File: VU032732.D

Acq: 14 Jun 2019 19:17

Instrument :
MSVOA_U
ClientSampleId :
C0XK8

Tot Ion: 43 Resp: 7076

Ion Ratio Lower Upper

43 100

58 31.2 0.0 60.8

