

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
 Data File : VU032733.D
 Acq On : 14 Jun 2019 19:42
 Operator : JC/SP
 Sample : K3365-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM56

Quant Time: Jun 15 00:30:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 14 23:49:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	99957	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	93864	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	46652	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	29216	4.50	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.00%
7) Chloroethane-d5	1.67	69	25141	4.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.60%
11) 1,1-Dichloroethene-d2	2.27	63	43754	3.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.40%
20) 2-Butanone-d5	4.18	46	101187	55.79	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.58%
24) Chloroform-d	4.64	84	61305	5.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.20%
26) 1,2-Dichloroethane-d4	5.30	65	35615	5.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	117.20%
32) Benzene-d6	5.33	84	117559	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
36) 1,2-Dichloropropane-d6	6.32	67	38906	5.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.20%
41) Toluene-d8	7.56	98	101486	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.00%
43) trans-1,3-Dichloropropene-	7.85	79	13765	4.48	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.60%
46) 2-Hexanone-d5	8.31	63	80565	52.31	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.62%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	34782	5.74	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	114.80%
64) 1,2-Dichlorobenzene-d4	11.85	152	43356	5.17	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.40%


Target Compounds					Ovalue
13) Acetone	2.32	43	4209	2.990 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032733.D
Acq On : 14 Jun 2019 19:42
Operator : JC/SP
Sample : K3365-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM56

Quant Time: Jun 15 00:30:03 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 23:49:20 2019
Response via : Initial Calibration

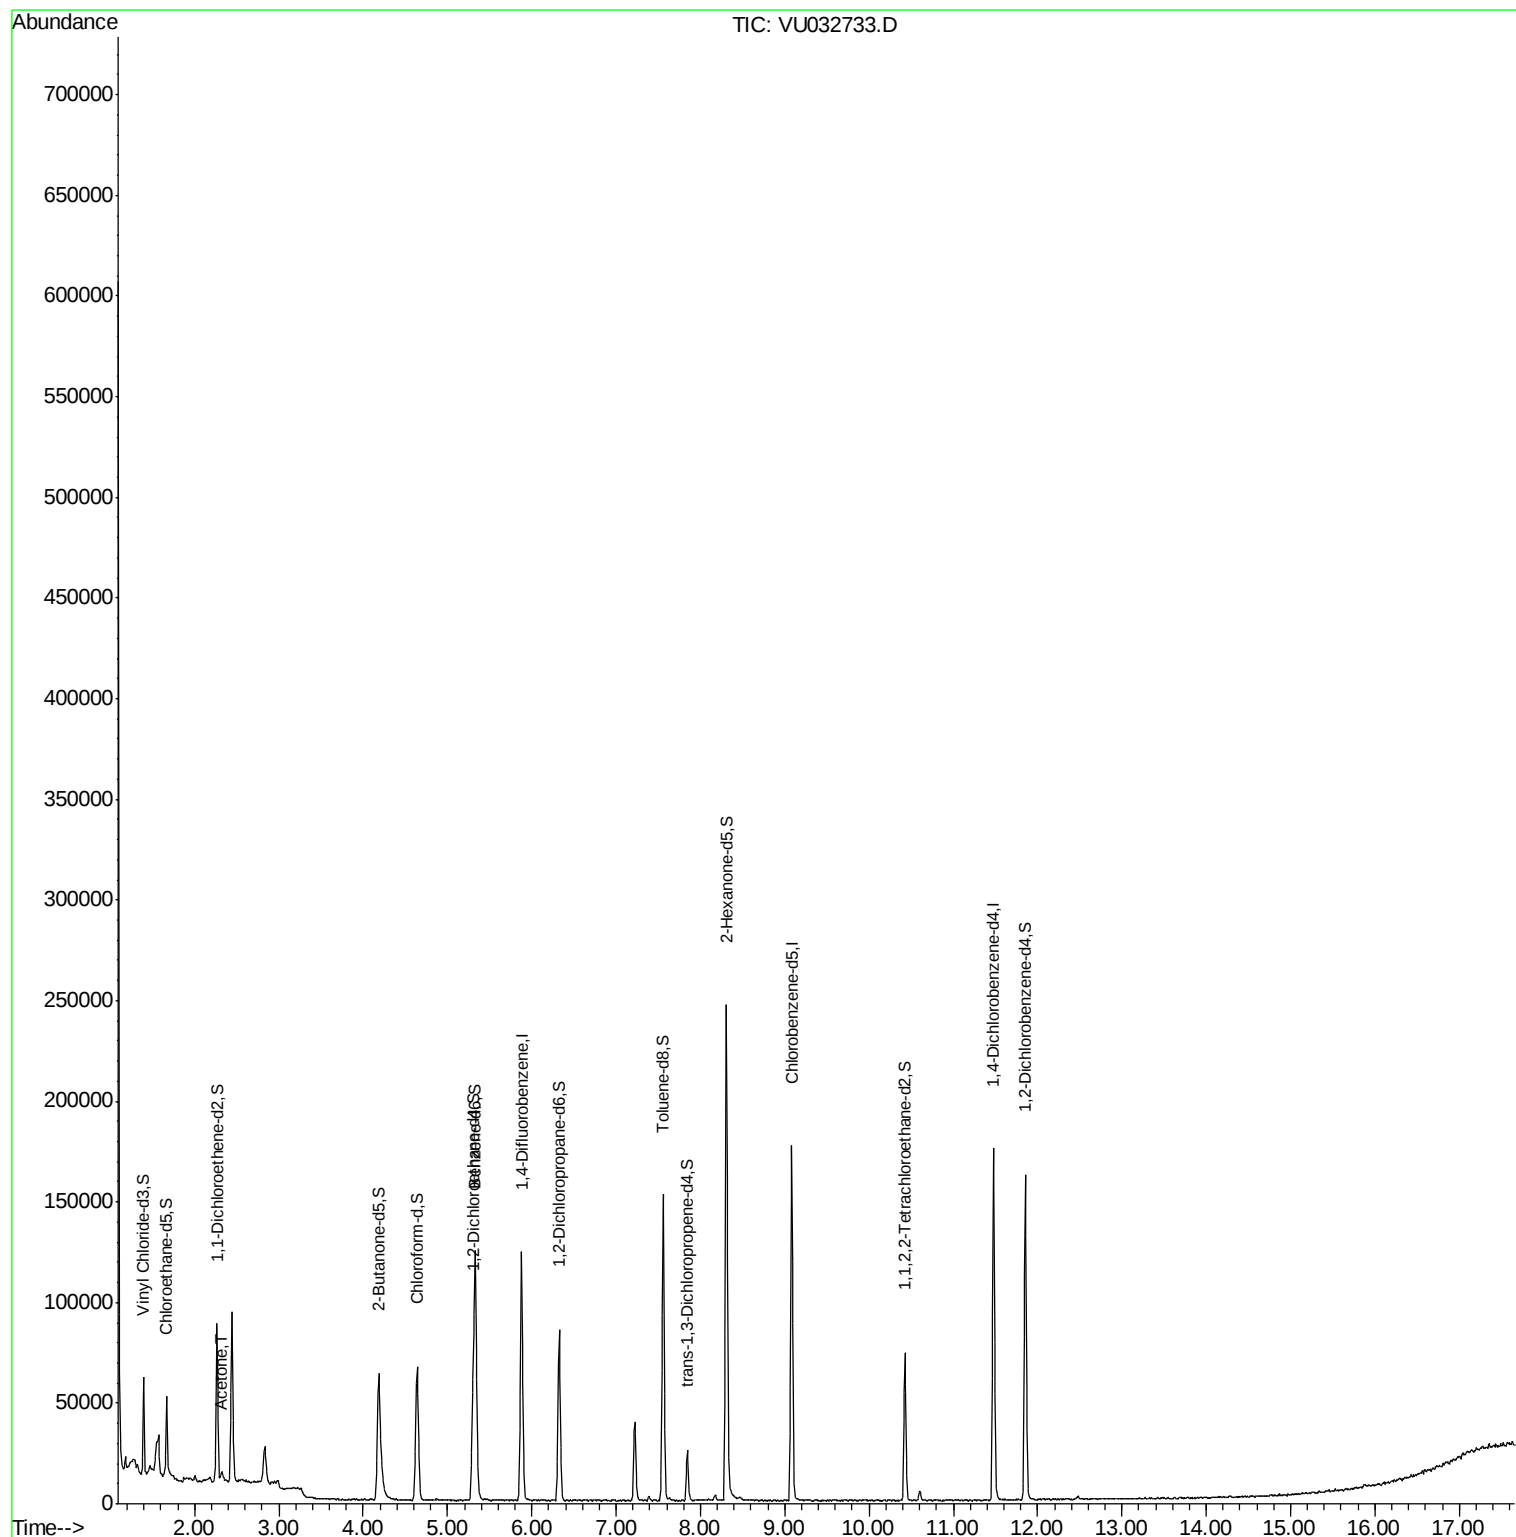

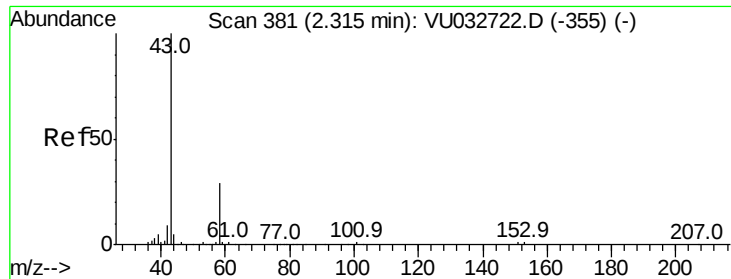

#13

Acetone

Concen: 2.990 ug/L

RT: 2.32 min Scan# 382

Delta R.T. 0.00 min

Lab File: VU032733.D

Acq: 14 Jun 2019 19:42

Instrument :
MSVOA_U
ClientSampleId :
COM56

Tot Ion: 43 Resp: 4209

Ion Ratio Lower Upper

43 100

58 26.2 0.0 60.8

