

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
 Data File : VU032739.D
 Acq On : 14 Jun 2019 22:10
 Operator : JC/SP
 Sample : K3365-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM63

Quant Time: Jun 17 09:00:22 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 14 23:49:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	104265	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	97258	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	47990	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	29860	4.40	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.00%
7) Chloroethane-d5	1.67	69	26173	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.40%
11) 1,1-Dichloroethene-d2	2.27	63	45858	3.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.60%
20) 2-Butanone-d5	4.18	46	103103	54.50	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.00%
24) Chloroform-d	4.64	84	63117	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.00%
26) 1,2-Dichloroethane-d4	5.30	65	36054	5.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.60%
32) Benzene-d6	5.33	84	120619	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.80%
36) 1,2-Dichloropropane-d6	6.32	67	40161	5.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.80%
41) Toluene-d8	7.56	98	105771	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
43) trans-1,3-Dichloropropene-	7.85	79	14106	4.43	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.60%
46) 2-Hexanone-d5	8.31	63	80293	50.32	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.64%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	35602	5.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.40%
64) 1,2-Dichlorobenzene-d4	11.85	152	44099	5.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.20%


Target Compounds					Ovalue
13) Acetone	2.32	43	4956	3.375 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032739.D
Acq On : 14 Jun 2019 22:10
Operator : JC/SP
Sample : K3365-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM63

Quant Time: Jun 17 09:00:22 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 23:49:20 2019
Response via : Initial Calibration

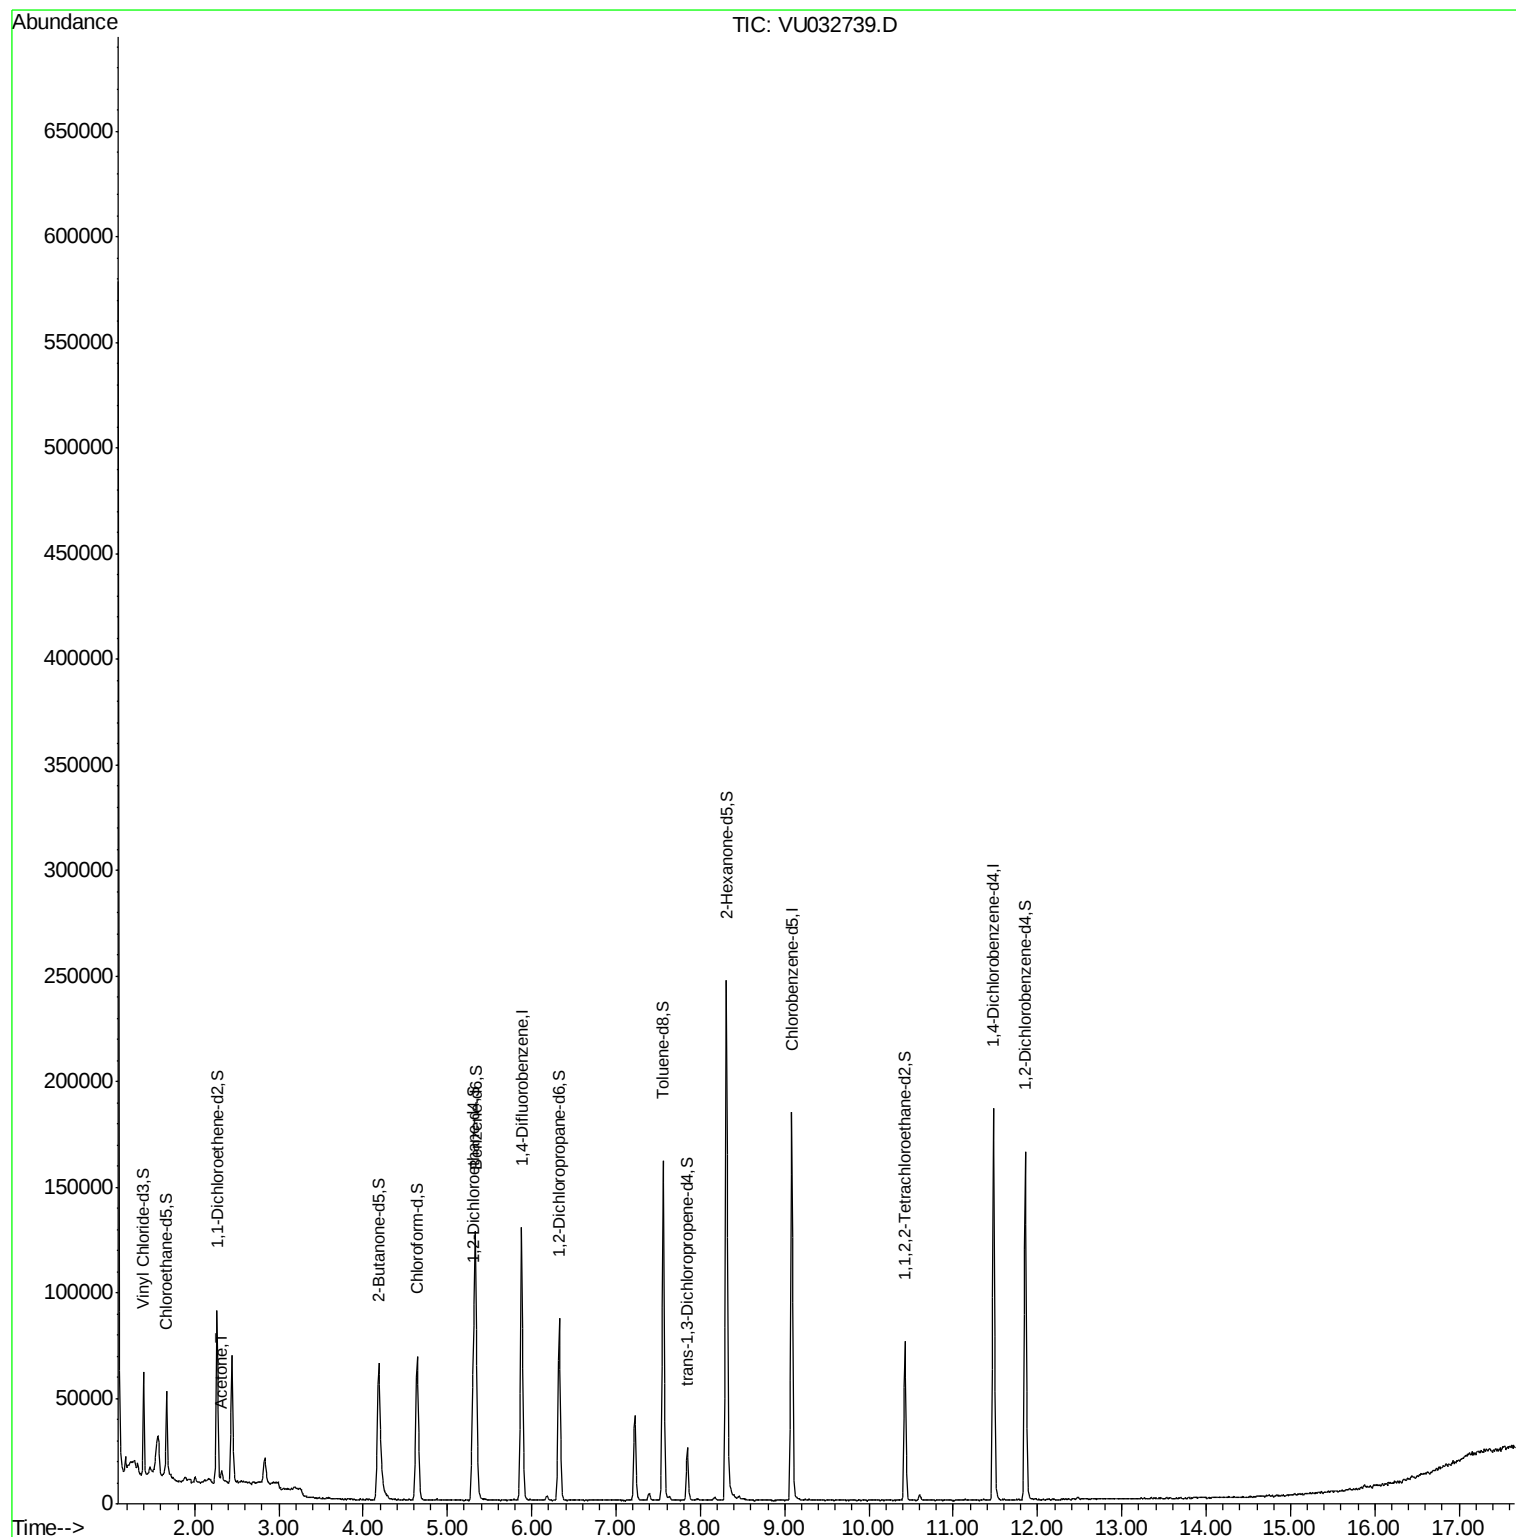

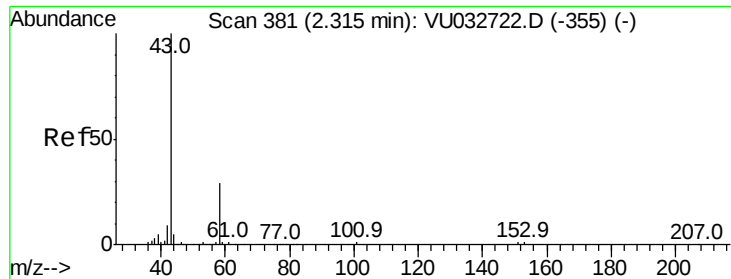

#13

Acetone

Concen: 3.375 ug/L

RT: 2.32 min Scan# 382

Delta R.T. 0.00 min

Lab File: VU032739.D

Acq: 14 Jun 2019 22:10

Instrument :

MSVOA_U

ClientSampleId :

COM63

Tot Ion: 43 Resp: 4956

Ion Ratio Lower Upper

43 100

58 24.8 0.0 60.8

