

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
 Data File : VU032741.D
 Acq On : 14 Jun 2019 23:00
 Operator : JC/SP
 Sample : K3383-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XK1

Quant Time: Jun 17 08:59:54 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 14 23:49:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	100788	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	94514	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	46808	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	28108	4.29	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.80%
7) Chloroethane-d5	1.67	69	24299	4.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.80%
11) 1,1-Dichloroethene-d2	2.27	63	42864	3.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.40%
20) 2-Butanone-d5	4.18	46	101796	55.66	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.32%
24) Chloroform-d	4.64	84	60966	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.80%
26) 1,2-Dichloroethane-d4	5.30	65	34638	5.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.00%
32) Benzene-d6	5.33	84	114311	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
36) 1,2-Dichloropropane-d6	6.32	67	38545	5.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.40%
41) Toluene-d8	7.56	98	100737	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
43) trans-1,3-Dichloropropene-	7.84	79	14721	4.76	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.20%
46) 2-Hexanone-d5	8.31	63	77461	49.95	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.90%
57) 1,1,2,2-Tetrachloroethane-	10.42	84	34965	5.73	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	114.60%
64) 1,2-Dichlorobenzene-d4	11.85	152	42519	5.05	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.00%


Target Compounds					Ovalue
13) Acetone	2.32	43	2442	1.720 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032741.D
Acq On : 14 Jun 2019 23:00
Operator : JC/SP
Sample : K3383-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XK1

Quant Time: Jun 17 08:59:54 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 23:49:20 2019
Response via : Initial Calibration

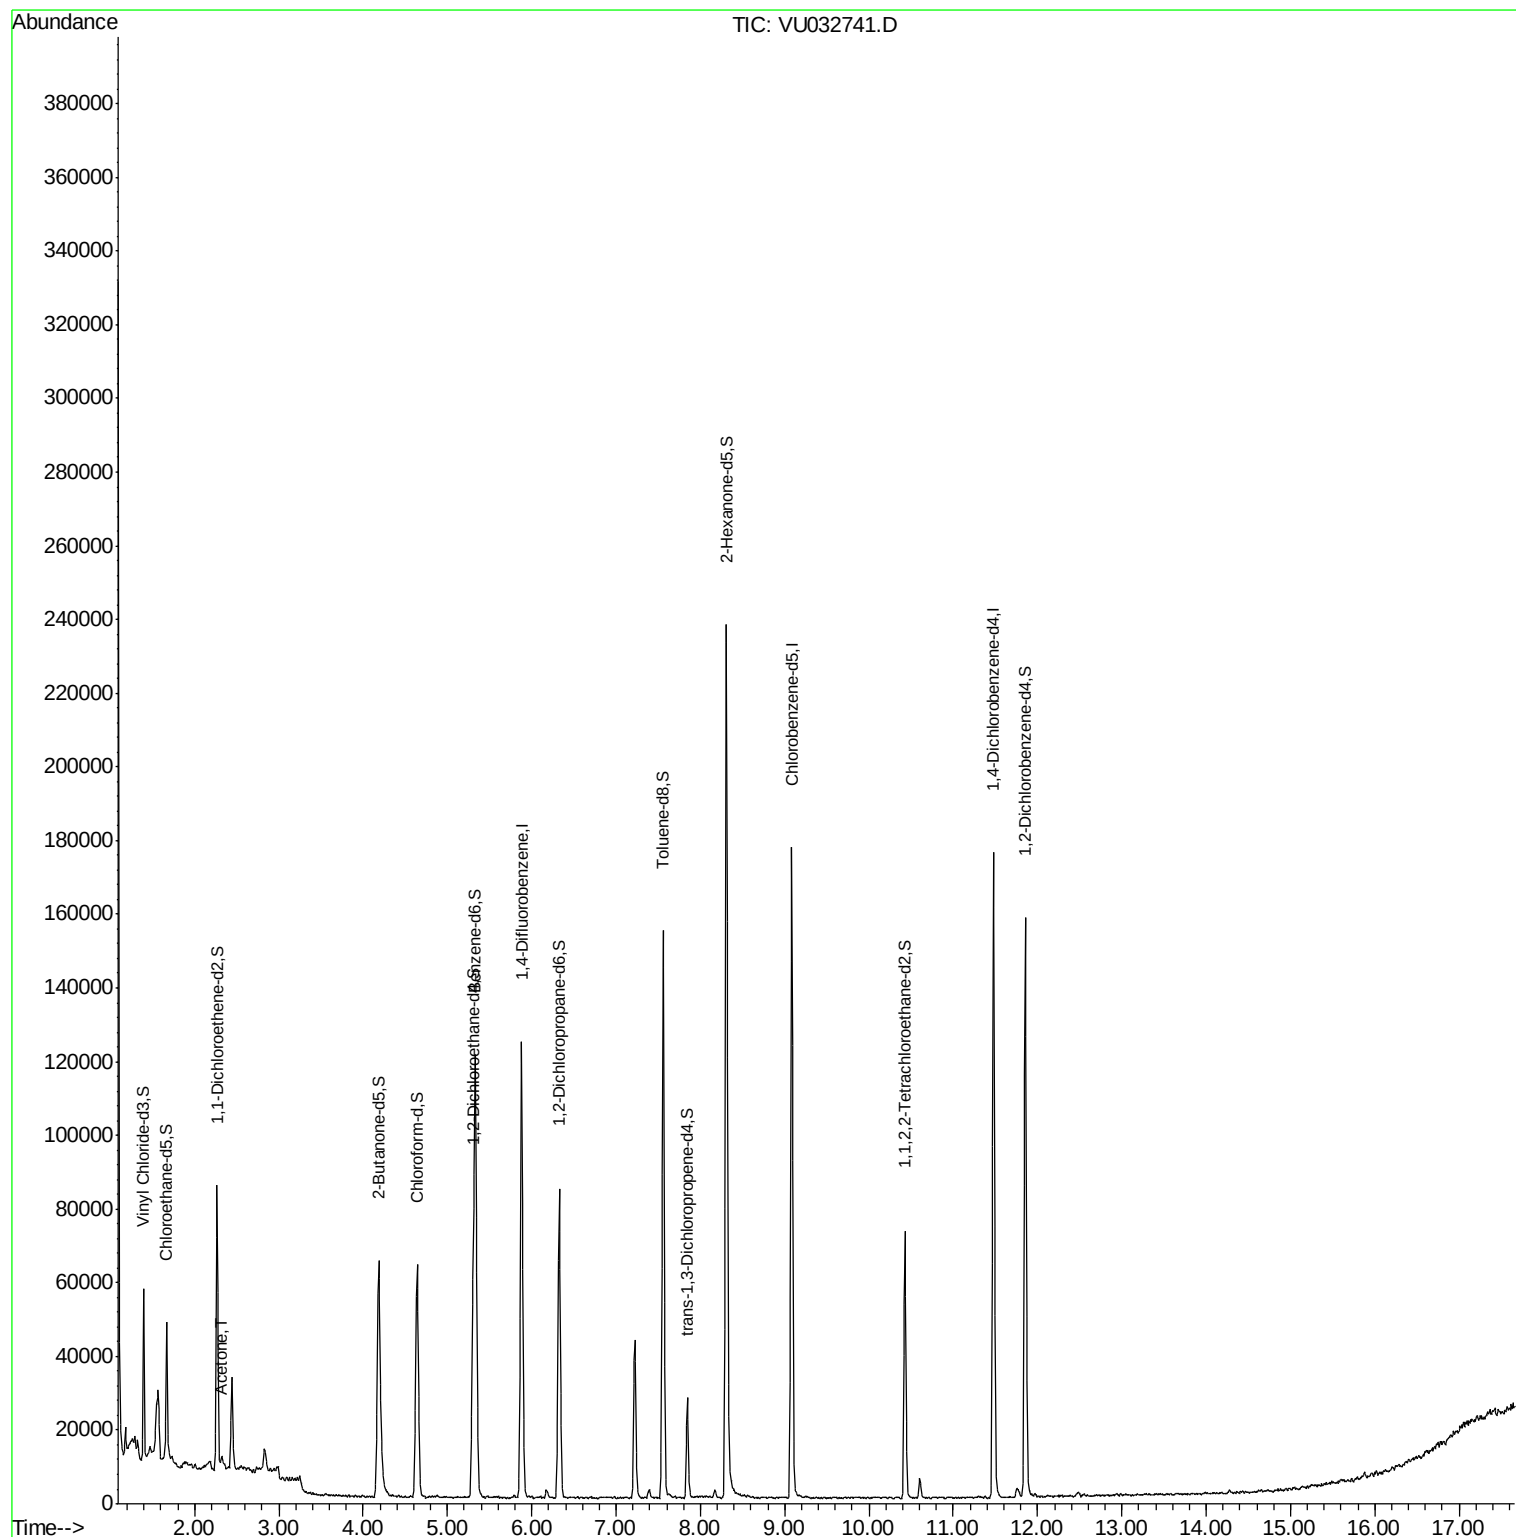

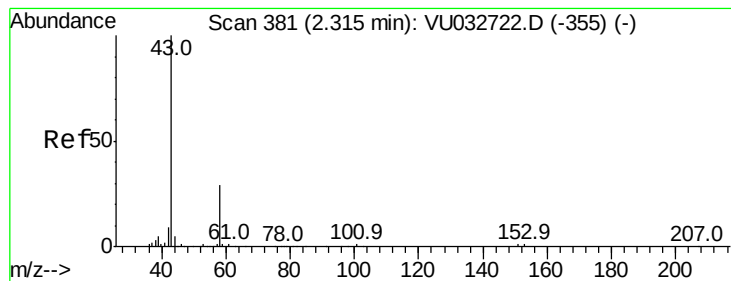

#13

Acetone

Concen: 1.720 ug/L

RT: 2.32 min Scan# 381

Delta R.T. 0.00 min

Lab File: VU032741.D

Acq: 14 Jun 2019 23:00

Instrument :
MSVOA_U
ClientSampleId :
C0XK1

Tot Ion: 43 Resp: 2442

Ion Ratio Lower Upper

43 100

58 28.9 0.0 60.8

