

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
 Data File : VU032742.D
 Acq On : 14 Jun 2019 23:24
 Operator : JC/SP
 Sample : K3383-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XK2

Quant Time: Jun 15 00:52:40 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 14 23:49:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	98420	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	92260	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	46621	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	26850	4.20	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.00%
7) Chloroethane-d5	1.67	69	24110	4.41	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.20%
11) 1,1-Dichloroethene-d2	2.27	63	42428	3.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.40%
20) 2-Butanone-d5	4.18	46	98695	55.26	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.52%
24) Chloroform-d	4.64	84	59575	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.00%
26) 1,2-Dichloroethane-d4	5.30	65	34510	5.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.20%
32) Benzene-d6	5.33	84	111563	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
36) 1,2-Dichloropropane-d6	6.32	67	37168	5.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.20%
41) Toluene-d8	7.56	98	99218	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.60%
43) trans-1,3-Dichloropropene-	7.84	79	14745	4.88	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.60%
46) 2-Hexanone-d5	8.31	63	75744	50.04	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.08%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	34647	5.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	116.20%
64) 1,2-Dichlorobenzene-d4	11.85	152	41753	4.98	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.60%


Target Compounds					Ovalue
13) Acetone	2.32	43	2168	1.564 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032742.D
Acq On : 14 Jun 2019 23:24
Operator : JC/SP
Sample : K3383-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XK2

Quant Time: Jun 15 00:52:40 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 23:49:20 2019
Response via : Initial Calibration

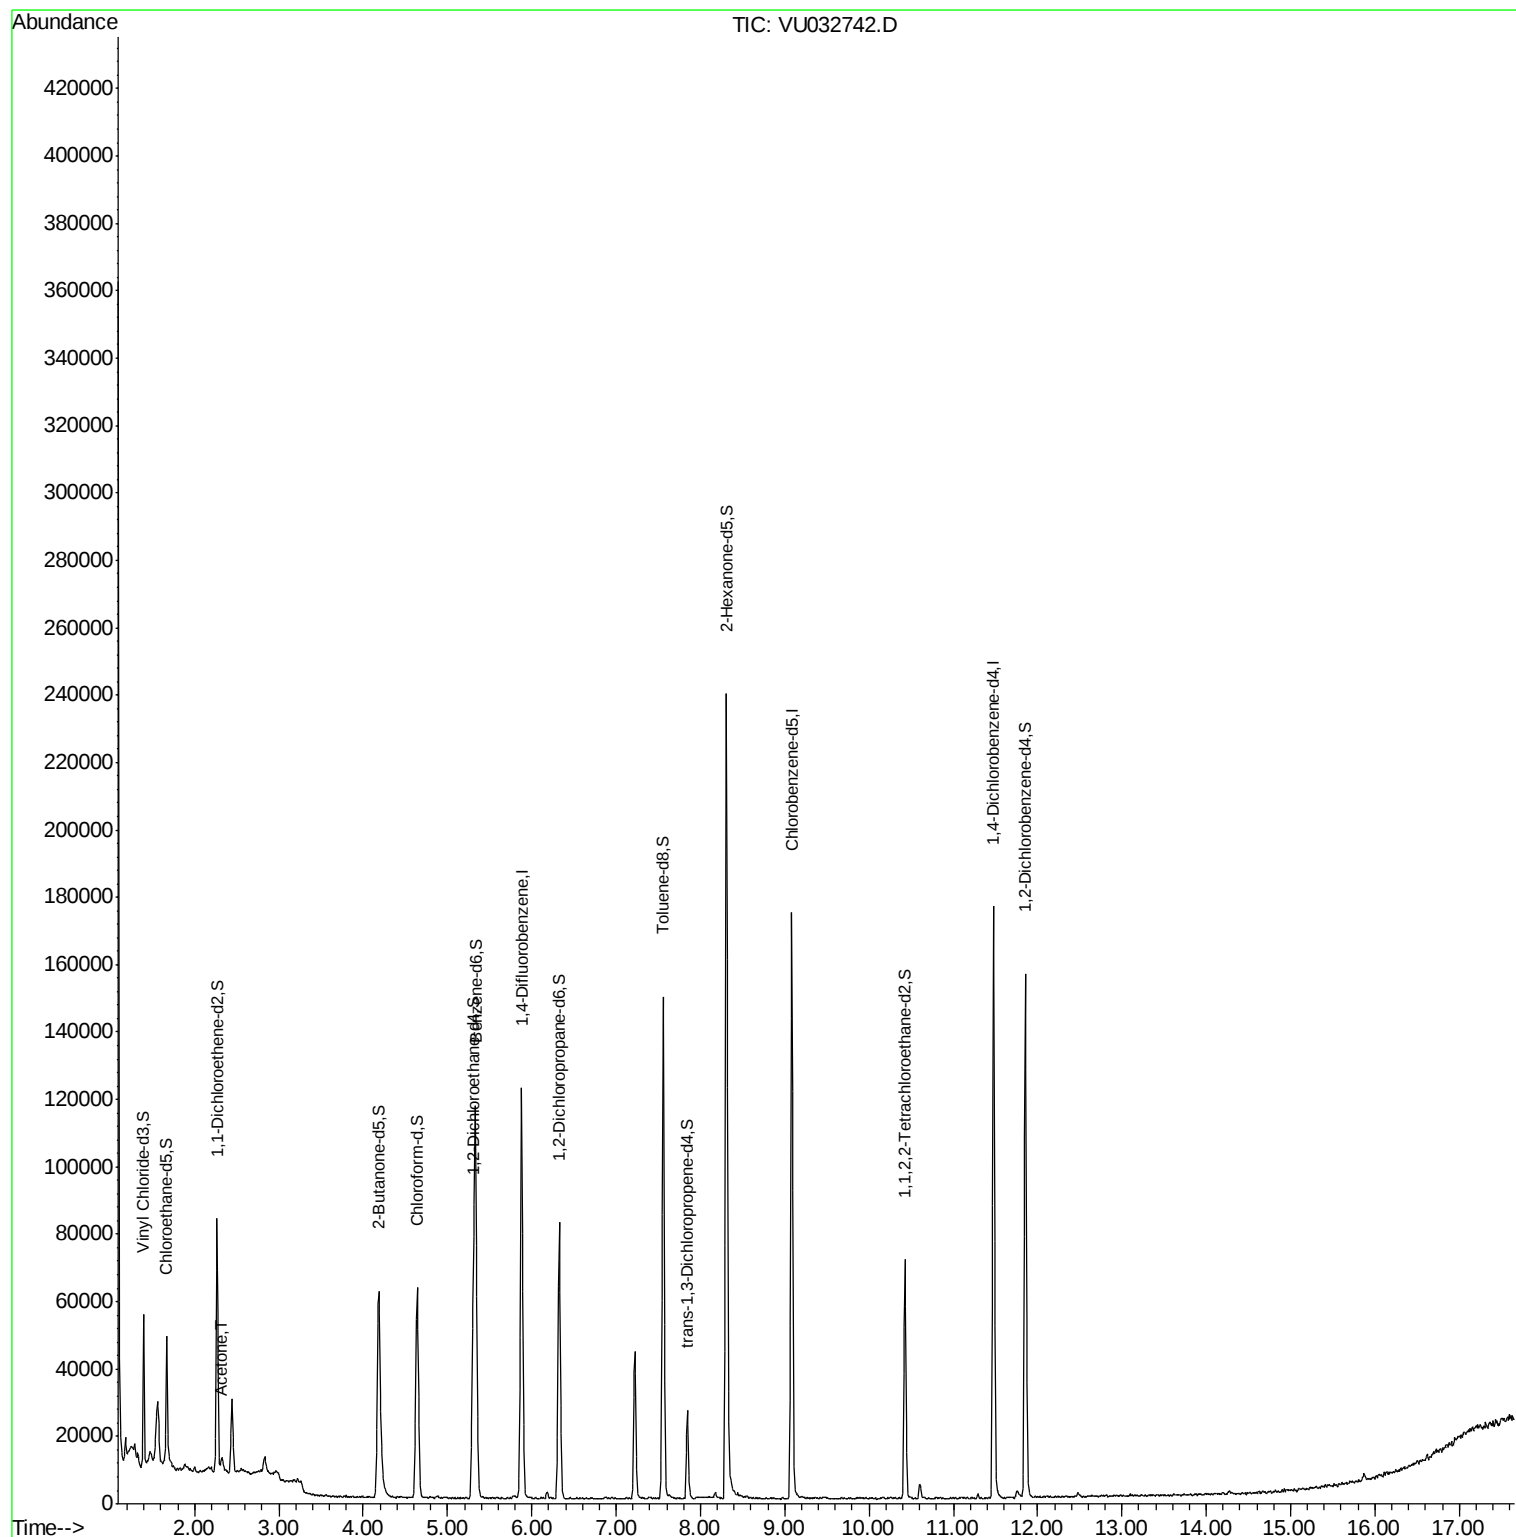

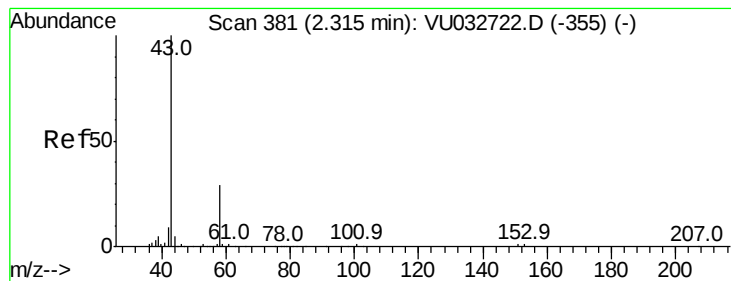

#13
 Acetone
 Concen: 1.564 ug/L
 RT: 2.32 min Scan# 382
 Delta R.T. 0.00 min
 Lab File: VU032742.D
 Acq: 14 Jun 2019 23:24

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XK2

Tot Ion: 43 Resp: 2168
 Ion Ratio Lower Upper
 43 100
 58 29.1 0.0 60.8

