

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
 Data File : VU032752.D
 Acq On : 15 Jun 2019 04:21
 Operator : JC/SP
 Sample : K3385-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM71

Quant Time: Jun 17 15:17:47 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 15 05:04:04 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	98695	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	92134	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	45674	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	25904	4.04	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.80%
7) Chloroethane-d5	1.67	69	24527	4.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.40%
11) 1,1-Dichloroethene-d2	2.26	63	42491	3.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.20%
20) 2-Butanone-d5	4.18	46	100804	56.29	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.58%
24) Chloroform-d	4.64	84	59818	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.00%
26) 1,2-Dichloroethane-d4	5.30	65	34400	5.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.60%
32) Benzene-d6	5.33	84	111662	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
36) 1,2-Dichloropropane-d6	6.32	67	36954	5.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.80%
41) Toluene-d8	7.56	98	96768	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
43) trans-1,3-Dichloropropene-	7.84	79	13754	4.56	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.20%
46) 2-Hexanone-d5	8.31	63	77574	51.32	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.64%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	33991	5.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	114.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	40874	4.98	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.60%


Target Compounds					Ovalue
13) Acetone	2.32	43	3222	2.318 ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032752.D
Acq On : 15 Jun 2019 04:21
Operator : JC/SP
Sample : K3385-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM71

Quant Time: Jun 17 15:17:47 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 15 05:04:04 2019
Response via : Initial Calibration

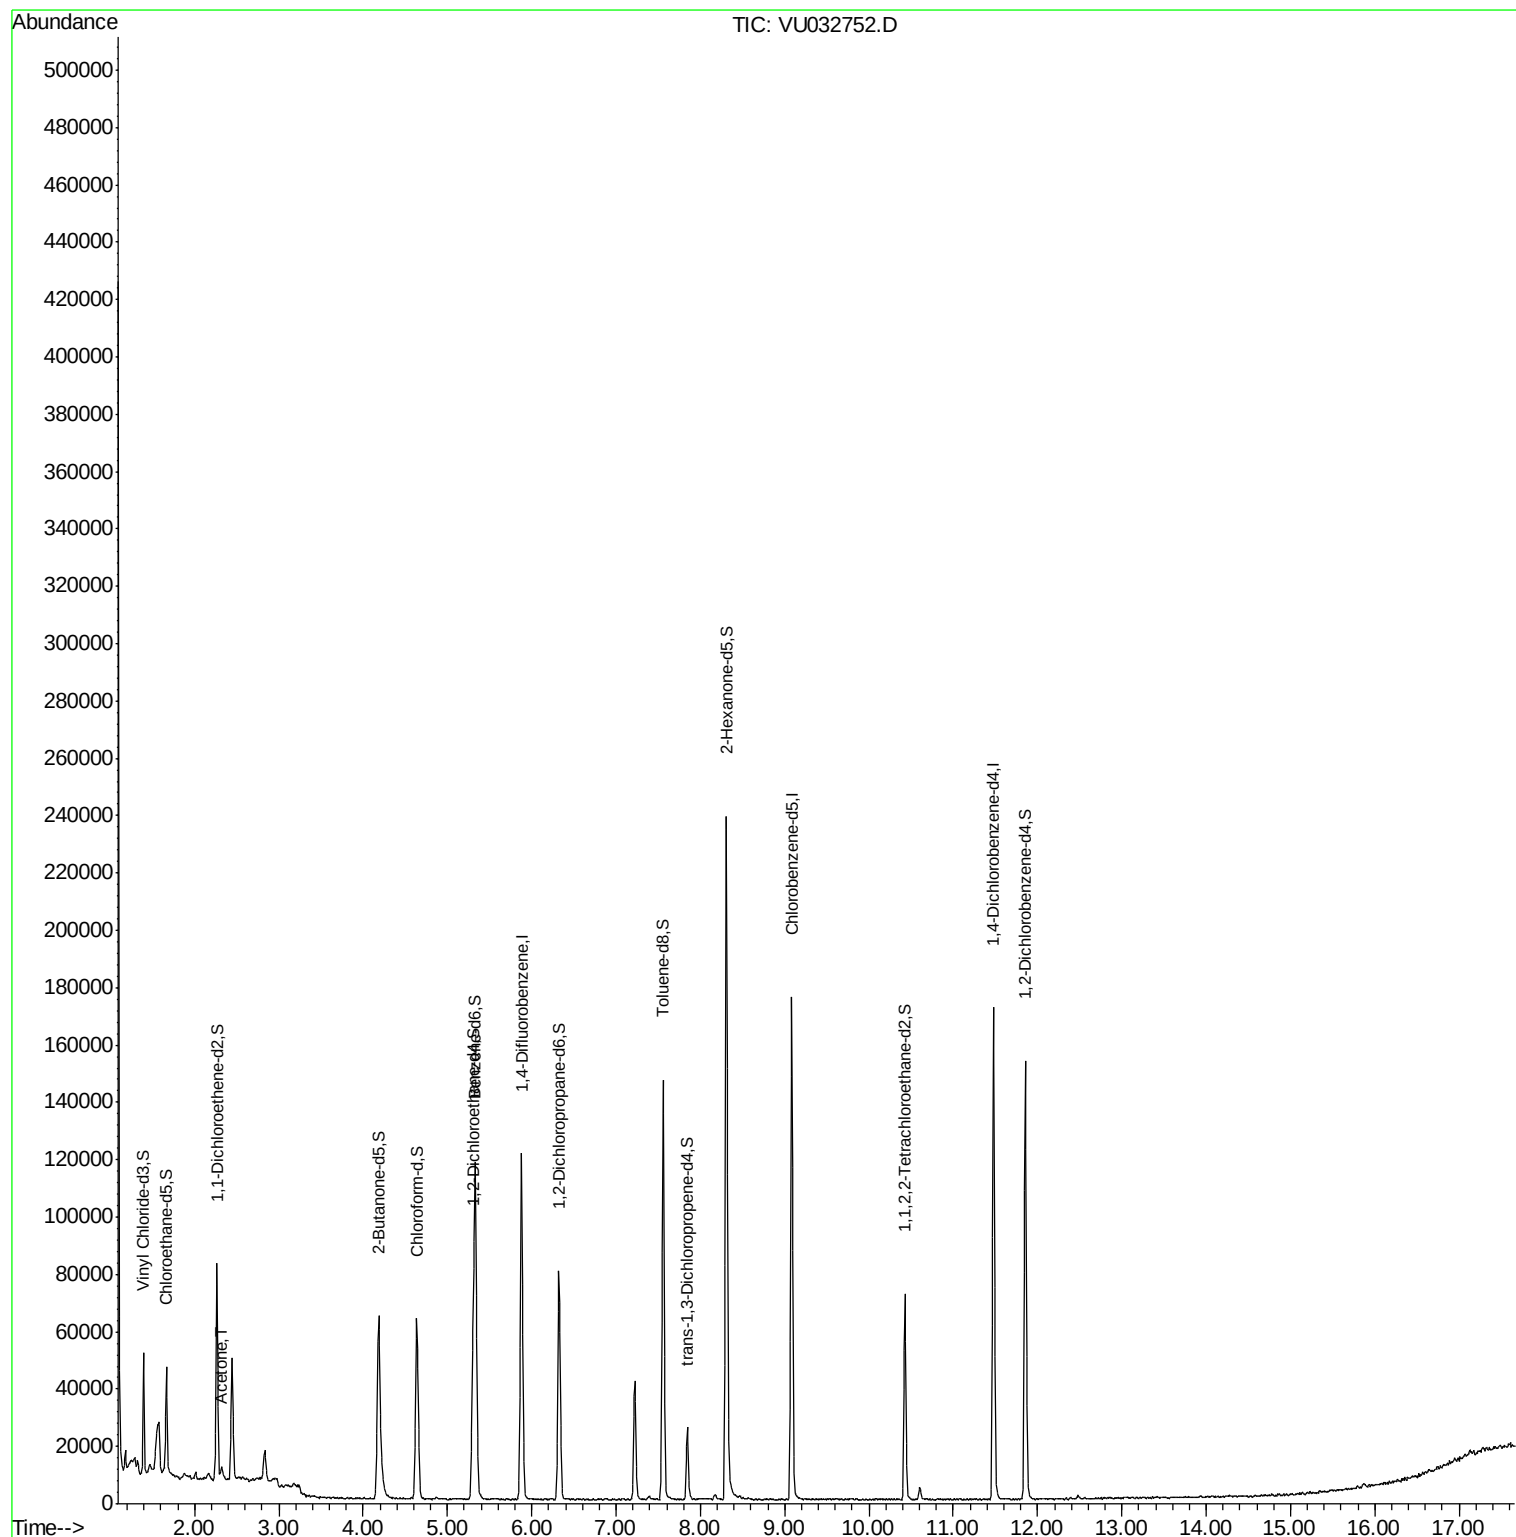

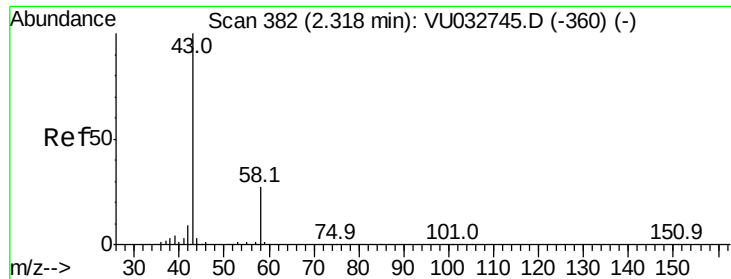

#13

Acetone

Concen: 2.318 ug/L

RT: 2.32 min Scan# 382

Delta R.T. 0.00 min

Lab File: VU032752.D

Acq: 15 Jun 2019 04:21

Instrument :
MSVOA_U
ClientSampleId :
COM71

Tot Ion: 43 Resp: 3222

Ion Ratio Lower Upper

43 100

58 23.3 0.0 60.8

