

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
 Data File : VU032754.D
 Acq On : 15 Jun 2019 05:11
 Operator : JC/SP
 Sample : K3385-05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM75

Quant Time: Jun 15 06:44:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 15 06:39:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	95888	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	90898	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	45363	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	26376	4.23	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.60%
7) Chloroethane-d5	1.67	69	23187	4.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.00%
11) 1,1-Dichloroethene-d2	2.27	63	41904	3.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.20%
20) 2-Butanone-d5	4.18	46	102552	58.94	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.88%
24) Chloroform-d	4.64	84	58692	5.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.00%
26) 1,2-Dichloroethane-d4	5.30	65	34691	5.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	119.00%
32) Benzene-d6	5.33	84	112175	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
36) 1,2-Dichloropropane-d6	6.32	67	38055	5.47	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.40%
41) Toluene-d8	7.56	98	96578	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
43) trans-1,3-Dichloropropene-	7.85	79	14184	4.77	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.40%
46) 2-Hexanone-d5	8.31	63	78292	52.50	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.00%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	34002	5.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	115.80%
64) 1,2-Dichlorobenzene-d4	11.85	152	40794	5.00	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.00%


Target Compounds					Ovalue
13) Acetone	2.32	43	3682	2.727 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032754.D
Acq On : 15 Jun 2019 05:11
Operator : JC/SP
Sample : K3385-05
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM75

Quant Time: Jun 15 06:44:09 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 15 06:39:33 2019
Response via : Initial Calibration

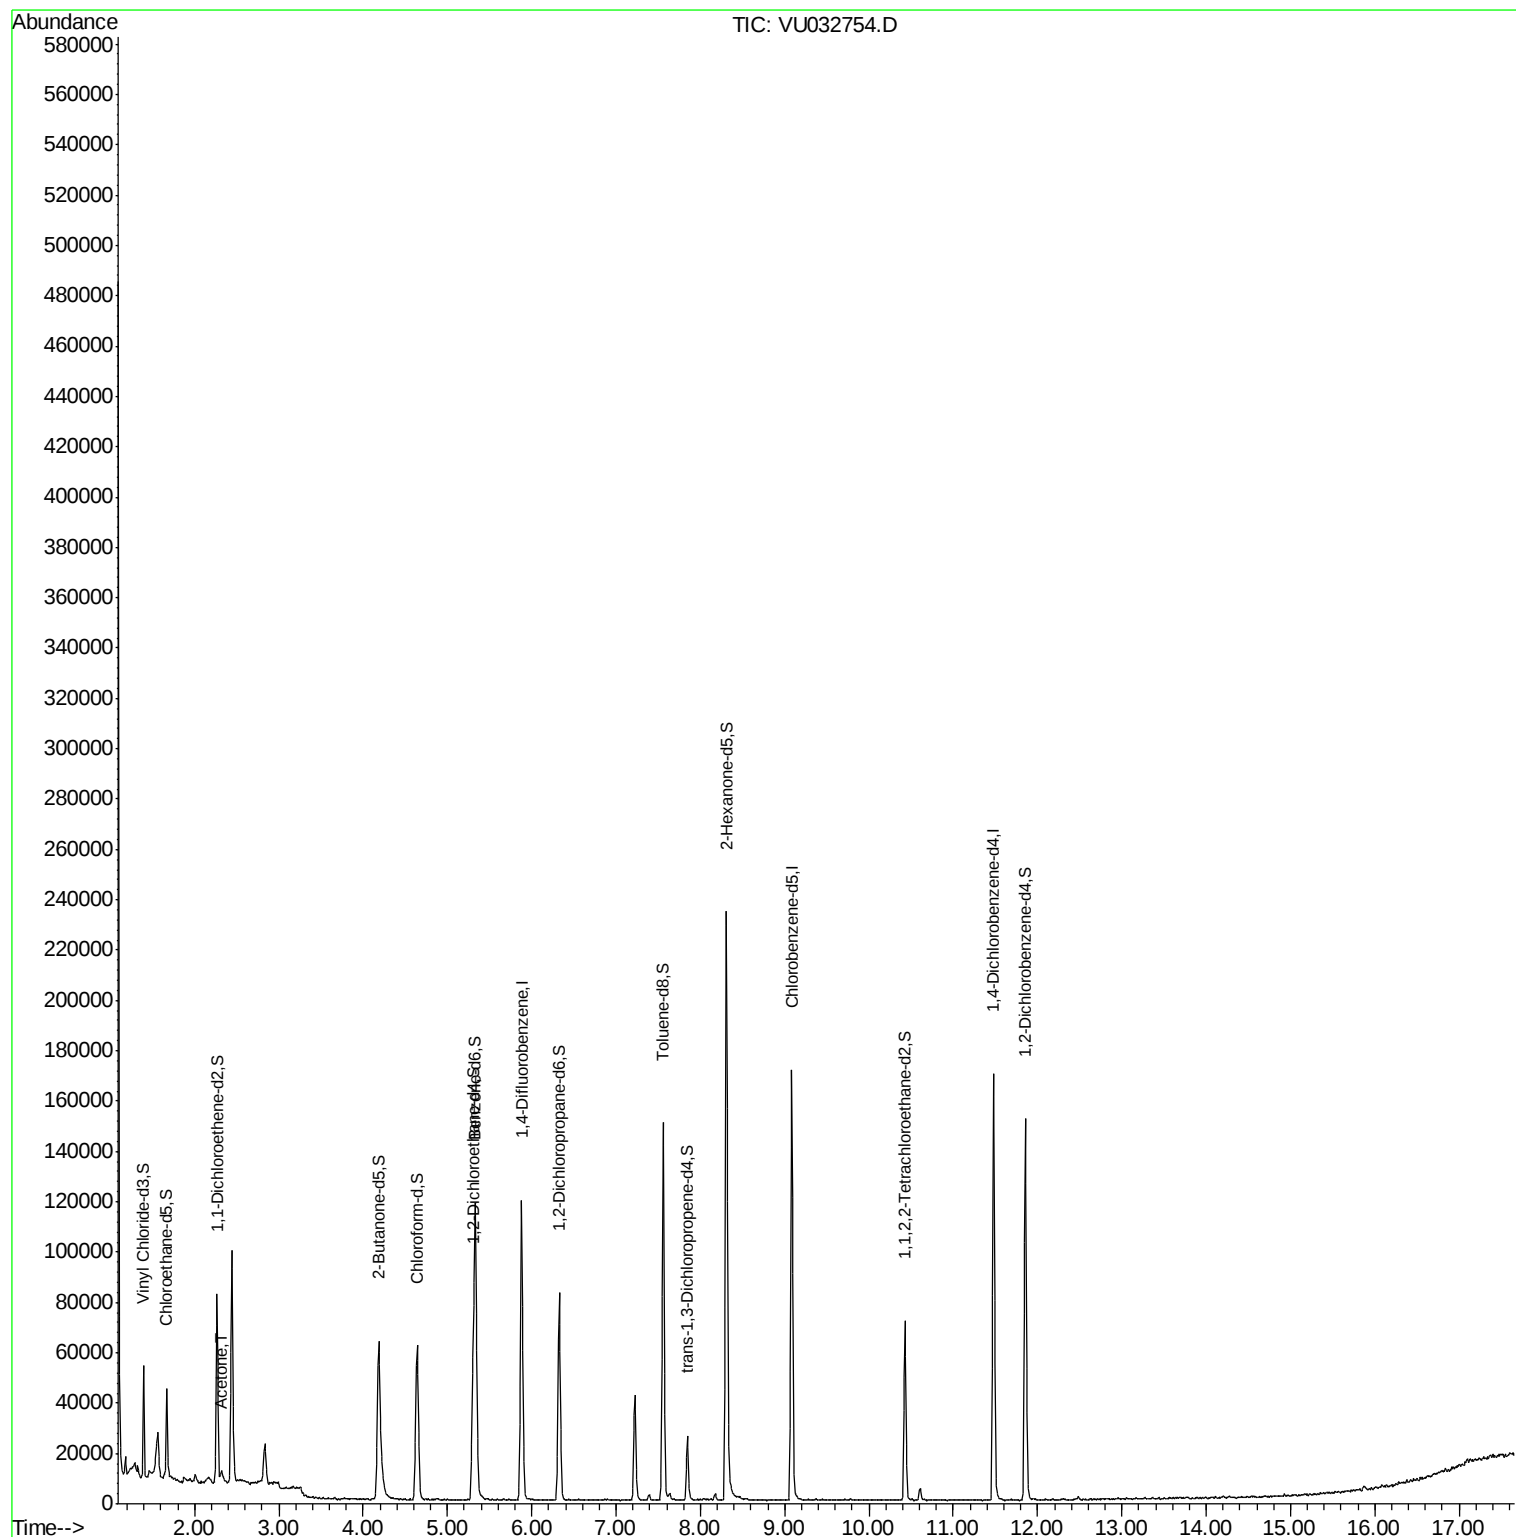

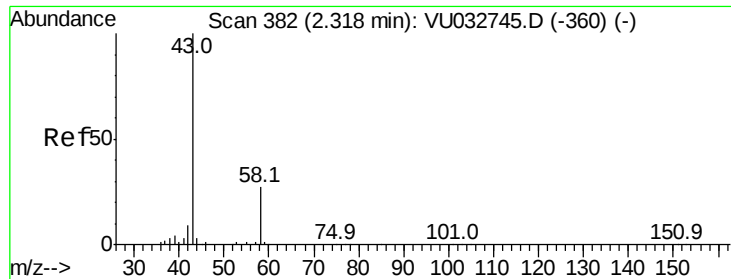

#13

Acetone

Concen: 2.727 ug/L

RT: 2.32 min Scan# 382

Delta R.T. -0.00 min

Lab File: VU032754.D

Acq: 15 Jun 2019 05:11

Instrument :

MSVOA_U

ClientSampleId :

COM75

Tot Ion: 43 Resp: 3682

Ion Ratio Lower Upper

43 100

58 30.2 0.0 60.8

