

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
 Data File : VU032761.D
 Acq On : 15 Jun 2019 08:04
 Operator : JC/SP
 Sample : K3385-12
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM98

Quant Time: Jun 17 15:21:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 17 01:26:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	94269	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	89838	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	43852	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	25937	4.23	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.60%
7) Chloroethane-d5	1.67	69	23944	4.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.40%
11) 1,1-Dichloroethene-d2	2.27	63	40890	3.29	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.80%
20) 2-Butanone-d5	4.18	46	99220	58.01	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.02%
24) Chloroform-d	4.64	84	59196	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.80%
26) 1,2-Dichloroethane-d4	5.30	65	33379	5.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	116.40%
32) Benzene-d6	5.33	84	107795	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
36) 1,2-Dichloropropane-d6	6.32	67	36388	5.29	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.80%
41) Toluene-d8	7.56	98	94645	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
43) trans-1,3-Dichloropropene-	7.85	79	13777	4.68	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.60%
46) 2-Hexanone-d5	8.31	63	76175	51.68	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.36%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	33106	5.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	114.20%
64) 1,2-Dichlorobenzene-d4	11.85	152	38972	4.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.80%


Target Compounds					Ovalue
13) Acetone	2.32	43	4597	3.463 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032761.D
Acq On : 15 Jun 2019 08:04
Operator : JC/SP
Sample : K3385-12
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM98

Quant Time: Jun 17 15:21:10 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 17 01:26:50 2019
Response via : Initial Calibration

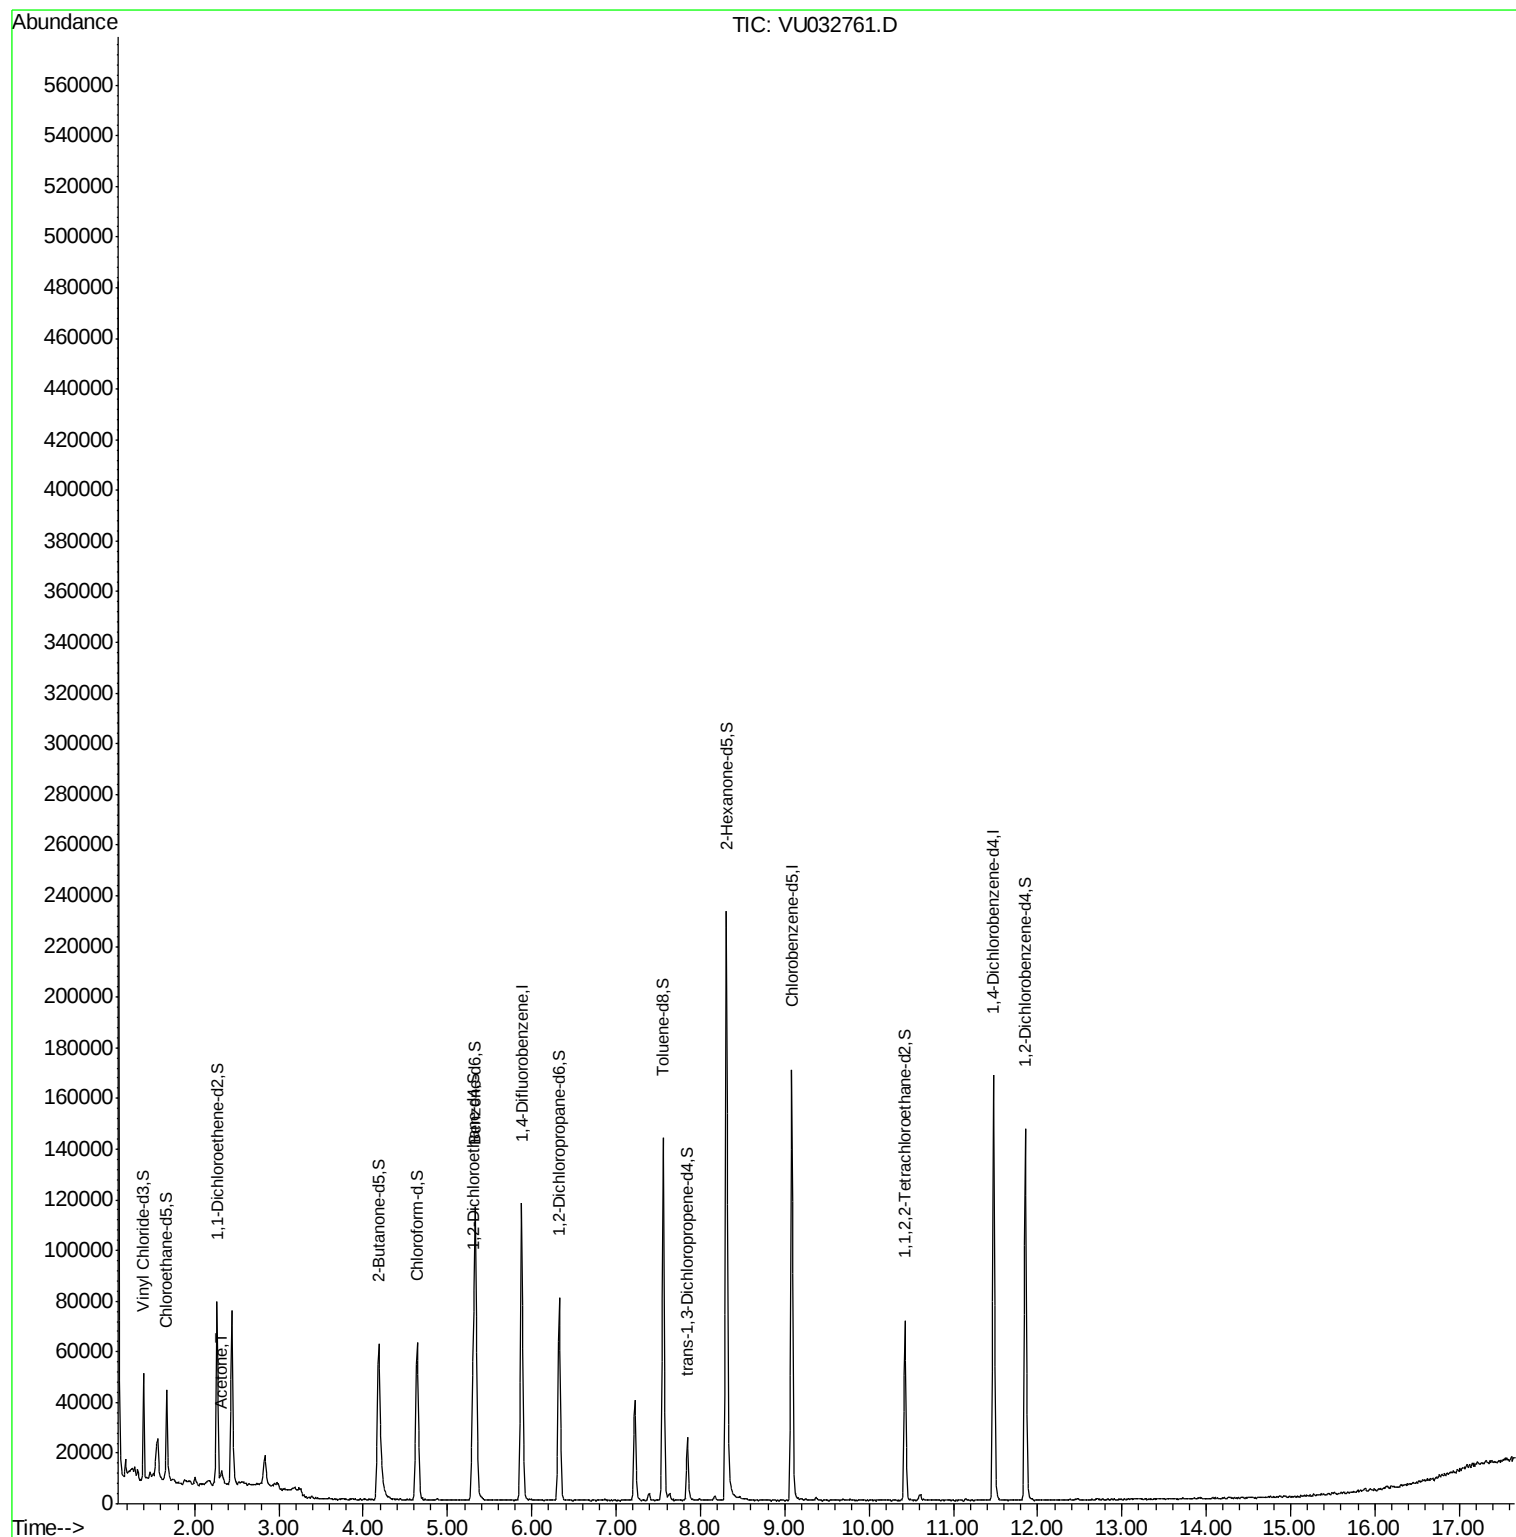

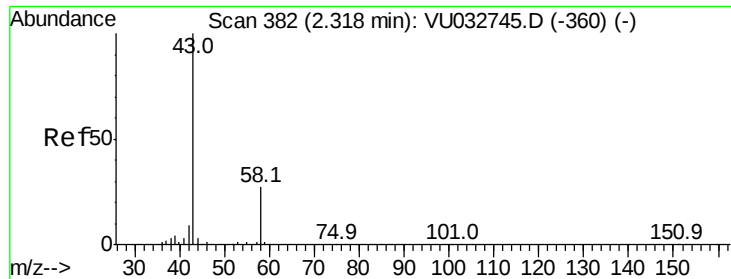

#13

Acetone

Concen: 3.463 ug/L

RT: 2.32 min Scan# 381

Delta R.T. -0.00 min

Lab File: VU032761.D

Acq: 15 Jun 2019 08:04

Instrument :
MSVOA_U
ClientSampleId :
COM98

Tot Ion: 43 Resp: 4597

Ion Ratio Lower Upper

43 100

58 26.5 0.0 60.8

