

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
 Data File : VU032764.D
 Acq On : 15 Jun 2019 09:18
 Operator : JC/SP
 Sample : K3385-15
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMA6

Quant Time: Jun 17 15:23:18 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 17 01:26:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	92336	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	89801	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	42139	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	25340	4.22	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.40%
7) Chloroethane-d5	1.67	69	23134	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.20%
11) 1,1-Dichloroethene-d2	2.27	63	39824	3.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.40%
20) 2-Butanone-d5	4.18	46	101791	60.75	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	121.50%
24) Chloroform-d	4.64	84	58339	5.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.40%
26) 1,2-Dichloroethane-d4	5.30	65	34042	6.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	121.20%
32) Benzene-d6	5.33	84	108314	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.00%
36) 1,2-Dichloropropane-d6	6.32	67	35308	5.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.60%
41) Toluene-d8	7.56	98	91588	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.80%
43) trans-1,3-Dichloropropene-	7.85	79	13417	4.56	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.20%
46) 2-Hexanone-d5	8.31	63	75621	51.32	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.64%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	33005	5.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.80%
64) 1,2-Dichlorobenzene-d4	11.85	152	38817	5.12	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.40%


Target Compounds					Ovalue
13) Acetone	2.32	43	3844	2.956 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032764.D
Acq On : 15 Jun 2019 09:18
Operator : JC/SP
Sample : K3385-15
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MA6

Quant Time: Jun 17 15:23:18 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 17 01:26:50 2019
Response via : Initial Calibration

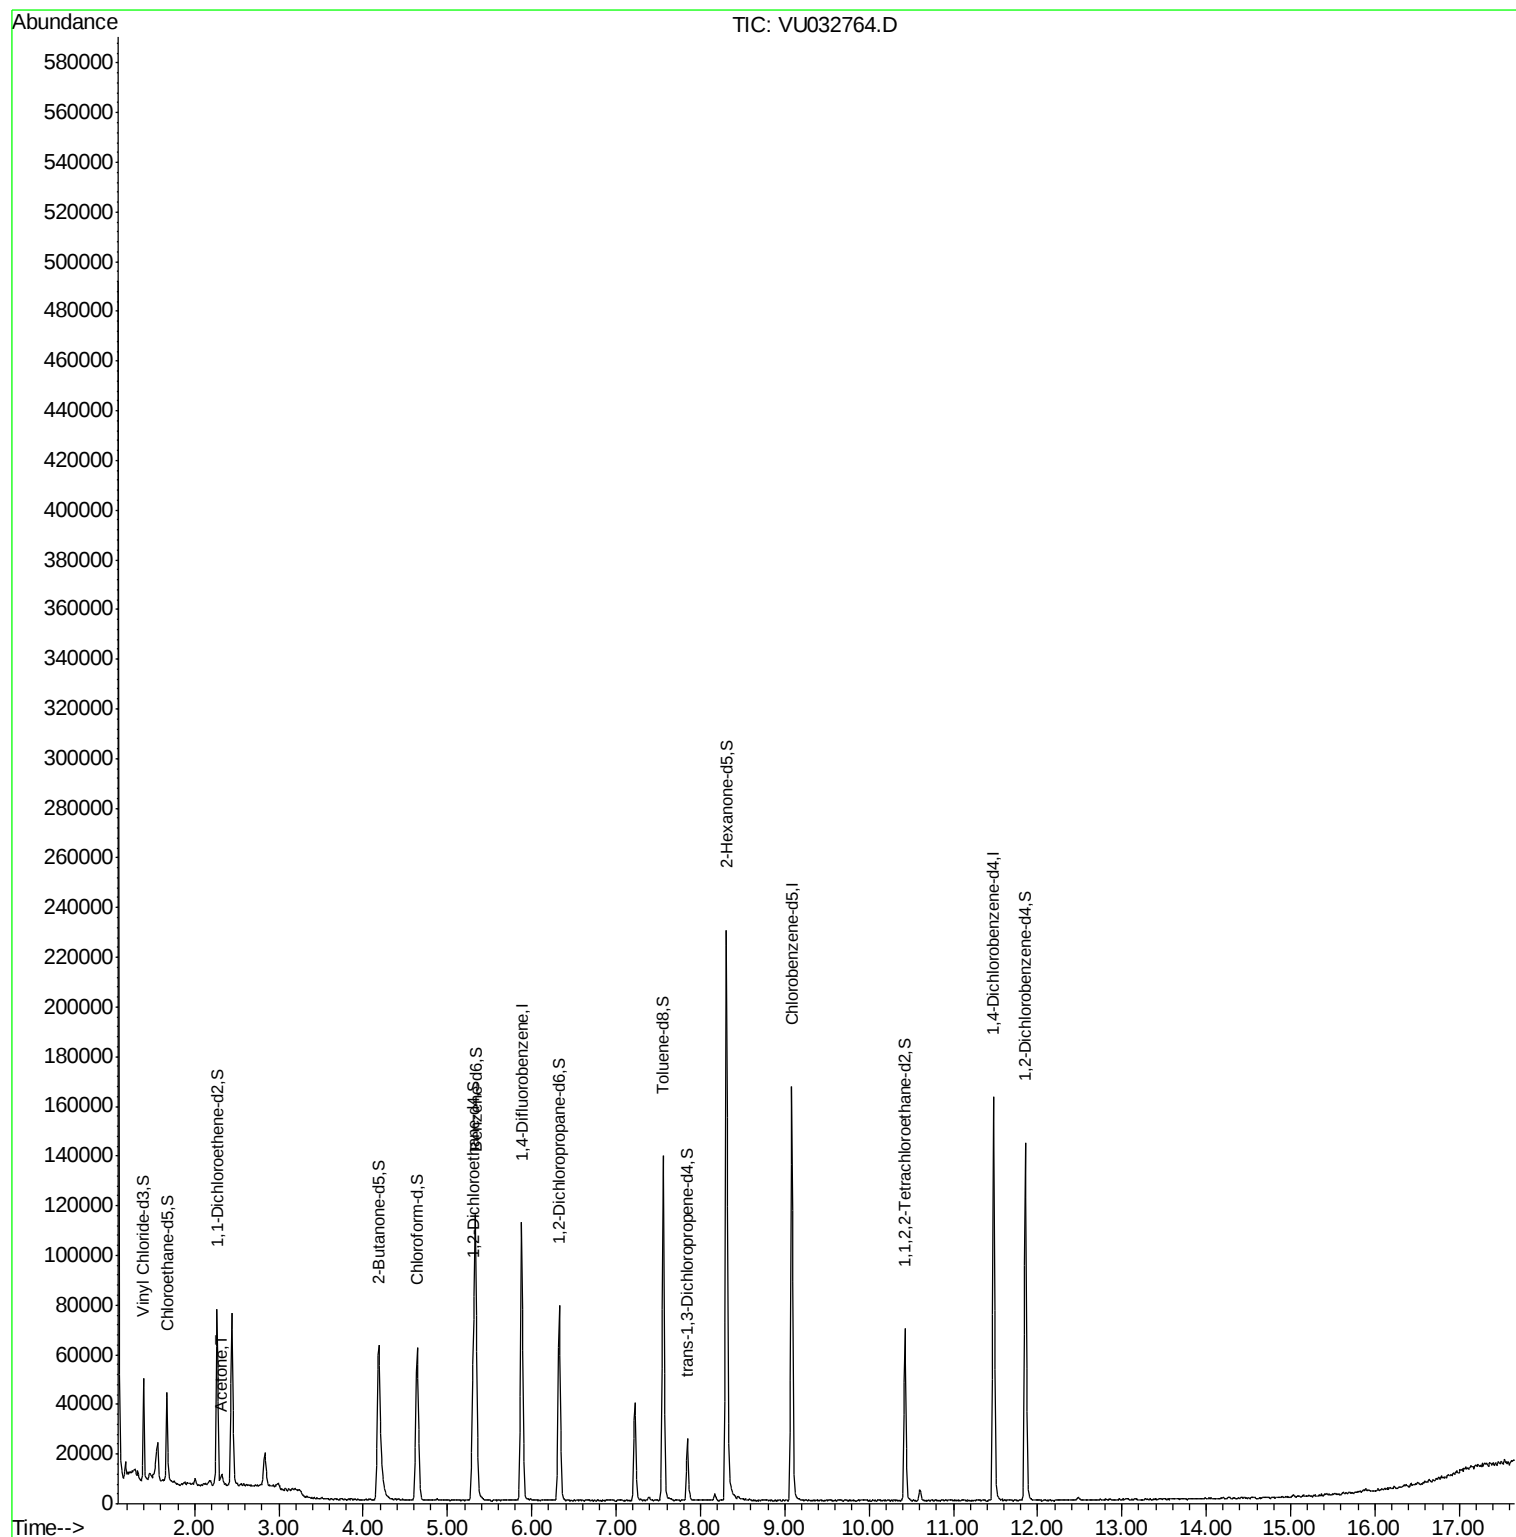

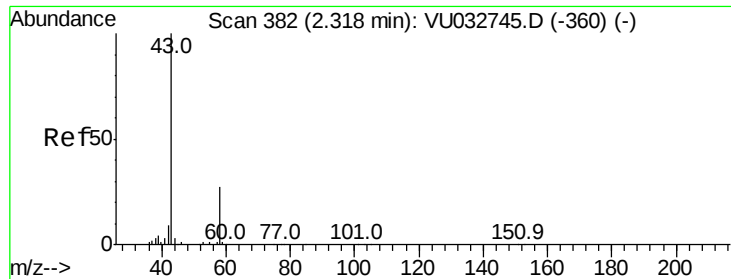

#13

Acetone

Concen: 2.956 ug/L

RT: 2.32 min Scan# 382

Delta R.T. -0.00 min

Lab File: VU032764.D

Acq: 15 Jun 2019 09:18

Instrument :

MSVOA_U

ClientSampleId :

COMA6

Tot Ion: 43 Resp: 3844

Ion Ratio Lower Upper

43 100

58 26.7 0.0 60.8

