

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
 Data File : VU032699.D
 Acq On : 13 Jun 2019 17:13
 Operator : JC/SP
 Sample : K3365-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM64

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	35	rBV3	5439	5358	1.50%	0.179%
2	1.396	87	95	110	rVB	46292	48591	13.64%	1.620%
3	1.573	135	150	160	rVB2	14034	30582	8.58%	1.019%
4	1.669	173	180	194	rVB	36498	44903	12.60%	1.497%
5	2.267	356	366	376	rBV	76677	114651	32.17%	3.822%
6	2.319	377	382	397	rVB2	6141	9591	2.69%	0.320%
7	2.444	413	421	435	rVB	14591	25935	7.28%	0.865%
8	4.184	950	962	993	rBV	54955	151321	42.46%	5.044%
9	4.640	1087	1104	1126	rBV2	59059	139529	39.15%	4.651%
10	5.331	1296	1319	1346	rBV2	114243	318717	89.44%	10.624%
11	5.881	1477	1490	1509	rBV	118334	243834	68.42%	8.128%
12	6.167	1573	1579	1589	rVB8	3639	6412	1.80%	0.214%
13	6.325	1616	1628	1649	rVB	75469	150802	42.32%	5.027%
14	6.537	1687	1694	1710	rVB6	3000	6099	1.71%	0.203%
15	7.225	1897	1908	1929	rBV2	40228	72493	20.34%	2.417%
16	7.560	2000	2012	2028	rBV	142892	252618	70.89%	8.421%
17	7.637	2028	2036	2053	rVB3	7660	15830	4.44%	0.528%
18	7.849	2092	2102	2119	rBV2	22510	38848	10.90%	1.295%
19	8.309	2235	2245	2285	rBV2	178466	356359	100.00%	11.879%
20	9.084	2473	2486	2517	rBV	172534	294095	82.53%	9.804%
21	9.380	2568	2578	2588	rBV4	3554	6244	1.75%	0.208%
22	9.794	2696	2707	2721	rBV2	16993	31320	8.79%	1.044%
23	10.039	2771	2783	2791	rBV3	2717	4462	1.25%	0.149%
24	10.428	2894	2904	2919	rBV	54940	89687	25.17%	2.990%
25	11.479	3218	3231	3254	rBV	169845	289451	81.22%	9.649%
26	11.855	3337	3348	3371	rBV	139952	246378	69.14%	8.213%
27	14.273	4092	4100	4111	rVB	3270	5756	1.62%	0.192%


Sum of corrected areas: 2999866

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032699.D
Acq On : 13 Jun 2019 17:13
Operator : JC/SP
Sample : K3365-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM64

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

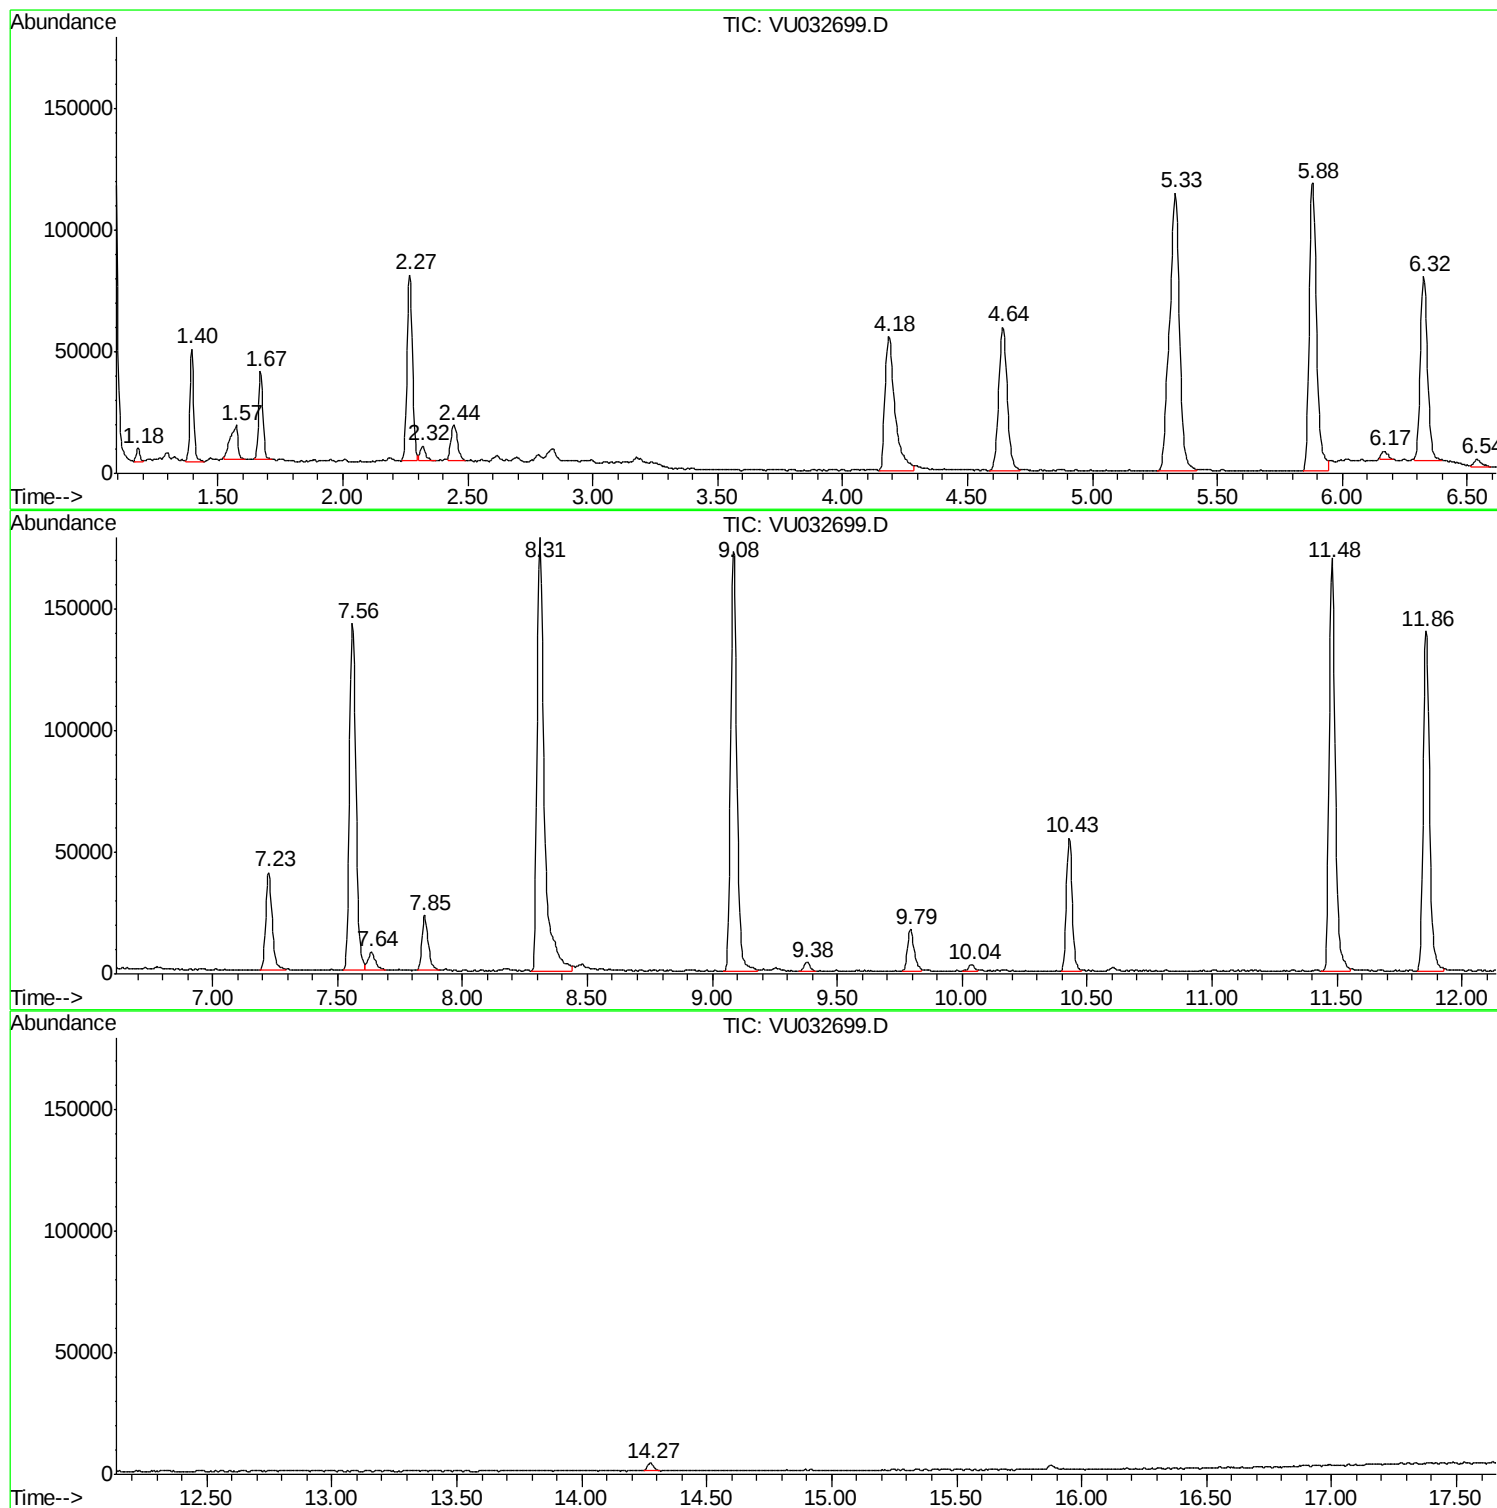

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032699.D
Acq On : 13 Jun 2019 17:13
Operator : JC/SP
Sample : K3365-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM64










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.44	0.53 ug/L	25935	1,4-Difluorobenzene	5.88

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol		60	C3H8O	000067-63-0	56
2	Isopropyl Alcohol		60	C3H8O	000067-63-0	9
3	Hvdrazine, ethyl-		60	C2H8N2	000624-80-6	9
4	Formamide		45	CH3NO	000075-12-7	5
5	Acetic acid, methoxy-		90	C3H6O3	000625-45-6	4

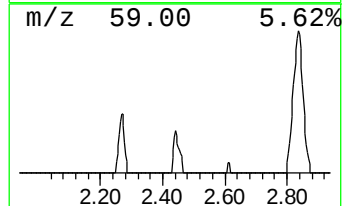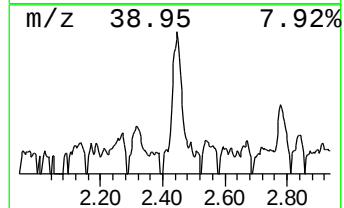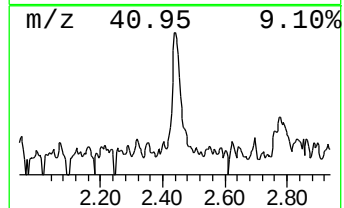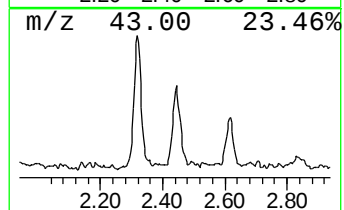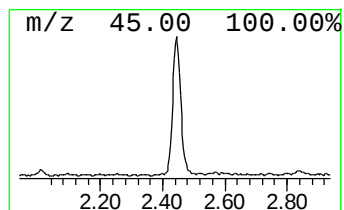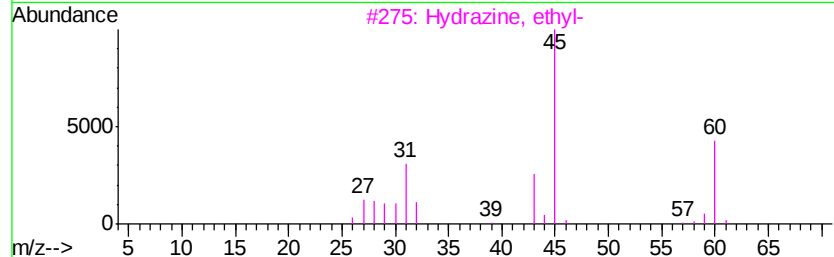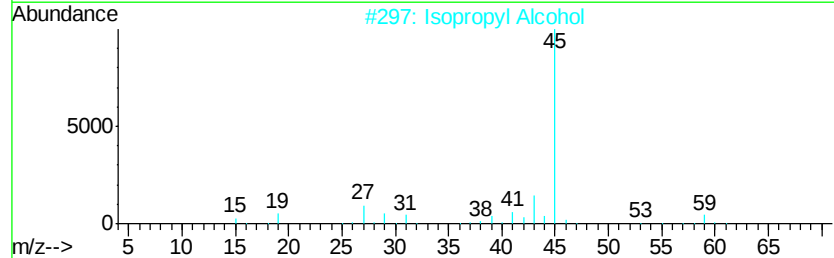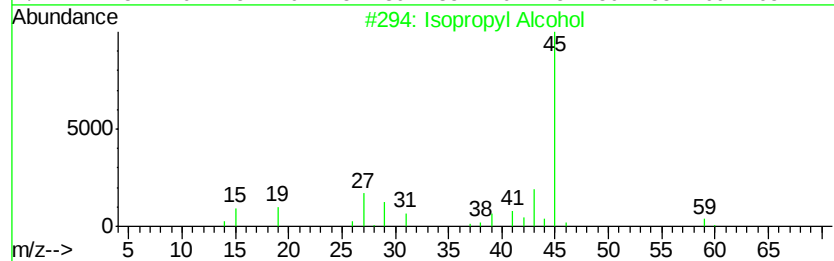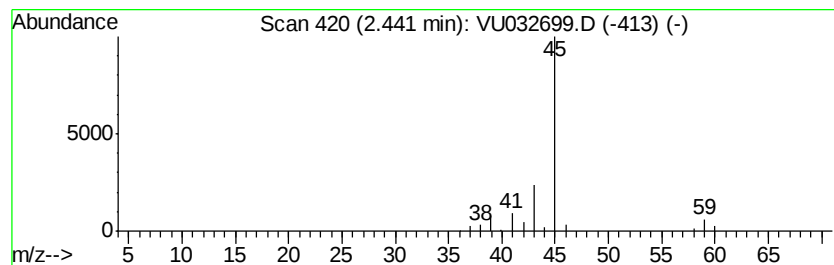

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061419\
Data File : VU032699.D
Acq On : 13 Jun 2019 17:13
Operator : JC/SP
Sample : K3365-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0M64

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.44	0.5	ug/L	25935	1	5.88	243834	5.0