

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
 Data File : VU032714.D
 Acq On : 13 Jun 2019 23:25
 Operator : JC/SP
 Sample : K3364-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM35

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	32	rBV2	6312	6065	1.70%	0.204%
2	1.396	88	95	106	rBV	45500	47411	13.27%	1.597%
3	1.566	136	148	157	rVB5	12719	29036	8.13%	0.978%
4	1.669	173	180	192	rBV	36246	46803	13.10%	1.576%
5	2.013	282	287	298	rVB2	3551	4991	1.40%	0.168%
6	2.267	356	366	377	rBV	75252	113532	31.79%	3.823%
7	2.318	378	382	393	rVB	4450	7118	1.99%	0.240%
8	2.444	410	421	438	rBV	73077	129427	36.24%	4.359%
9	2.833	534	542	557	rVB2	9508	19440	5.44%	0.655%
10	4.186	948	963	1002	rBV	56056	163634	45.81%	5.511%
11	4.640	1088	1104	1129	rBV	61425	144958	40.58%	4.882%
12	5.331	1298	1319	1341	rBV2	117935	325553	91.15%	10.964%
13	5.881	1477	1490	1514	rBV	109276	212981	59.63%	7.173%
14	6.170	1570	1580	1593	rBV6	6522	13317	3.73%	0.448%
15	6.325	1616	1628	1653	rBV	76744	155043	43.41%	5.221%
16	7.225	1898	1908	1926	rBV2	36078	64816	18.15%	2.183%
17	7.392	1950	1960	1973	rVB6	2729	4877	1.37%	0.164%
18	7.559	2001	2012	2030	rBV	141475	248536	69.58%	8.370%
19	7.849	2092	2102	2130	rVB	20029	35950	10.06%	1.211%
20	8.312	2236	2246	2288	rBV3	148987	357179	100.00%	12.029%
21	9.087	2473	2487	2512	rBV	157095	267467	74.88%	9.007%
22	10.427	2894	2904	2926	rBV	53291	88165	24.68%	2.969%
23	10.604	2950	2959	2966	rBV3	2635	4075	1.14%	0.137%
24	11.482	3221	3232	3259	rBV	142061	243727	68.24%	8.208%
25	11.855	3337	3348	3372	rBV	135897	235300	65.88%	7.924%


Sum of corrected areas: 2969401

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032714.D
Acq On : 13 Jun 2019 23:25
Operator : JC/SP
Sample : K3364-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM35

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

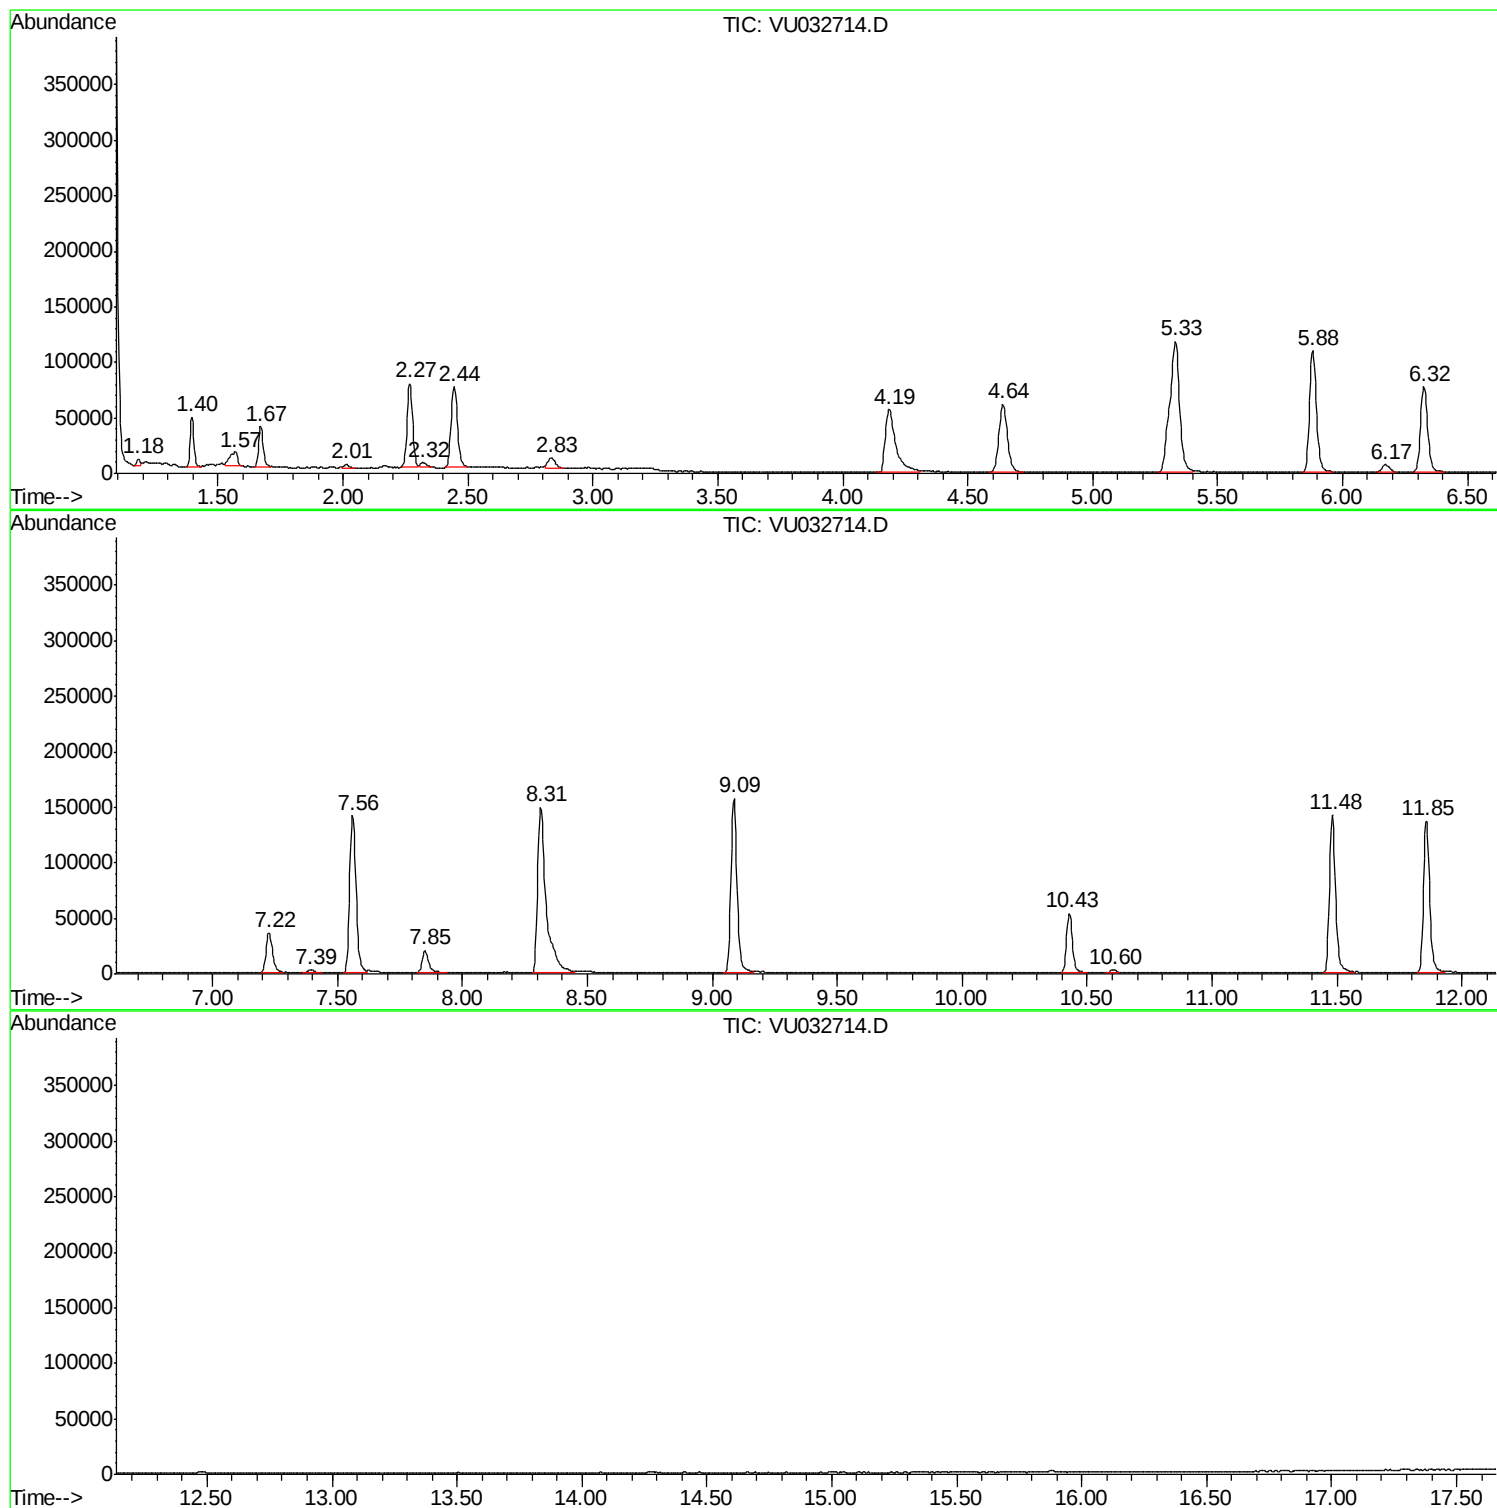

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032714.D
Acq On : 13 Jun 2019 23:25
Operator : JC/SP
Sample : K3364-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM35










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.44	3.04 ug/L	129427	1,4-Difluorobenzene	5.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	90
2		Isopropyl Alcohol	60	C3H8O	000067-63-0	83
3		Isopropyl Alcohol	60	C3H8O	000067-63-0	78
4		Isopropyl Alcohol	60	C3H8O	000067-63-0	78
5		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

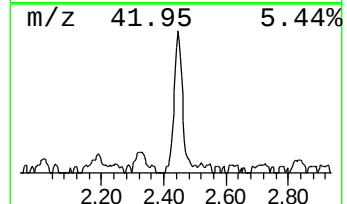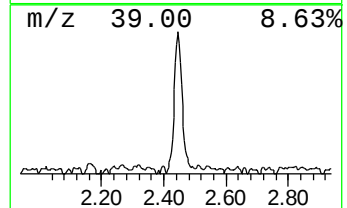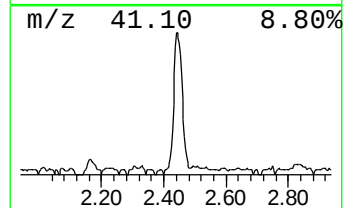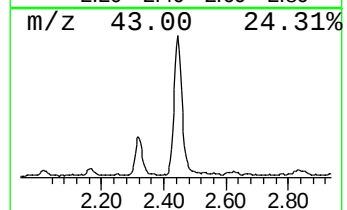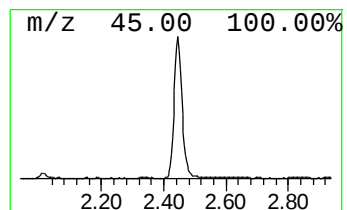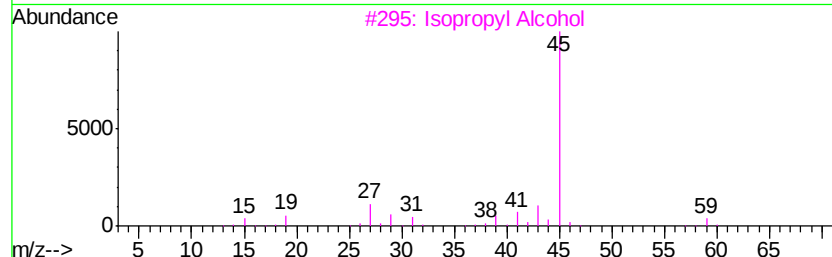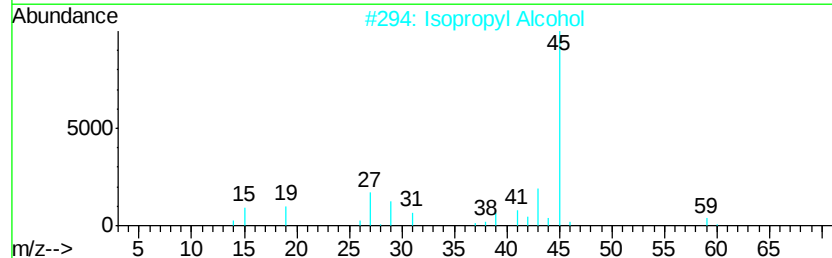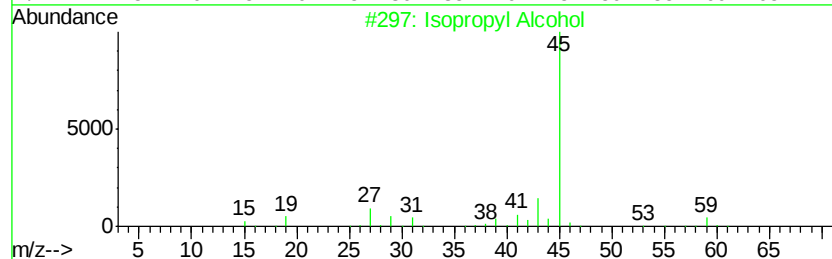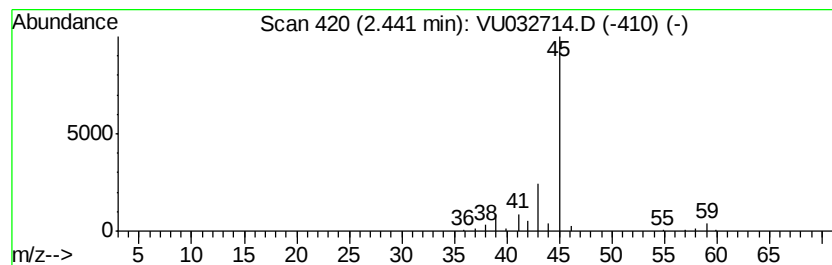

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061419\
Data File : VU032714.D
Acq On : 13 Jun 2019 23:25
Operator : JC/SP
Sample : K3364-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM35

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.44	3.0	ug/L	129427	1	5.88	212981	5.0