


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
Data File : VU032696.D
Acq On : 13 Jun 2019 15:54
Operator : JC/SP
Sample : BFB17
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB17

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Jun 17 17:34:05 2019

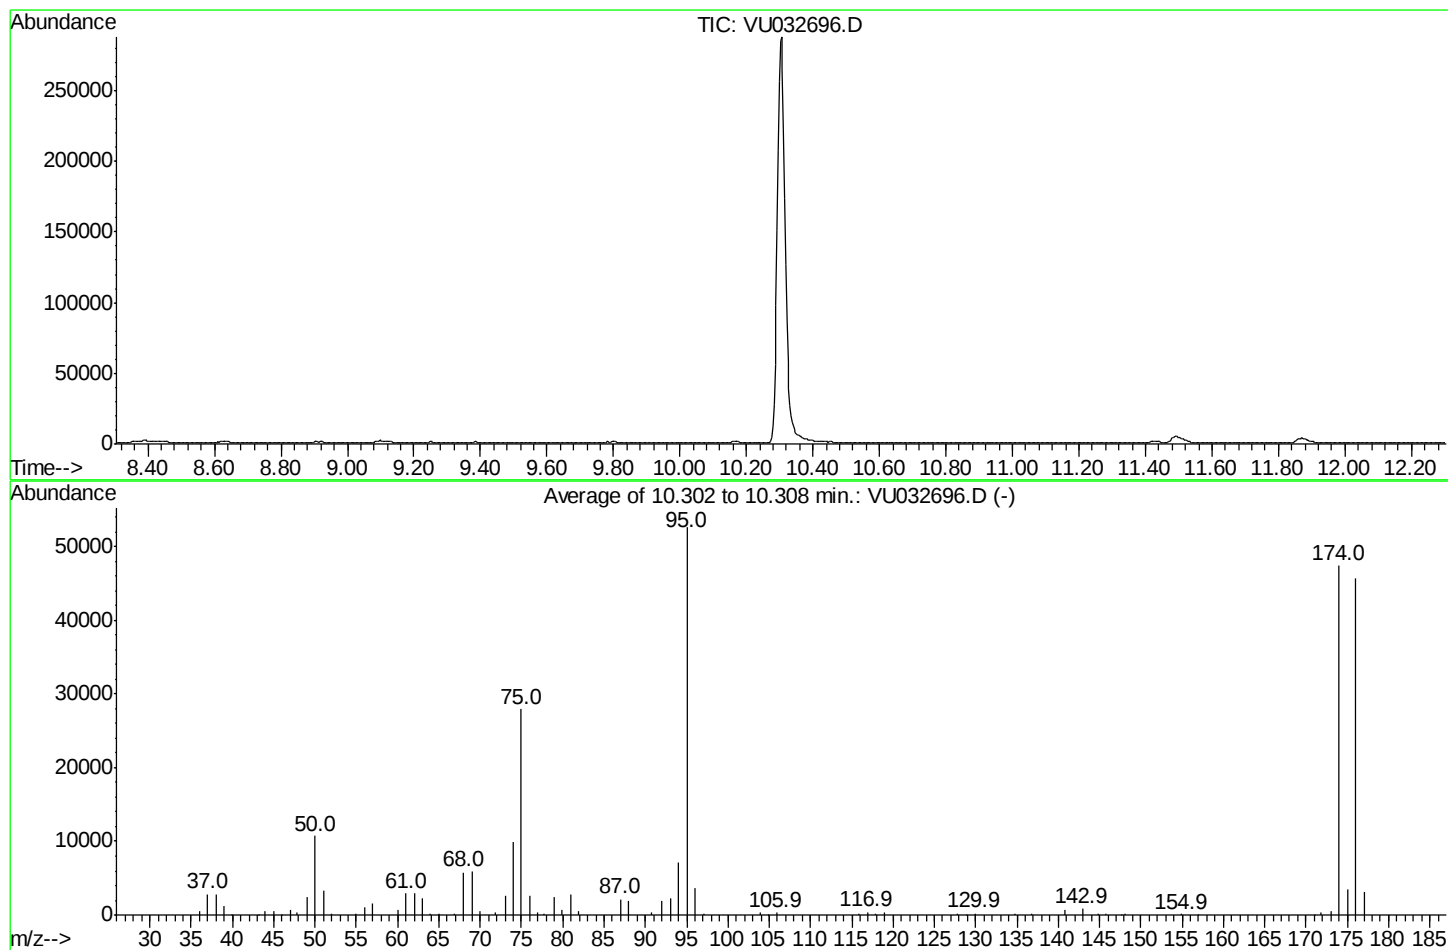

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	10768	PASS
75	95	30	80	53.1	27973	PASS
95	95	100	100	100.0	52640	PASS
96	95	5	9	6.8	3576	PASS
173	174	0.00	2	1.3	594	PASS
174	95	50	120	90.1	47421	PASS
175	174	5	9	7.5	3569	PASS
176	174	95	101	96.4	45712	PASS
177	176	5	9	7.0	3210	PASS

Scan 2853 (10.263 min): VU032696.D
BFB17

m/z	Abundance
39.90	630.0
44.00	359.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

m/z	Abundance
36.00	581.0
37.00	2947.0
38.00	2854.0
39.00	1147.0
40.00	723.0
43.10	112.0
44.00	800.0
45.00	563.0
45.90	104.0
47.00	664.0
47.90	381.0
49.00	2634.0
50.00	11206.0
51.00	3367.0
52.00	194.0
54.90	197.0
56.00	1021.0
57.00	1591.0
60.00	651.0
61.00	3114.0
62.00	2911.0
63.00	2290.0
63.90	263.0
65.00	265.0
66.90	145.0
68.00	5853.0
69.00	6022.0
70.00	477.0
71.90	383.0
73.00	2701.0
74.00	10205.0
75.00	28760.0
76.00	2687.0
76.90	298.0
77.80	144.0
78.90	2589.0
79.90	611.0
80.90	2882.0
81.90	595.0
87.00	2209.0
87.90	2179.0
90.80	272.0
92.00	2058.0
93.00	2431.0
94.00	7373.0
95.00	53928.0
96.00	3726.0
97.10	111.0
103.80	320.0
104.90	104.0
105.90	286.0
115.90	240.0
116.90	388.0
117.80	205.0
118.90	308.0
127.80	203.0
128.80	130.0
129.80	250.0
134.80	109.0
136.80	110.0
140.80	685.0
142.90	869.0
144.90	123.0
145.80	120.0
148.00	152.0
155.00	136.0
171.90	325.0
173.00	550.0
174.00	47408.0
175.00	3635.0
176.00	45704.0
177.00	3246.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

m/z	Abundance
36.00	527.0
37.00	2877.0
38.00	2865.0
39.00	1231.0
40.00	656.0
44.00	872.0
45.00	581.0
45.90	106.0
47.00	657.0
47.90	371.0
49.00	2483.0
50.00	11078.0
51.00	3444.0
52.00	150.0
54.90	218.0
56.00	1068.0
57.00	1610.0
60.00	676.0
61.00	2980.0
62.00	2990.0
63.00	2258.0
63.90	264.0
65.00	262.0
66.90	152.0
68.00	5939.0
69.00	6149.0
70.00	497.0
71.90	354.0
73.00	2725.0
74.00	10213.0
75.00	28784.0
76.00	2627.0
77.00	299.0
77.70	156.0
78.90	2506.0
79.90	653.0
80.90	2958.0
81.90	599.0
87.00	2180.0
87.90	2044.0
90.80	298.0
92.00	1879.0
93.00	2334.0
94.00	7338.0
95.00	54320.0
96.00	3673.0
97.10	124.0
103.80	296.0
105.90	290.0
115.90	235.0
116.90	404.0
117.80	233.0
119.00	267.0
127.80	237.0
128.80	110.0
129.90	222.0
134.70	114.0
136.90	125.0
140.90	704.0
142.90	829.0
144.90	123.0
145.80	127.0
148.00	143.0
154.90	142.0
156.90	109.0
171.10	121.0
171.80	315.0
173.10	617.0
174.00	48968.0
175.00	3689.0
176.00	47112.0
177.00	3377.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

m/z	Abundance
35.90	453.0
37.00	2532.0
38.00	2555.0
39.00	1128.0
39.90	613.0
44.00	863.0
45.00	541.0
47.10	570.0
47.80	319.0
49.00	2195.0
50.00	10020.0
51.00	3254.0
51.90	125.0
54.90	207.0
56.00	970.0
57.00	1565.0
60.00	614.0
61.00	2564.0
62.00	2746.0
63.00	2026.0
64.00	231.0
65.00	246.0
66.90	156.0
68.00	5423.0
69.00	5719.0
70.00	469.0
71.90	289.0
73.00	2549.0
74.00	9372.0
75.00	26376.0
76.00	2335.0
77.00	328.0
77.80	155.0
78.90	2263.0
79.90	618.0
80.90	2745.0
81.80	542.0
87.00	2015.0
87.90	1771.0
90.80	303.0
92.00	1575.0
93.10	2180.0
94.00	6477.0
95.00	49672.0
96.00	3330.0
97.00	112.0
103.90	233.0
105.90	280.0
115.90	233.0
116.90	371.0
117.80	237.0
118.90	235.0
127.80	236.0
130.00	225.0
134.80	111.0
136.90	114.0
140.90	649.0
143.00	709.0
144.90	111.0
145.80	115.0
147.70	108.0
148.10	110.0
154.90	137.0
156.90	127.0
171.10	122.0
171.80	281.0
173.10	616.0
174.00	45888.0
175.00	3383.0
176.00	44320.0
177.00	3009.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17