


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061419\
 Data File : VU032721.D
 Acq On : 14 Jun 2019 13:46
 Operator : JC/SP
 Sample : BFB18
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB18

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Jun 17 17:34:05 2019

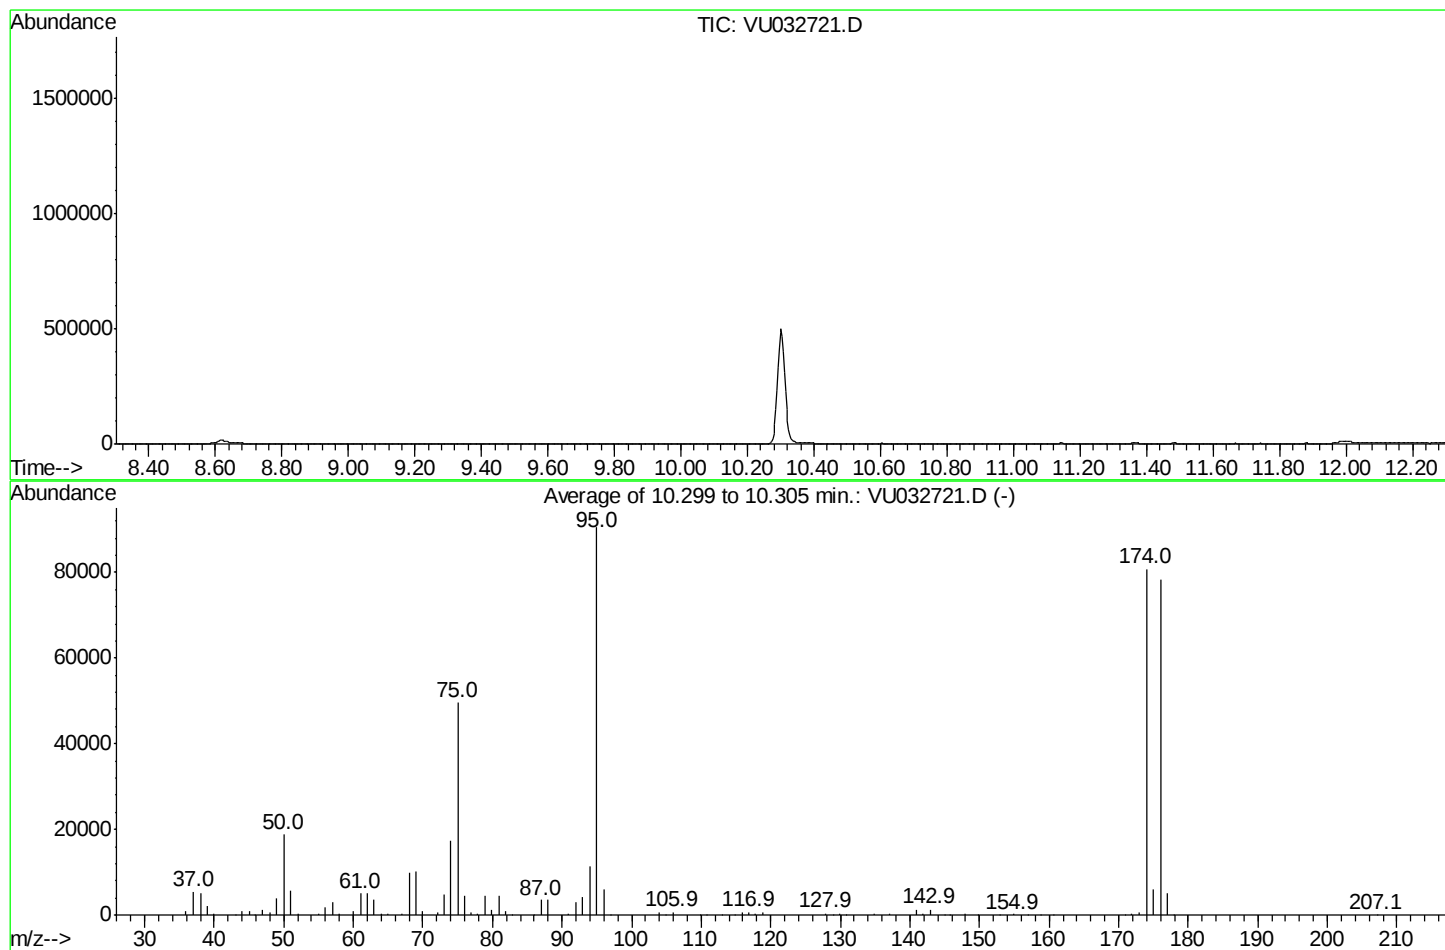

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	18773	PASS
75	95	30	80	54.8	49576	PASS
95	95	100	100	100.0	90533	PASS
96	95	5	9	6.6	5960	PASS
173	174	0.00	2	0.8	664	PASS
174	95	50	120	89.2	80738	PASS
175	174	5	9	7.5	6039	PASS
176	174	95	101	96.9	78237	PASS
177	176	5	9	6.5	5059	PASS

Scan 2851 (10.257 min): VU032721.D
BFB18

m/z	Abundance
35.90	285.0
39.90	712.0
44.00	500.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
36.00	1267.0
37.00	5496.0
38.00	4995.0
39.00	2056.0
40.00	850.0
44.00	1456.0
45.00	999.0
45.80	113.0
47.00	1183.0
48.00	528.0
49.00	4330.0
50.00	18928.0
51.00	5941.0
52.00	290.0
55.10	298.0
56.00	1686.0
57.00	2979.0
57.90	206.0
60.00	949.0
61.00	5158.0
62.00	5127.0
63.00	3741.0
64.00	367.0
64.90	210.0
66.90	241.0
68.00	10021.0
69.00	10488.0
70.00	900.0
72.00	540.0
73.00	4756.0
74.00	17568.0
75.00	50096.0
76.00	4571.0
76.90	662.0
77.80	347.0
78.90	4499.0
79.90	1277.0
80.90	4570.0
81.90	993.0
82.90	149.0
86.00	113.0
87.00	3646.0
88.00	3861.0
90.90	428.0
92.00	2949.0
93.00	4368.0
94.00	11621.0
95.00	90520.0
96.00	5880.0
97.00	164.0
103.90	523.0
104.90	139.0
105.90	673.0
109.90	107.0
110.80	160.0
112.90	149.0
114.80	132.0
115.90	447.0
116.90	705.0
117.80	388.0
118.90	589.0
127.90	331.0
128.90	146.0
129.80	362.0
130.90	138.0
134.90	179.0
137.00	194.0
140.90	1092.0
141.90	172.0
142.90	1301.0
144.90	130.0
147.80	206.0
152.80	103.0
154.90	287.0
156.90	140.0
158.80	156.0
171.00	121.0
171.90	426.0
174.00	78640.0
175.00	5956.0
176.00	76400.0
177.00	4982.0
177.90	126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
36.00	1289.0
37.00	5696.0
38.00	5345.0
39.00	2059.0
39.90	921.0
44.00	1512.0
45.00	1031.0
45.80	135.0
47.00	1216.0
48.10	546.0
49.00	4160.0
50.00	19408.0
51.00	5826.0
52.00	315.0
55.10	297.0
56.00	1708.0
57.00	3065.0
57.90	188.0
60.00	941.0
61.00	5220.0
62.00	5232.0
63.00	3753.0
64.00	374.0
64.90	226.0
67.00	251.0
68.00	10070.0
69.00	10443.0
70.00	929.0
72.10	591.0
73.00	4885.0
74.00	17816.0
75.00	51144.0
76.00	4656.0
77.00	581.0
77.90	329.0
78.90	4615.0
79.90	1313.0
80.90	4674.0
81.90	1000.0
82.90	154.0
86.00	112.0
87.00	3745.0
88.00	3824.0
90.90	436.0
92.00	3205.0
93.00	4379.0
94.00	11851.0
95.00	93744.0
96.00	6183.0
97.00	144.0
103.90	530.0
104.90	133.0
105.90	695.0
110.80	170.0
112.90	132.0
114.80	155.0
115.90	472.0
116.90	688.0
117.80	432.0
118.90	640.0
127.90	367.0
129.00	131.0
129.80	305.0
130.90	143.0
134.90	241.0
137.00	220.0
141.00	1182.0
141.90	170.0
142.90	1330.0
144.90	119.0
145.70	100.0
147.90	203.0
154.90	282.0
156.90	162.0
158.90	135.0
160.70	114.0
171.00	106.0
171.90	400.0
173.00	1005.0
174.00	83544.0
175.00	6224.0
176.00	80960.0
177.00	5232.0
178.00	124.0
207.10	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
36.00	1200.0
37.00	5297.0
38.10	5086.0
39.00	1816.0
39.90	950.0
43.10	108.0
44.00	1461.0
45.00	977.0
45.90	120.0
47.00	1136.0
48.00	554.0
49.00	3652.0
50.00	17984.0
51.00	5304.0
52.00	280.0
55.10	288.0
56.00	1585.0
57.00	2840.0
58.00	148.0
60.00	882.0
61.00	4828.0
62.00	4831.0
63.00	3436.0
63.90	359.0
65.00	215.0
67.10	249.0
68.00	9227.0
69.00	9506.0
70.00	831.0
72.10	566.0
73.00	4599.0
74.00	16448.0
75.00	47488.0
76.00	4194.0
77.00	490.0
77.90	328.0
78.90	4276.0
79.90	1188.0
80.90	4437.0
81.90	854.0
82.80	128.0
86.90	3340.0
88.00	3374.0
90.90	450.0
92.00	2975.0
93.00	4065.0
94.00	11085.0
95.00	87336.0
96.00	5817.0
97.10	126.0
103.90	521.0
104.80	132.0
105.90	582.0
110.80	148.0
113.00	110.0
114.80	144.0
115.90	462.0
116.90	627.0
117.80	421.0
118.90	634.0
127.90	371.0
128.90	133.0
129.90	281.0
130.90	149.0
134.90	248.0
137.00	200.0
141.00	1158.0
141.90	149.0
142.90	1226.0
145.80	118.0
147.90	189.0
149.80	113.0
154.90	238.0
156.80	171.0
158.90	107.0
170.80	100.0
171.90	337.0
173.00	987.0
174.00	80032.0
175.00	5938.0
176.00	77352.0
177.00	4965.0
178.00	123.0
207.10	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18