

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061421\
 Data File : VU044201.D
 Acq On : 14 Jun 2021 23:40
 Operator : SY/MD
 Sample : M2672-39
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 15 04:58:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060921W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 10 05:11:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.385	168	184764	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.260	114	316040	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.423	117	319341	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.819	152	150900	50.000	ug/l	0.00


System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.713	65	137132	46.672	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.340%	
35) Dibromofluoromethane	5.298	113	107184	48.754	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.500%	
50) Toluene-d8	7.906	98	420737	49.832	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.660%	
62) 4-Bromofluorobenzene	10.639	95	150747	44.552	ug/l	0.00
Spiked Amount	50.000		Recovery	=	89.100%	

Target Compounds			Qvalue			
3) Chloromethane	1.523	50	413	Below Cal		92
5) Bromomethane	1.871	94	444	0.346 ug/l		94
6) Chloroethane	1.935	64	130	Below Cal	#	42
10) Methyl Iodide	2.736	142	699	0.266 ug/l	#	77
11) Tert butyl alcohol	3.195	59	1865	2.360 ug/l	#	73
16) Acetone	2.652	43	13414	6.758 ug/l		97
18) Methyl Acetate	2.967	43	1018	0.269 ug/l	#	50
20) Methylene Chloride	3.057	84	10255	2.740 ug/l		95
25) 2-Butanone	4.729	43	4591	1.872 ug/l		94
29) Tetrahydrofuran	5.070	42	333	0.250 ug/l	#	41
31) Cyclohexane	5.382	56	4020	0.969 ug/l	#	1
36) 1,1-Dichloropropene	5.385	75	15520	4.414 ug/l	#	46
37) Ethyl Acetate	4.729	43	4591	1.090 ug/l	#	67
38) Carbon Tetrachloride	5.385	117	19773	6.229 ug/l	#	17
41) Methacrylonitrile	5.089	41	612	0.284 ug/l	#	23
43) Isopropyl Acetate	5.922	43	17667	2.957 ug/l		99
45) 1,2-Dichloropropane	7.047	63	1575	0.557 ug/l	#	43
48) Methyl methacrylate	6.909	41	6644	2.285 ug/l	#	11
49) 1,4-Dioxane	7.047	88	233	3.064 ug/l	#	1
51) 4-Methyl-2-Pentanone	7.800	43	7557	1.748 ug/l		99
54) cis-1,3-Dichloropropene	7.745	75	30418	7.178 ug/l	#	64
57) 1,3-Dichloropropane	8.735	76	20864	4.534 ug/l	#	42
59) 2-Hexanone	8.735	43	265995	77.085 ug/l	#	50
74) N-amyl acetate	10.330	43	1418	0.312 ug/l	#	85
76) 1,2,3-Trichloropropane	10.639	75	75094	14.843 ug/l	#	47
81) trans-1,4-Dichloro-2-b...	10.639	75	75094	53.804 ug/l	#	13
89) n-Butylbenzene	12.217	91	2018	0.209 ug/l		97
92) 1,2-Dibromo-3-Chloropr...	13.005	75	218	0.219 ug/l	#	73
93) 1,2,4-Trichlorobenzene	13.848	180	1767	0.560 ug/l		96
94) Hexachlorobutadiene	14.031	225	415	0.245 ug/l		90
95) Naphthalene	14.095	128	9255	3.659 ug/l		97
96) 1,2,3-Trichlorobenzene	14.336	180	1898	0.620 ug/l		92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jun 15 04:58:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060921W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 10 05:11:37 2021
Response via : Initial Calibration

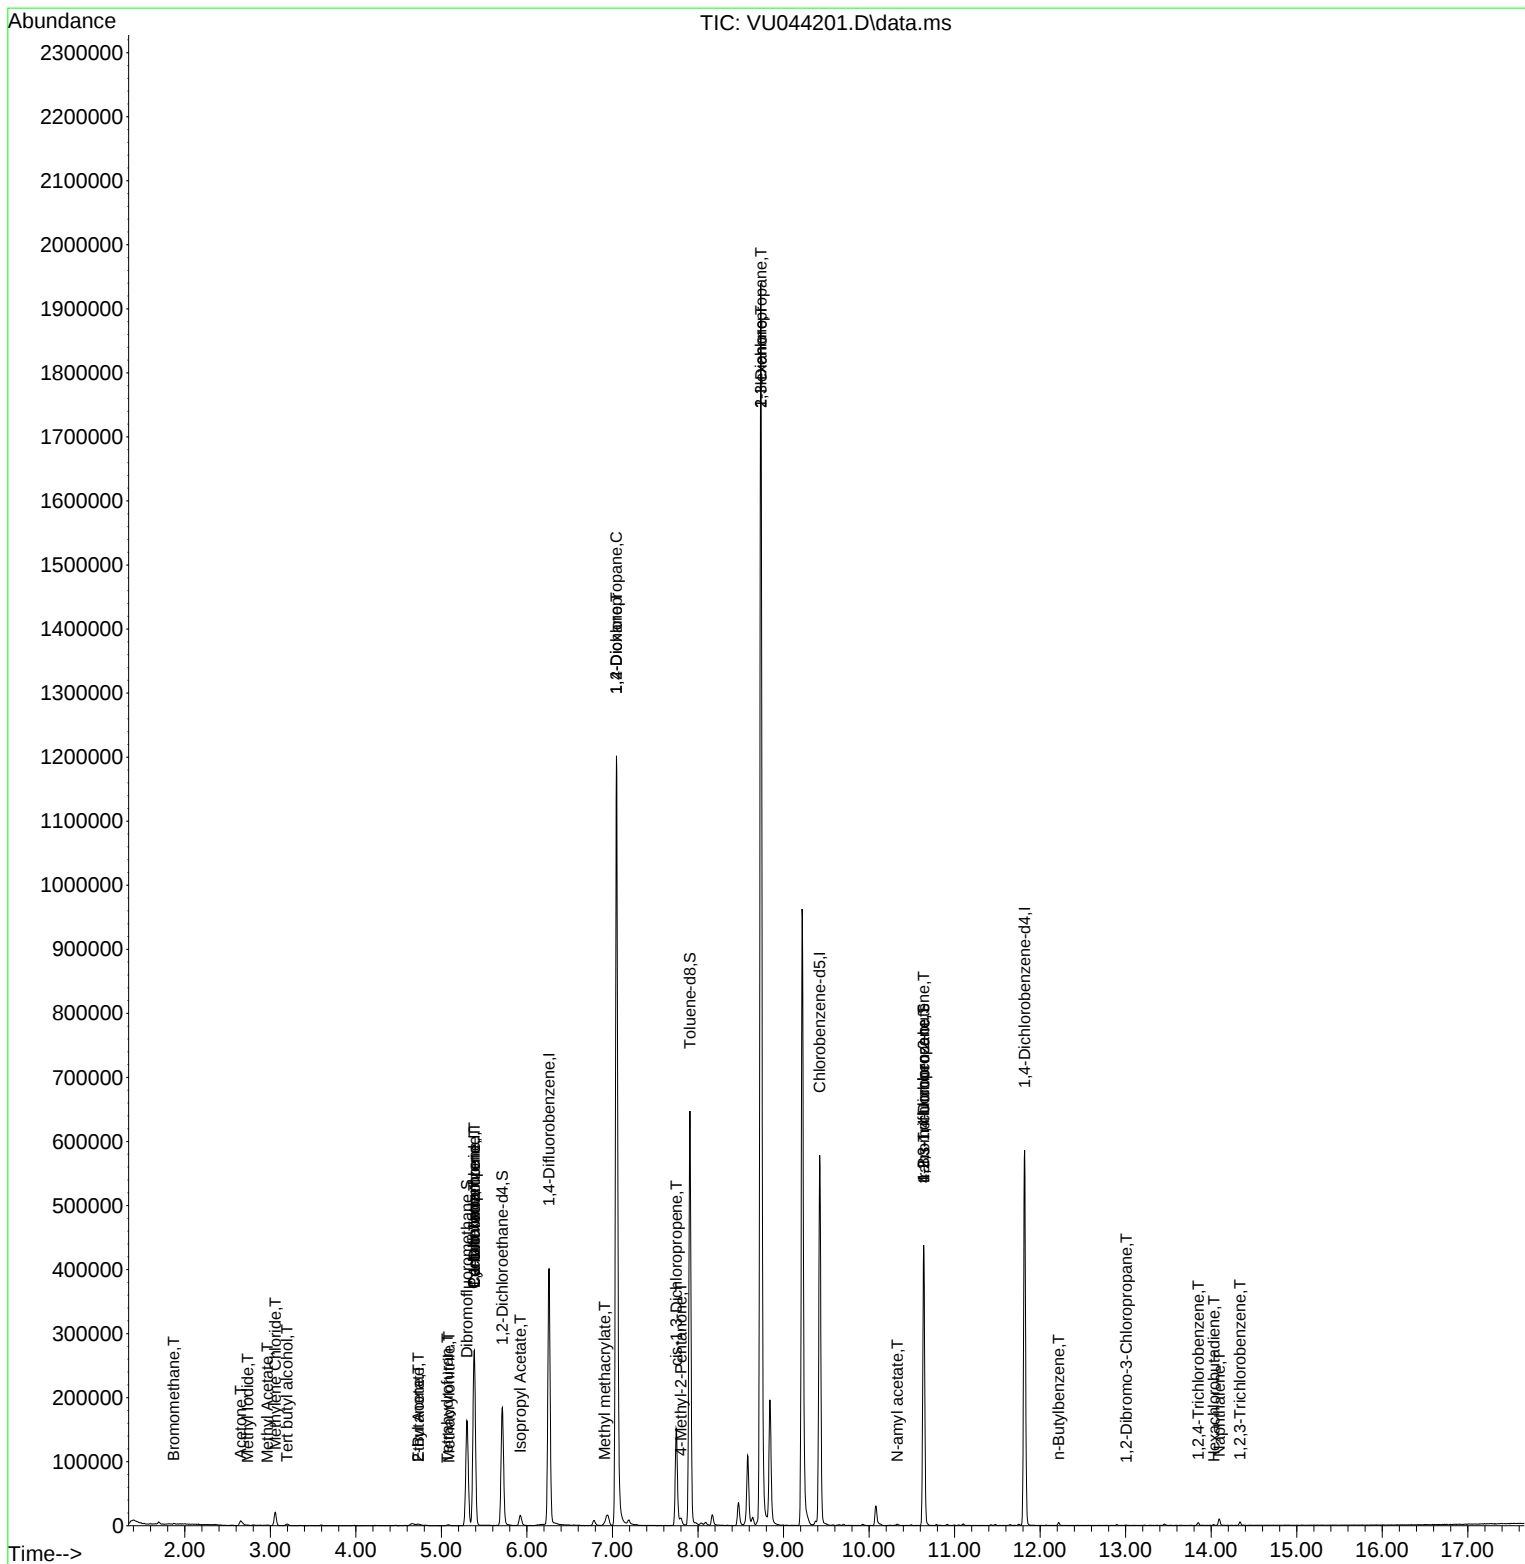

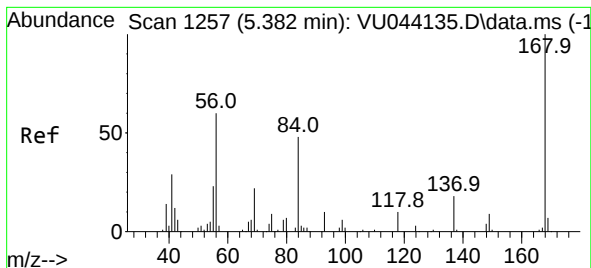

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.385 min Scan# 1258

Delta R.T. 0.003 min

Lab File: VU044201.D





Acq: 14 Jun 2021 23:40

Tgt Ion:168 Resp: 184764

Ion Ratio Lower Upper

168 100

99 61.7 51.3 76.9

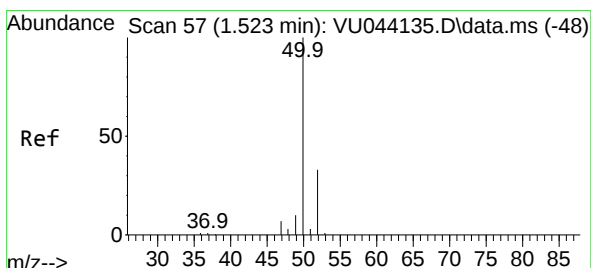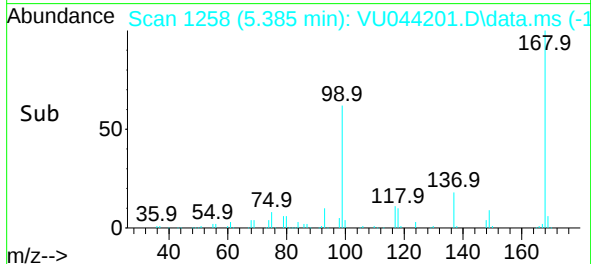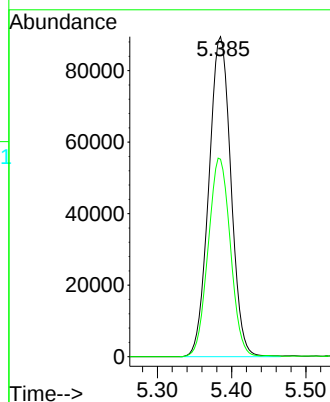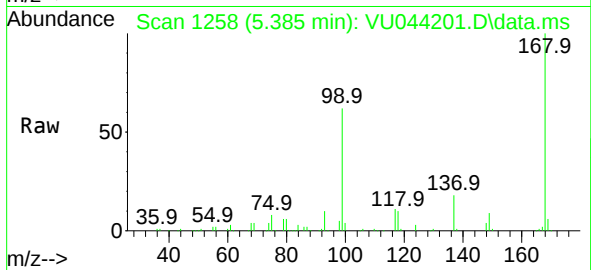

#3

Chloromethane

Concen: Below Cal

RT: 1.523 min Scan# 57

Delta R.T. 0.000 min

Lab File: VU044201.D




Acq: 14 Jun 2021 23:40


Tgt Ion: 50 Resp: 413

Ion Ratio Lower Upper

50 100

52 28.6 26.6 39.8


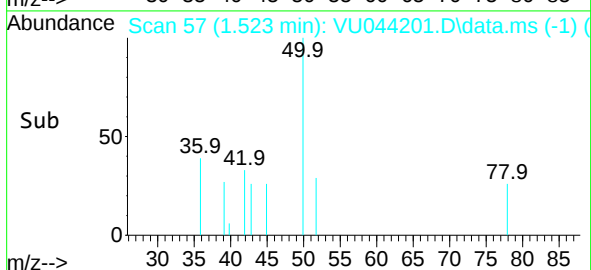
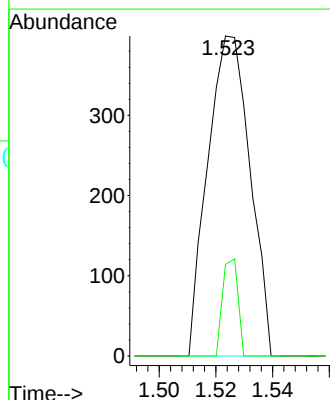
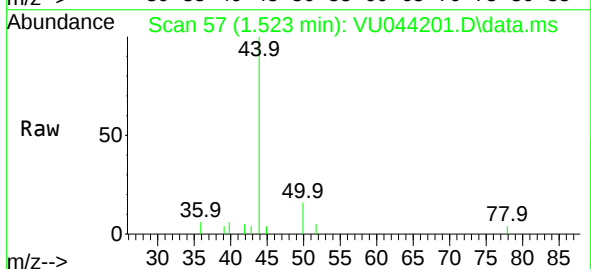




#5
Bromomethane
Concen: 0.346 ug/l
RT: 1.871 min Scan# 165
Delta R.T. 0.032 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 94 Resp: 444
Ion Ratio Lower Upper
94 100
96 86.4 74.1 111.1

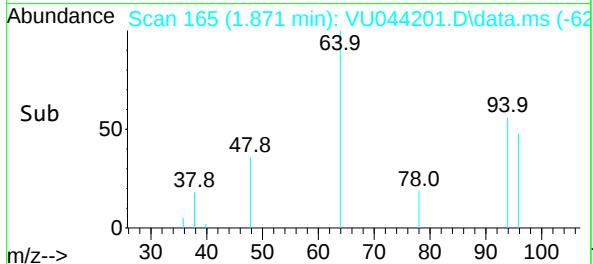

#6
Chloroethane
Concen: Below Cal
RT: 1.935 min Scan# 185
Delta R.T. 0.010 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40


Tgt Ion: 64 Resp: 130
Ion Ratio Lower Upper
64 100
66 0.0 26.1 39.1#

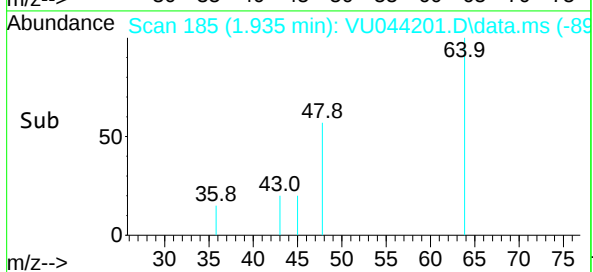






#10
Methyl Iodide
Concen: 0.266 ug/l
RT: 2.736 min Scan# 434
Delta R.T. 0.010 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Instrument :
MSVOA_U
ClientSampleId :







Tgt Ion:142 Resp: 699
Ion Ratio Lower Upper
142 100
127 33.3 37.0 55.6#
141 0.0 11.6 17.4#



#11
Tert butyl alcohol
Concen: 2.360 ug/l
RT: 3.195 min Scan# 577
Delta R.T. -0.004 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Tgt Ion: 59 Resp: 1865
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#


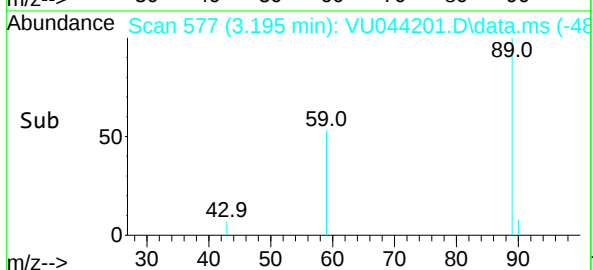






#16
Acetone
Concen: 6.758 ug/l
RT: 2.652 min Scan# 408
Delta R.T. 0.019 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 43 Resp: 13414
Ion Ratio Lower Upper
43 100
58 37.0 28.0 42.0

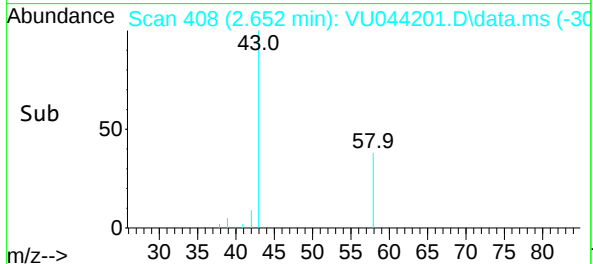

#18
Methyl Acetate
Concen: 0.269 ug/l
RT: 2.967 min Scan# 506
Delta R.T. 0.013 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Tgt Ion: 43 Resp: 1018
Ion Ratio Lower Upper
43 100
74 0.0 20.3 30.5#

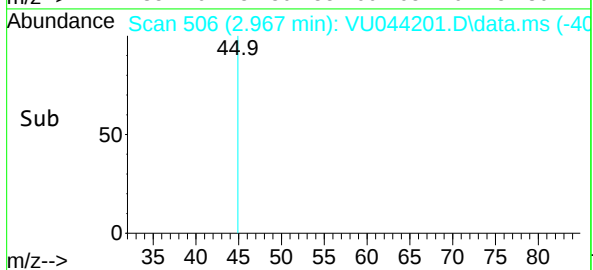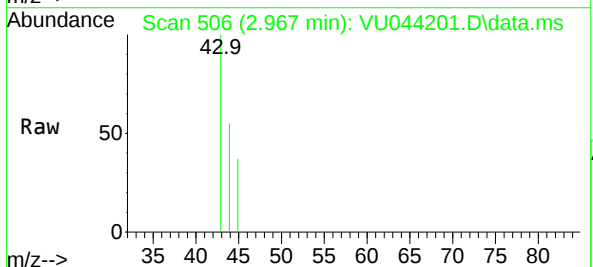



#20

Methylene Chloride

Concen: 2.740 ug/l

RT: 3.057 min Scan# 534

Delta R.T. 0.006 min

Lab File: VU044201.D

Acq: 14 Jun 2021 23:40

Tgt Ion: 84 Resp: 10255





Ion Ratio Lower Upper

84 100

49 113.0 96.9 145.3

51 36.2 31.0 46.6

86 64.4 51.0 76.6

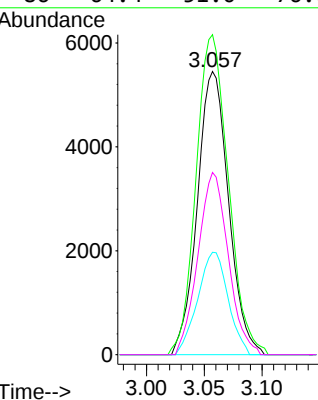

#25

2-Butanone

Concen: 1.872 ug/l

RT: 4.729 min Scan# 1054

Delta R.T. 0.019 min

Lab File: VU044201.D




Acq: 14 Jun 2021 23:40


Tgt Ion: 43 Resp: 4591

Ion Ratio Lower Upper

43 100

72 24.9 22.6 33.8

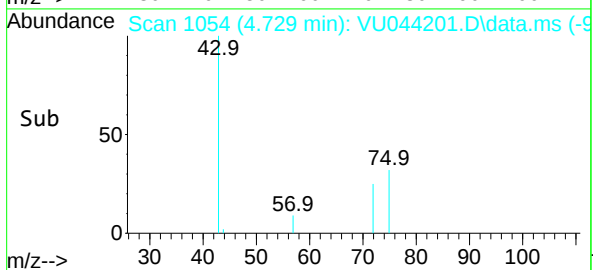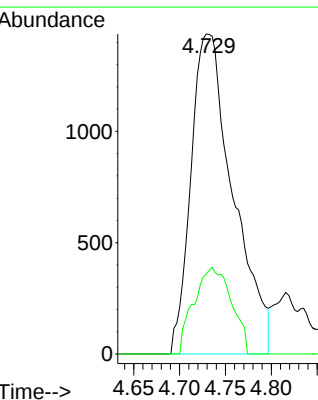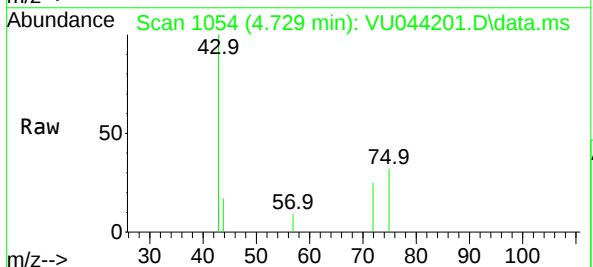



#29

Tetrahydrofuran

Concen: 0.250 ug/l

RT: 5.070 min Scan# 1160

Delta R.T. 0.013 min





Lab File: VU044201.D

Acq: 14 Jun 2021 23:40

Instrument :
MSVOA_U
ClientSampled :

Tgt Ion: 42 Resp: 333

Ion	Ratio	Lower	Upper
42	100		
72	105.7	38.6	57.8#
71	64.6	35.5	53.3#

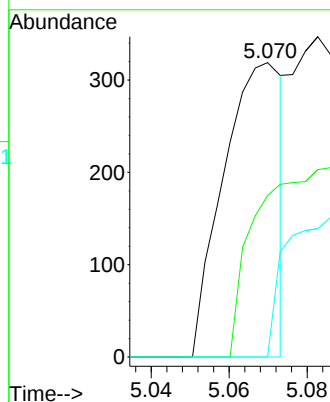

#31

Cyclohexane

Concen: 0.969 ug/l

RT: 5.382 min Scan# 1257




Delta R.T. -0.013 min


Lab File: VU044201.D

Acq: 14 Jun 2021 23:40

Tgt Ion: 56 Resp: 4020

Ion	Ratio	Lower	Upper
56	100		
69	192.9	25.5	38.3#
84	142.4	66.3	99.5#

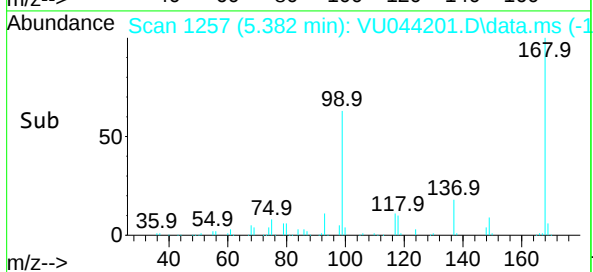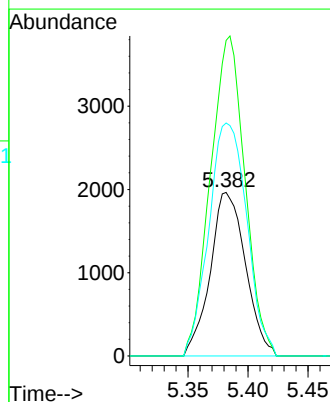







#33

1,2-Dichloroethane-d4
Concen: 46.672 ug/l
RT: 5.713 min Scan# 1360
Delta R.T. 0.003 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Instrument :
MSVOA_U
ClientSampled :




Tgt Ion: 65 Resp: 137132
Ion Ratio Lower Upper
65 100
67 53.7 0.0 106.6

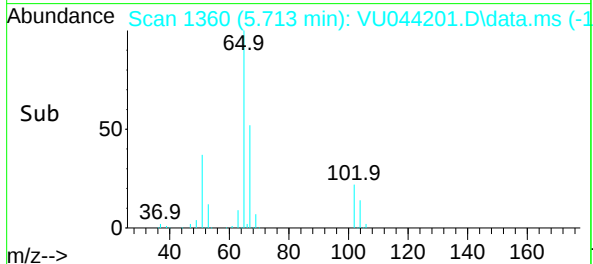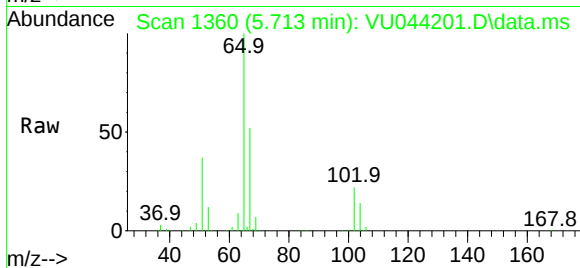


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.260 min Scan# 1530
Delta R.T. 0.004 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Tgt Ion: 114 Resp: 316040
Ion Ratio Lower Upper
114 100
63 22.1 0.0 45.8
88 16.9 0.0 34.0

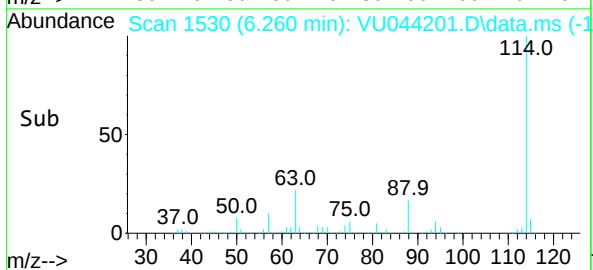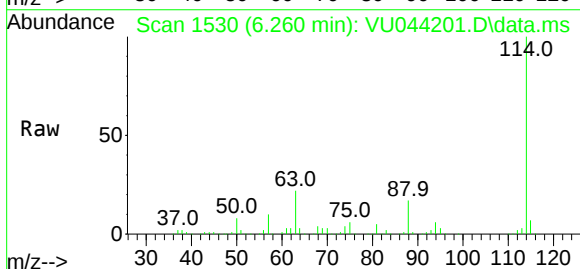



#35

Dibromofluoromethane

Concen: 48.754 ug/l

RT: 5.298 min Scan# 1231

Delta R.T. 0.000 min

Lab File: VU044201.D

Acq: 14 Jun 2021 23:40





Tgt Ion:113 Resp: 107184

Ion Ratio Lower Upper

113 100

111 103.0 81.0 121.4

192 18.8 14.3 21.5

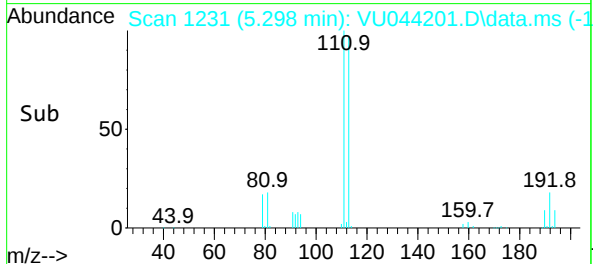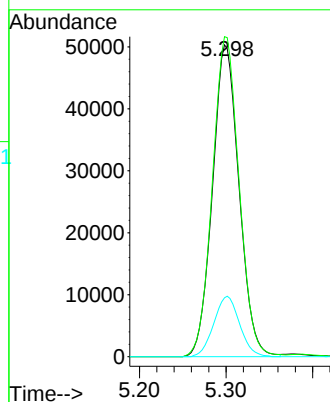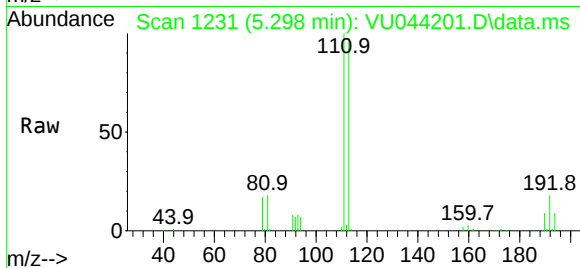

#36

1,1-Dichloropropene

Concen: 4.414 ug/l

RT: 5.385 min Scan# 1258

Delta R.T. -0.148 min

Lab File: VU044201.D

Acq: 14 Jun 2021 23:40




Tgt Ion: 75 Resp: 15520


Ion Ratio Lower Upper

75 100

110 4.2 16.4 49.4#

77 0.0 24.7 37.1#


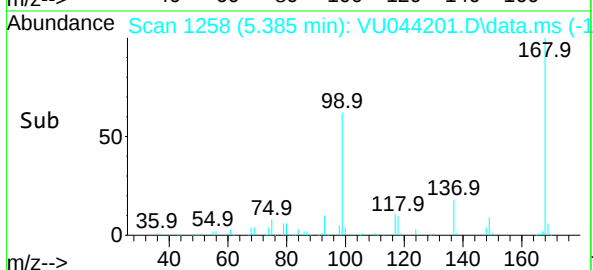
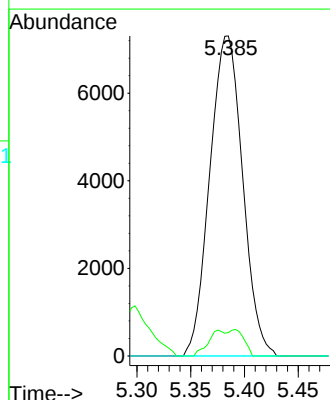
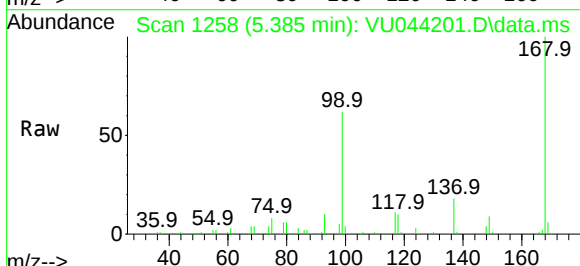




#37
Ethyl Acetate
Concen: 1.090 ug/l
RT: 4.729 min Scan# 1054
Delta R.T. -0.080 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 43 Resp: 4591
Ion Ratio Lower Upper
43 100
61 0.0 11.9 17.9#
70 0.0 9.4 14.0#

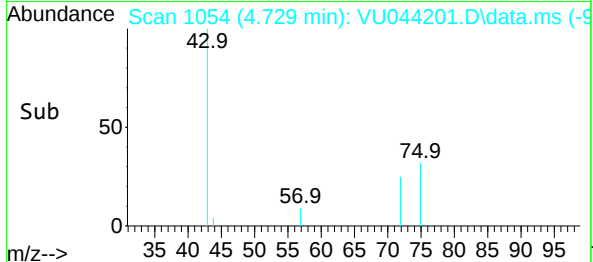

#38
Carbon Tetrachloride
Concen: 6.229 ug/l
RT: 5.385 min Scan# 1258
Delta R.T. -0.148 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Tgt Ion: 117 Resp: 19773
Ion Ratio Lower Upper
117 100
119 6.3 76.6 114.8#
121 0.0 24.6 36.8#

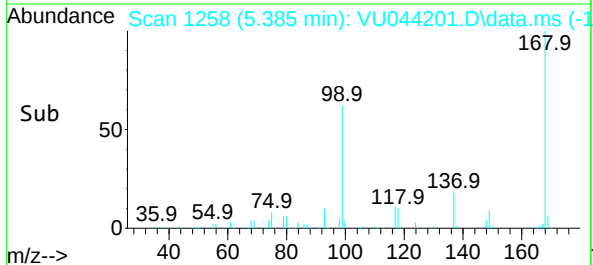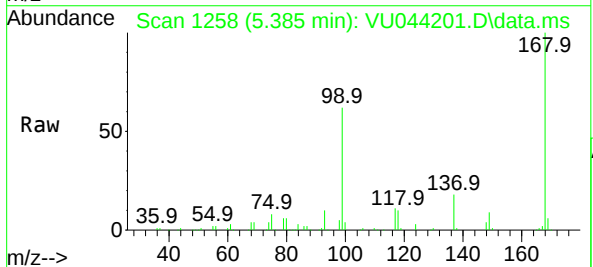



#41

Methacrylonitrile

Concen: 0.284 ug/l

RT: 5.089 min Scan# 1166

Delta R.T. 0.109 min

Lab File: VU044201.D

Acq: 14 Jun 2021 23:40

Tgt Ion: 41 Resp: 612





Ion Ratio Lower Upper

41 100

39 3.3 41.4 62.0#

67 0.0 62.6 93.8#

52 0.0 24.1 36.1#

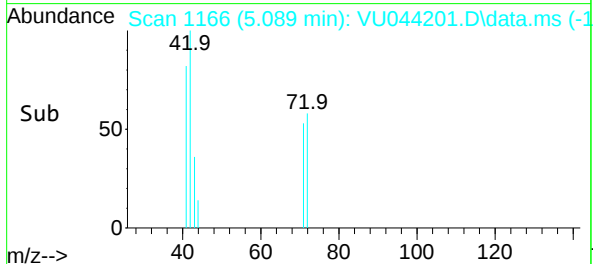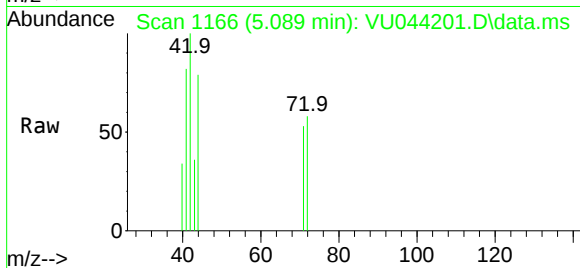

#43

Isopropyl Acetate

Concen: 2.957 ug/l

RT: 5.922 min Scan# 1425

Delta R.T. 0.003 min

Lab File: VU044201.D

Acq: 14 Jun 2021 23:40




Tgt Ion: 43 Resp: 17667


Ion Ratio Lower Upper

43 100

61 23.3 17.8 26.8

87 14.0 11.1 16.7

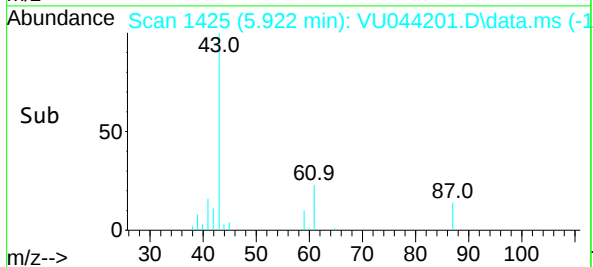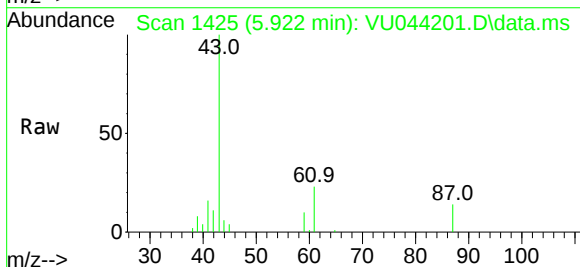







#45

1,2-Dichloropropane
Concen: 0.557 ug/l
RT: 7.047 min Scan# 1775
Delta R.T. 0.247 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Instrument :
MSVOA_U
ClientSampled :




Tgt Ion: 63 Resp: 1575
Ion Ratio Lower Upper
63 100
65 0.0 25.7 38.5#

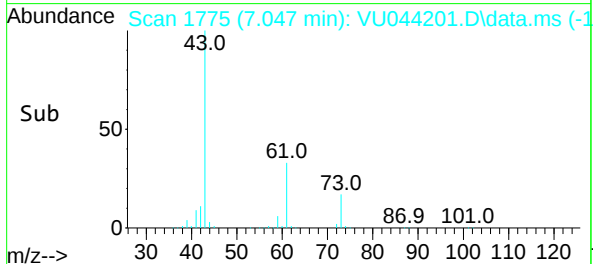


#48

Methyl methacrylate
Concen: 2.285 ug/l
RT: 6.909 min Scan# 1732
Delta R.T. -0.058 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Tgt Ion: 41 Resp: 6644
Ion Ratio Lower Upper
41 100
69 0.0 74.0 111.0#
39 0.0 41.5 62.3#

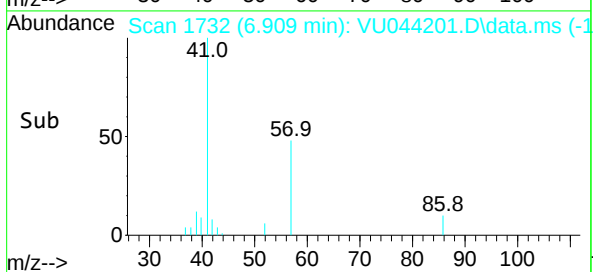



#49

1,4-Dioxane

Concen: 3.064 ug/l

RT: 7.047 min Scan# 1775

Delta R.T. 0.077 min

Lab File: VU044201.D

Acq: 14 Jun 2021 23:40





Tgt Ion: 88 Resp: 233

Ion Ratio Lower Upper

88 100

43 490473.0 23.4 35.0#

58 2590.1 58.1 87.1#

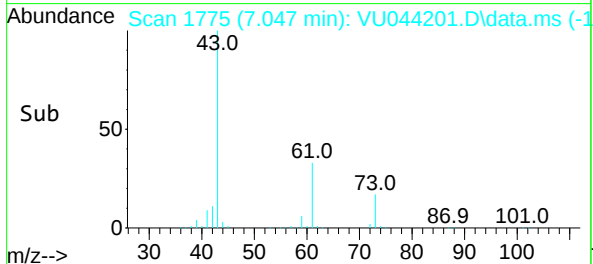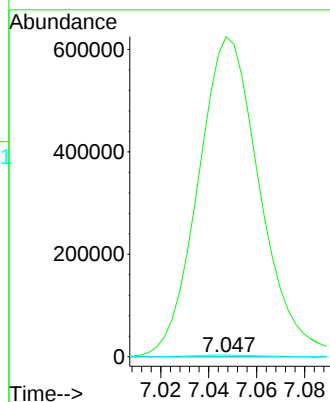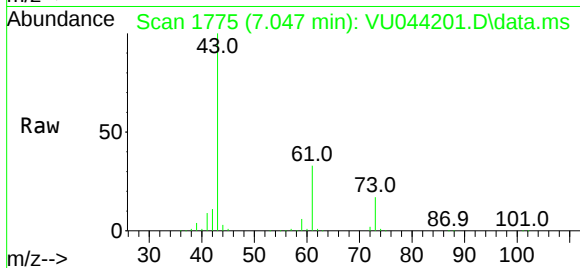

#50

Toluene-d8

Concen: 49.832 ug/l

RT: 7.906 min Scan# 2042

Delta R.T. -0.000 min

Lab File: VU044201.D




Acq: 14 Jun 2021 23:40


Tgt Ion: 98 Resp: 420737

Ion Ratio Lower Upper

98 100

100 65.2 52.2 78.4


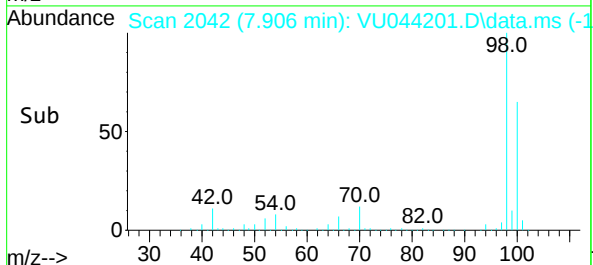
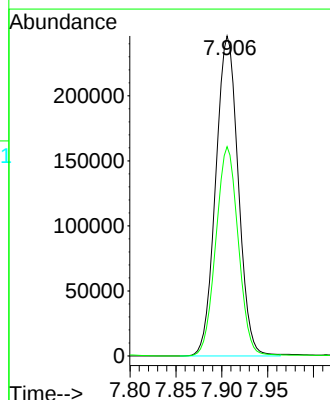
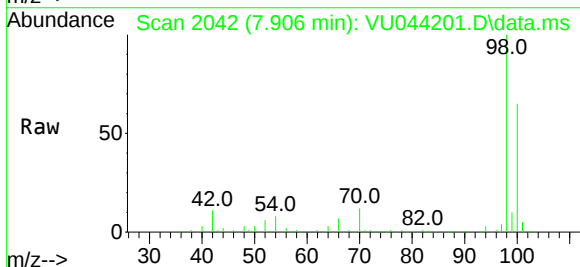




#51
4-Methyl-2-Pentanone
Concen: 1.748 ug/l
RT: 7.800 min Scan# 2009
Delta R.T. -0.000 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 43 Resp: 7557
Ion Ratio Lower Upper
43 100
58 43.9 34.5 51.7



#54
cis-1,3-Dichloropropene
Concen: 7.178 ug/l
RT: 7.745 min Scan# 1992
Delta R.T. 0.132 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Tgt Ion: 75 Resp: 30418
Ion Ratio Lower Upper
75 100
77 0.0 25.9 38.9#
39 29.0 33.2 49.8#

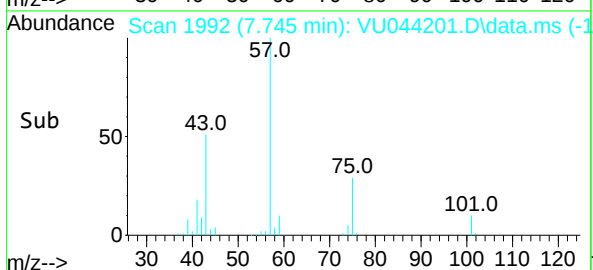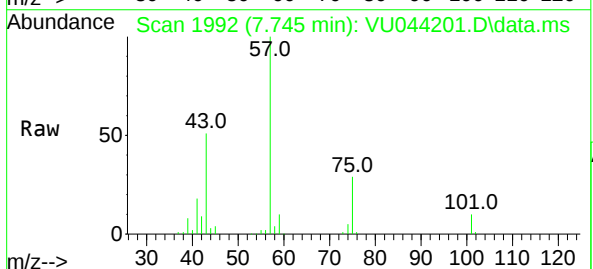

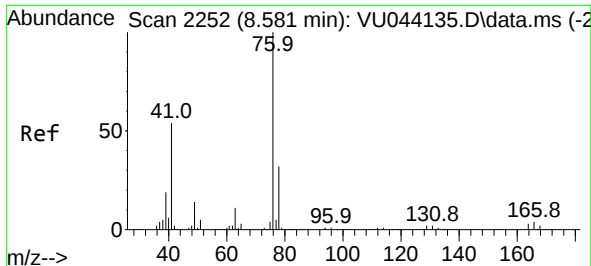

#57

1,3-Dichloropropane

Concen: 4.534 ug/l

RT: 8.735 min Scan# 2300

Delta R.T. 0.154 min

Lab File: VU044201.D





Acq: 14 Jun 2021 23:40

Tgt Ion: 76 Resp: 20864

Ion Ratio Lower Upper

76 100

78 0.0 25.9 38.9#

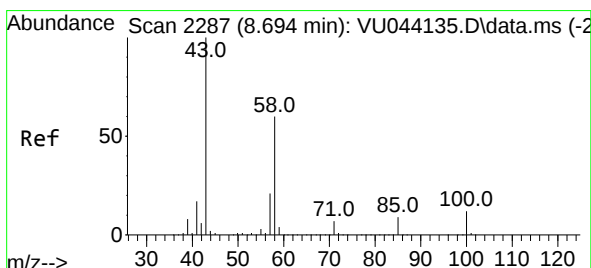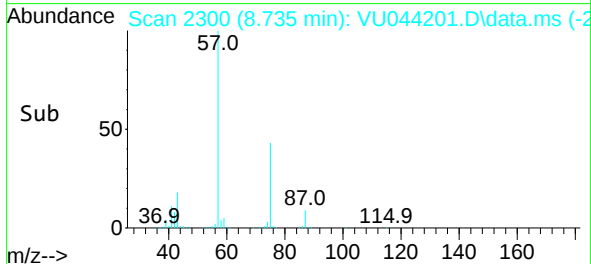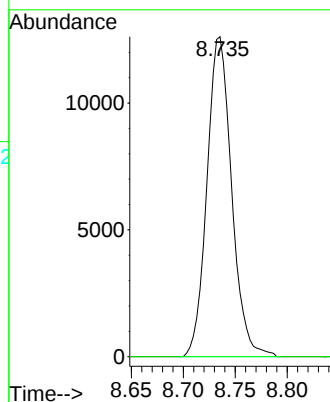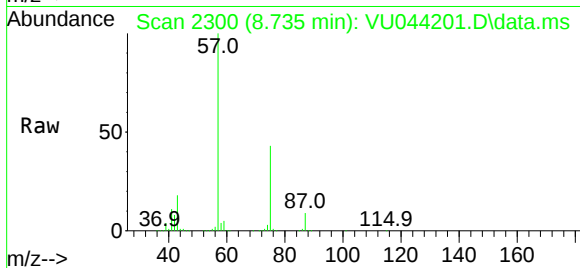

#59

2-Hexanone

Concen: 77.085 ug/l

RT: 8.735 min Scan# 2300

Delta R.T. 0.041 min

Lab File: VU044201.D




Acq: 14 Jun 2021 23:40


Tgt Ion: 43 Resp: 265995

Ion Ratio Lower Upper

43 100

58 22.0 30.0 90.1#


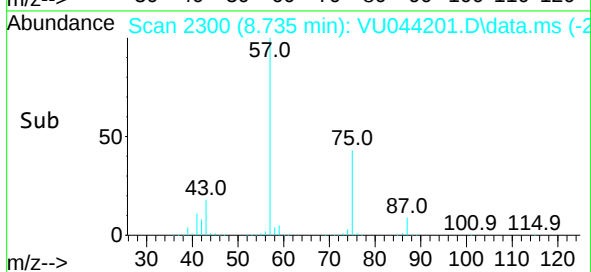
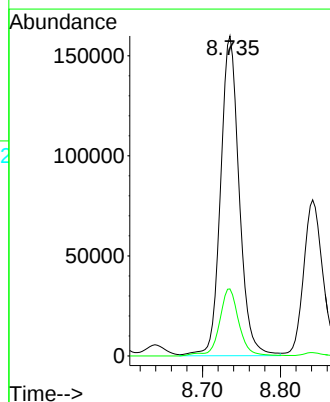
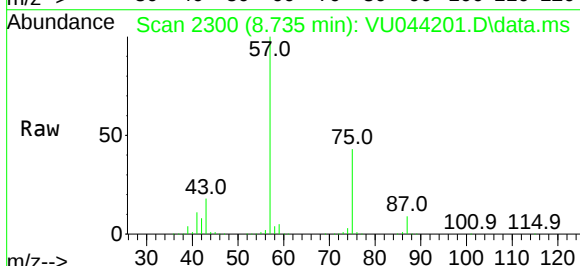


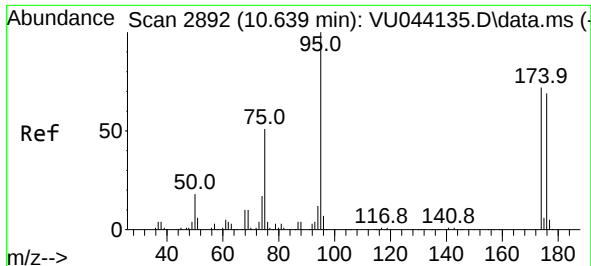

#62
4-Bromofluorobenzene
Concen: 44.552 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.000 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 95 Resp: 150747
Ion Ratio Lower Upper
95 100
174 73.5 0.0 144.4
176 70.8 0.0 138.0

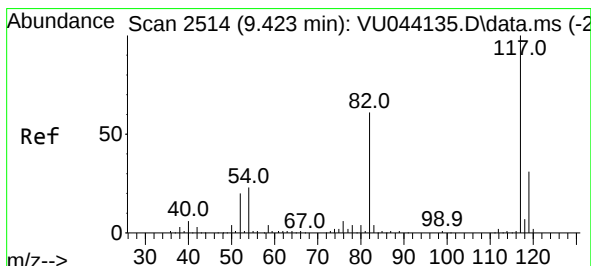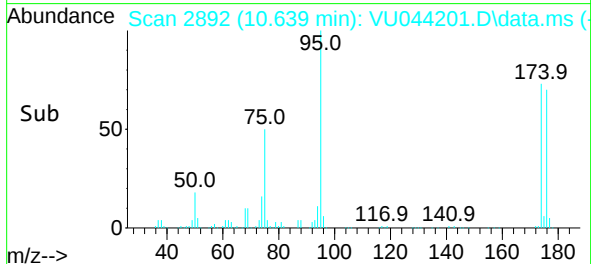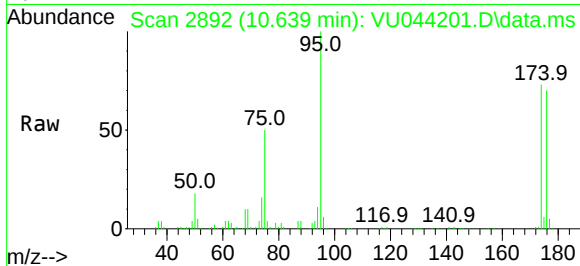

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.423 min Scan# 2514
Delta R.T. -0.000 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Tgt Ion: 117 Resp: 319341
Ion Ratio Lower Upper
117 100
82 59.8 48.8 73.2
119 32.0 25.0 37.6


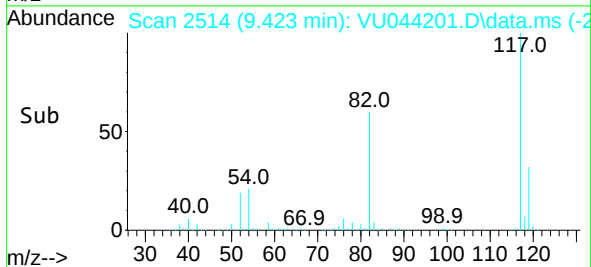

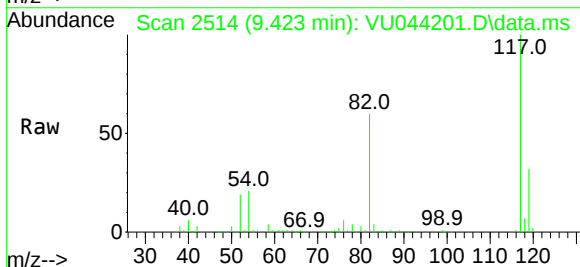


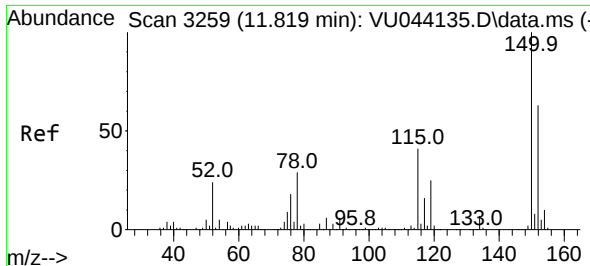

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.819 min Scan# 3259
Delta R.T. -0.000 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion:152 Resp: 150900
Ion Ratio Lower Upper
152 100
115 60.4 43.8 131.3
150 154.7 0.0 350.6

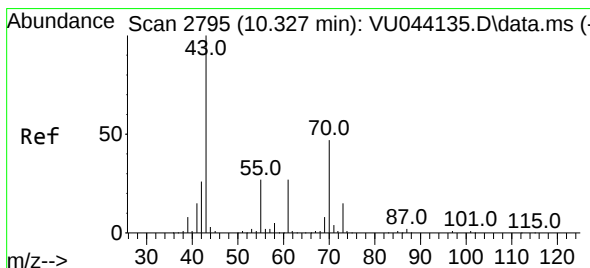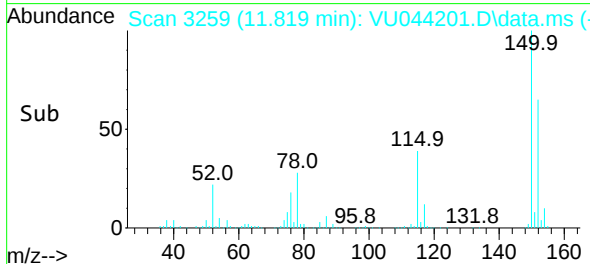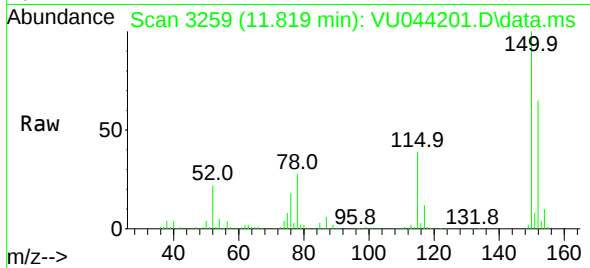

#74
N-ethyl acetate
Concen: 0.312 ug/l
RT: 10.330 min Scan# 2796
Delta R.T. 0.003 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Tgt Ion: 43 Resp: 1418
Ion Ratio Lower Upper
43 100
70 39.9 37.7 56.5
55 19.5 22.4 33.6#
61 15.9 21.5 32.3#


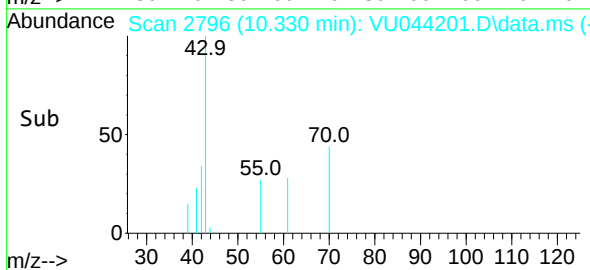

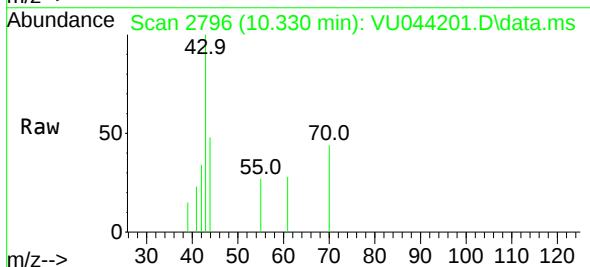


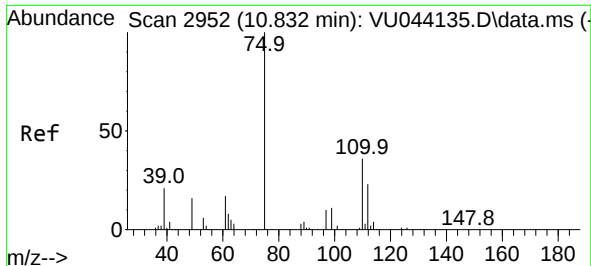

#76
1,2,3-Trichloropropane
Concen: 14.843 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.193 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 75 Resp: 75094
Ion Ratio Lower Upper
75 100
77 1.2 14.9 44.5#

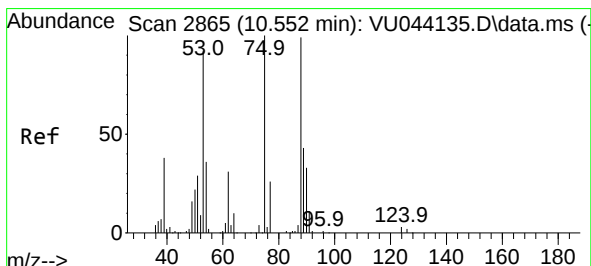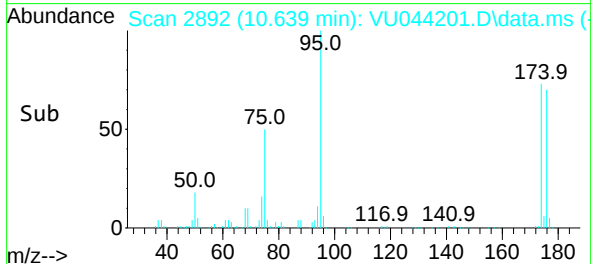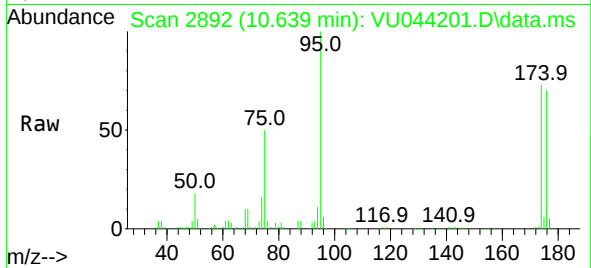

#81
trans-1,4-Dichloro-2-butene
Concen: 53.804 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. 0.087 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Tgt Ion: 75 Resp: 75094
Ion Ratio Lower Upper
75 100
53 0.0 74.2 111.2#
89 0.0 35.0 52.6#


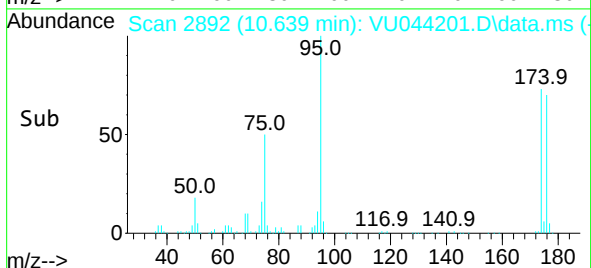

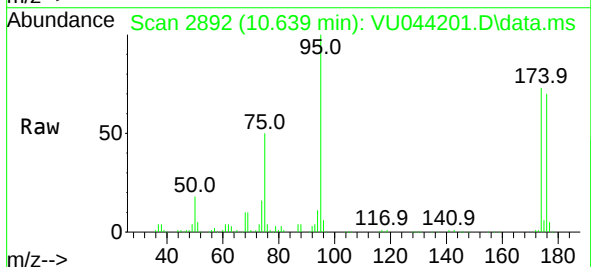


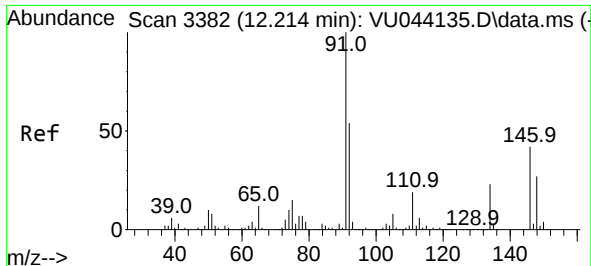

#89
n-Butylbenzene
Concen: 0.209 ug/l
RT: 12.217 min Scan# 3383
Delta R.T. 0.003 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 91 Resp: 2018
Ion Ratio Lower Upper
91 100
92 53.4 27.1 81.2
134 20.7 11.9 35.5

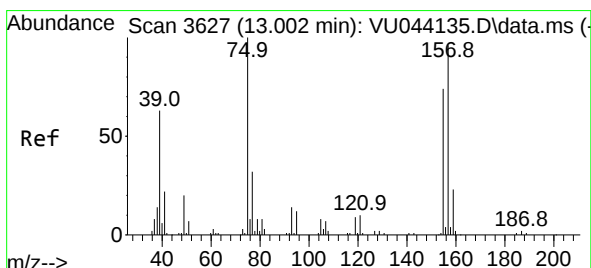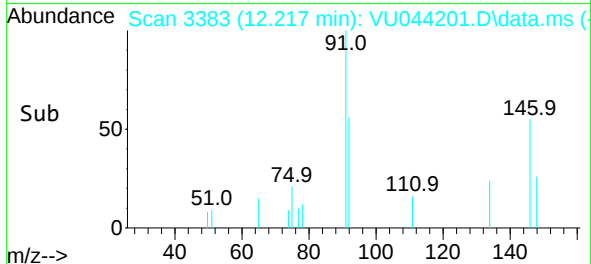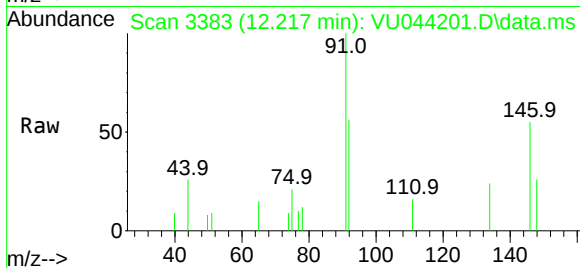

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.219 ug/l
RT: 13.005 min Scan# 3628
Delta R.T. 0.003 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Tgt Ion: 75 Resp: 218
Ion Ratio Lower Upper
75 100
155 27.5 38.2 114.6#
157 92.7 48.3 144.9


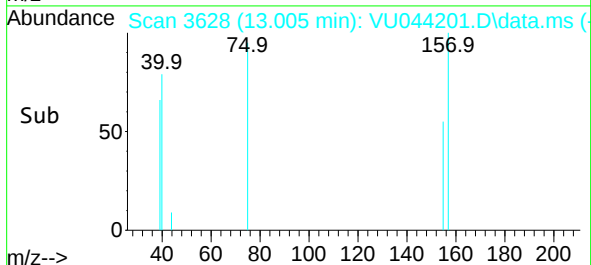

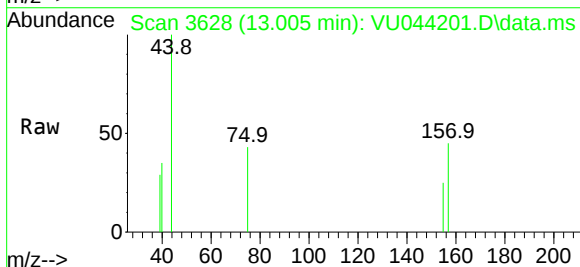


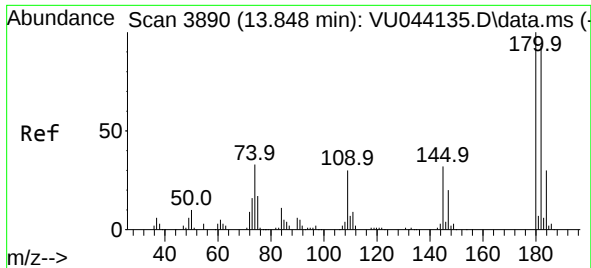

#93
1,2,4-Trichlorobenzene
Concen: 0.560 ug/l
RT: 13.848 min Scan# 3890
Delta R.T. -0.000 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion:180 Resp: 1767
Ion Ratio Lower Upper
180 100
182 93.9 47.3 141.8
145 25.4 16.1 48.2

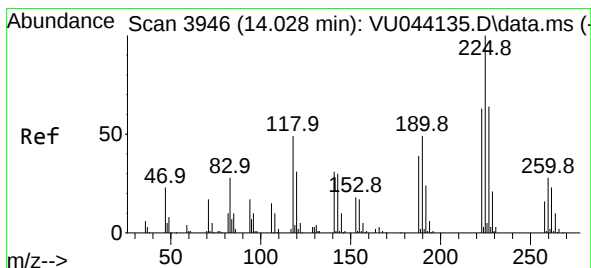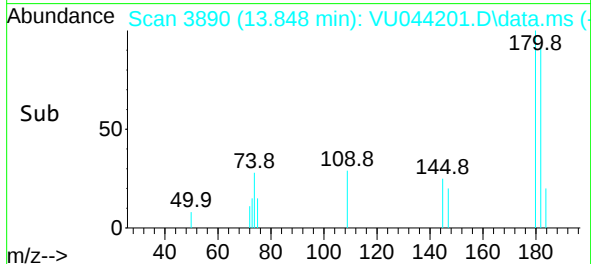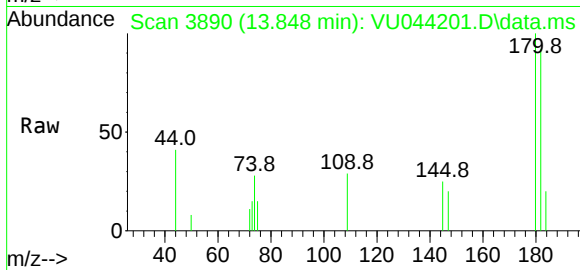

#94
Hexachlorobutadiene
Concen: 0.245 ug/l
RT: 14.031 min Scan# 3947
Delta R.T. 0.003 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Tgt Ion:225 Resp: 415
Ion Ratio Lower Upper
225 100
223 61.7 31.2 93.6
227 49.2 32.2 96.6


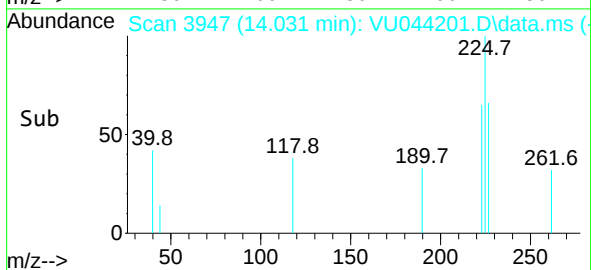

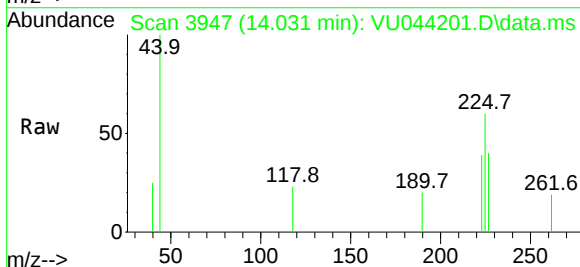


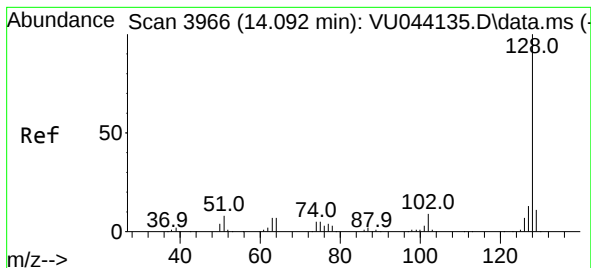

#95
Naphthalene
Concen: 3.659 ug/l
RT: 14.095 min Scan# 3967
Delta R.T. 0.003 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion:128 Resp: 9255
Ion Ratio Lower Upper
128 100
127 13.5 10.2 15.2
129 9.1 8.6 13.0

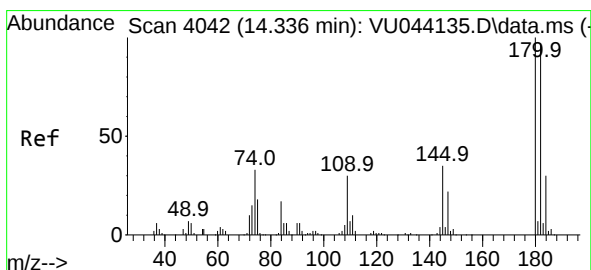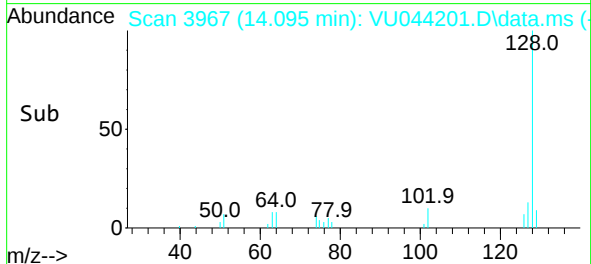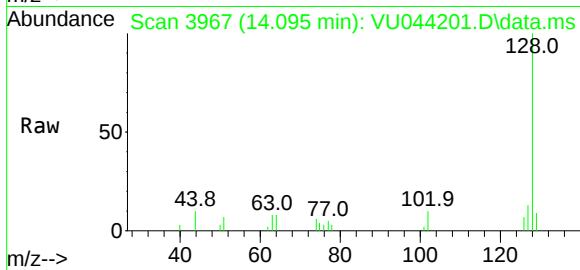

#96
1,2,3-Trichlorobenzene
Concen: 0.620 ug/l
RT: 14.336 min Scan# 4042
Delta R.T. 0.000 min
Lab File: VU044201.D
Acq: 14 Jun 2021 23:40

Tgt Ion:180 Resp: 1898
Ion Ratio Lower Upper
180 100
182 105.1 47.9 143.7
145 31.2 17.2 51.6

