

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU061421\  
 Data File : VU044215.D  
 Acq On : 15 Jun 2021 05:07  
 Operator : SY/MD  
 Sample : M2706-01  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 47 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :

Quant Time: Jun 15 05:39:26 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U060921W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Jun 10 05:11:37 2021  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc        | Units   | Dev(Min) |
|-------------------------------|--------|------|----------|-------------|---------|----------|
| -----                         |        |      |          |             |         |          |
| Internal Standards            |        |      |          |             |         |          |
| 1) Pentafluorobenzene         | 5.385  | 168  | 177180   | 50.000      | ug/l    | 0.00     |
| 34) 1,4-Difluorobenzene       | 6.259  | 114  | 312839   | 50.000      | ug/l    | 0.00     |
| 63) Chlorobenzene-d5          | 9.423  | 117  | 298557   | 50.000      | ug/l    | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 11.819 | 152  | 156706   | 50.000      | ug/l    | 0.00     |
| System Monitoring Compounds   |        |      |          |             |         |          |
| 33) 1,2-Dichloroethane-d4     | 5.713  | 65   | 131838   | 46.791      | ug/l    | 0.00     |
| Spiked Amount                 | 50.000 |      | Recovery | =           | 93.580% |          |
| 35) Dibromofluoromethane      | 5.298  | 113  | 104527   | 48.032      | ug/l    | 0.00     |
| Spiked Amount                 | 50.000 |      | Recovery | =           | 96.060% |          |
| 50) Toluene-d8                | 7.906  | 98   | 390806   | 46.760      | ug/l    | 0.00     |
| Spiked Amount                 | 50.000 |      | Recovery | =           | 93.520% |          |
| 62) 4-Bromofluorobenzene      | 10.639 | 95   | 142779   | 42.629      | ug/l    | 0.00     |
| Spiked Amount                 | 50.000 |      | Recovery | =           | 85.260% |          |
| Target Compounds              |        |      |          |             |         |          |
|                               |        |      |          |             | Qvalue  |          |
| 3) Chloromethane              | 1.523  | 50   | 302      | Below Cal   |         | 97       |
| 4) Vinyl Chloride             | 1.610  | 62   | 2456     | 0.824 ug/l  |         | 97       |
| 6) Chloroethane               | 1.912  | 64   | 35       | Below Cal   | #       | 42       |
| 16) Acetone                   | 2.658  | 43   | 10788    | 5.319 ug/l  |         | 100      |
| 18) Methyl Acetate            | 2.973  | 43   | 1011     | 0.279 ug/l  | #       | 67       |
| 21) trans-1,2-Dichloroethene  | 3.366  | 96   | 537      | 0.223 ug/l  | #       | 89       |
| 25) 2-Butanone                | 4.735  | 43   | 1851     | 0.787 ug/l  |         | 100      |
| 27) cis-1,2-Dichloroethene    | 4.677  | 96   | 10907    | 4.063 ug/l  |         | 87       |
| 28) Bromochloromethane        | 5.095  | 49   | 588      | 0.265 ug/l  | #       | 17       |
| 30) Chloroform                | 5.099  | 83   | 8808     | 1.939 ug/l  |         | 97       |
| 31) Cyclohexane               | 5.385  | 56   | 3624     | 0.911 ug/l  | #       | 1        |
| 36) 1,1-Dichloropropene       | 5.385  | 75   | 14590    | 4.192 ug/l  | #       | 50       |
| 38) Carbon Tetrachloride      | 5.385  | 117  | 18499    | 5.887 ug/l  | #       | 17       |
| 43) Isopropyl Acetate         | 6.054  | 43   | 8401     | 1.421 ug/l  | #       | 58       |
| 44) Trichloroethene           | 6.552  | 130  | 13494    | 5.678 ug/l  |         | 99       |
| 48) Methyl methacrylate       | 7.060  | 41   | 862      | 0.300 ug/l  | #       | 36       |
| 76) 1,2,3-Trichloropropane    | 10.639 | 75   | 70388    | 13.397 ug/l | #       | 47       |
| 78) n-propylbenzene           | 10.912 | 91   | 3949     | 0.289 ug/l  |         | 95       |
| 80) 1,3,5-Trimethylbenzene    | 11.095 | 105  | 12488    | 1.338 ug/l  |         | 99       |
| 81) trans-1,4-Dichloro-2-b... | 10.639 | 75   | 70388    | 48.564 ug/l | #       | 13       |
| 83) tert-Butylbenzene         | 11.426 | 119  | 4344     | 0.496 ug/l  |         | 90       |
| 84) 1,2,4-Trimethylbenzene    | 11.475 | 105  | 19918    | 2.124 ug/l  |         | 99       |
| 85) sec-Butylbenzene          | 11.648 | 105  | 4031     | 0.350 ug/l  |         | 93       |
| 86) p-Isopropyltoluene        | 11.748 | 119  | 6369     | 0.646 ug/l  |         | 98       |
| 89) n-Butylbenzene            | 12.211 | 91   | 5895     | 0.589 ug/l  | #       | 37       |
| 90) Hexachloroethane          | 12.471 | 117  | 688      | 0.441 ug/l  | #       | 14       |
| 95) Naphthalene               | 14.098 | 128  | 459      | 2.875 ug/l  | #       | 69       |
| -----                         |        |      |          |             |         |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU061421\  
Data File : VU044215.D  
Acq On : 15 Jun 2021 05:07  
Operator : SY/MD  
Sample : M2706-01  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 47 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :

Quant Time: Jun 15 05:39:26 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U060921W.M  
Quant Title : SW846 8260  
QLast Update : Thu Jun 10 05:11:37 2021  
Response via : Initial Calibration




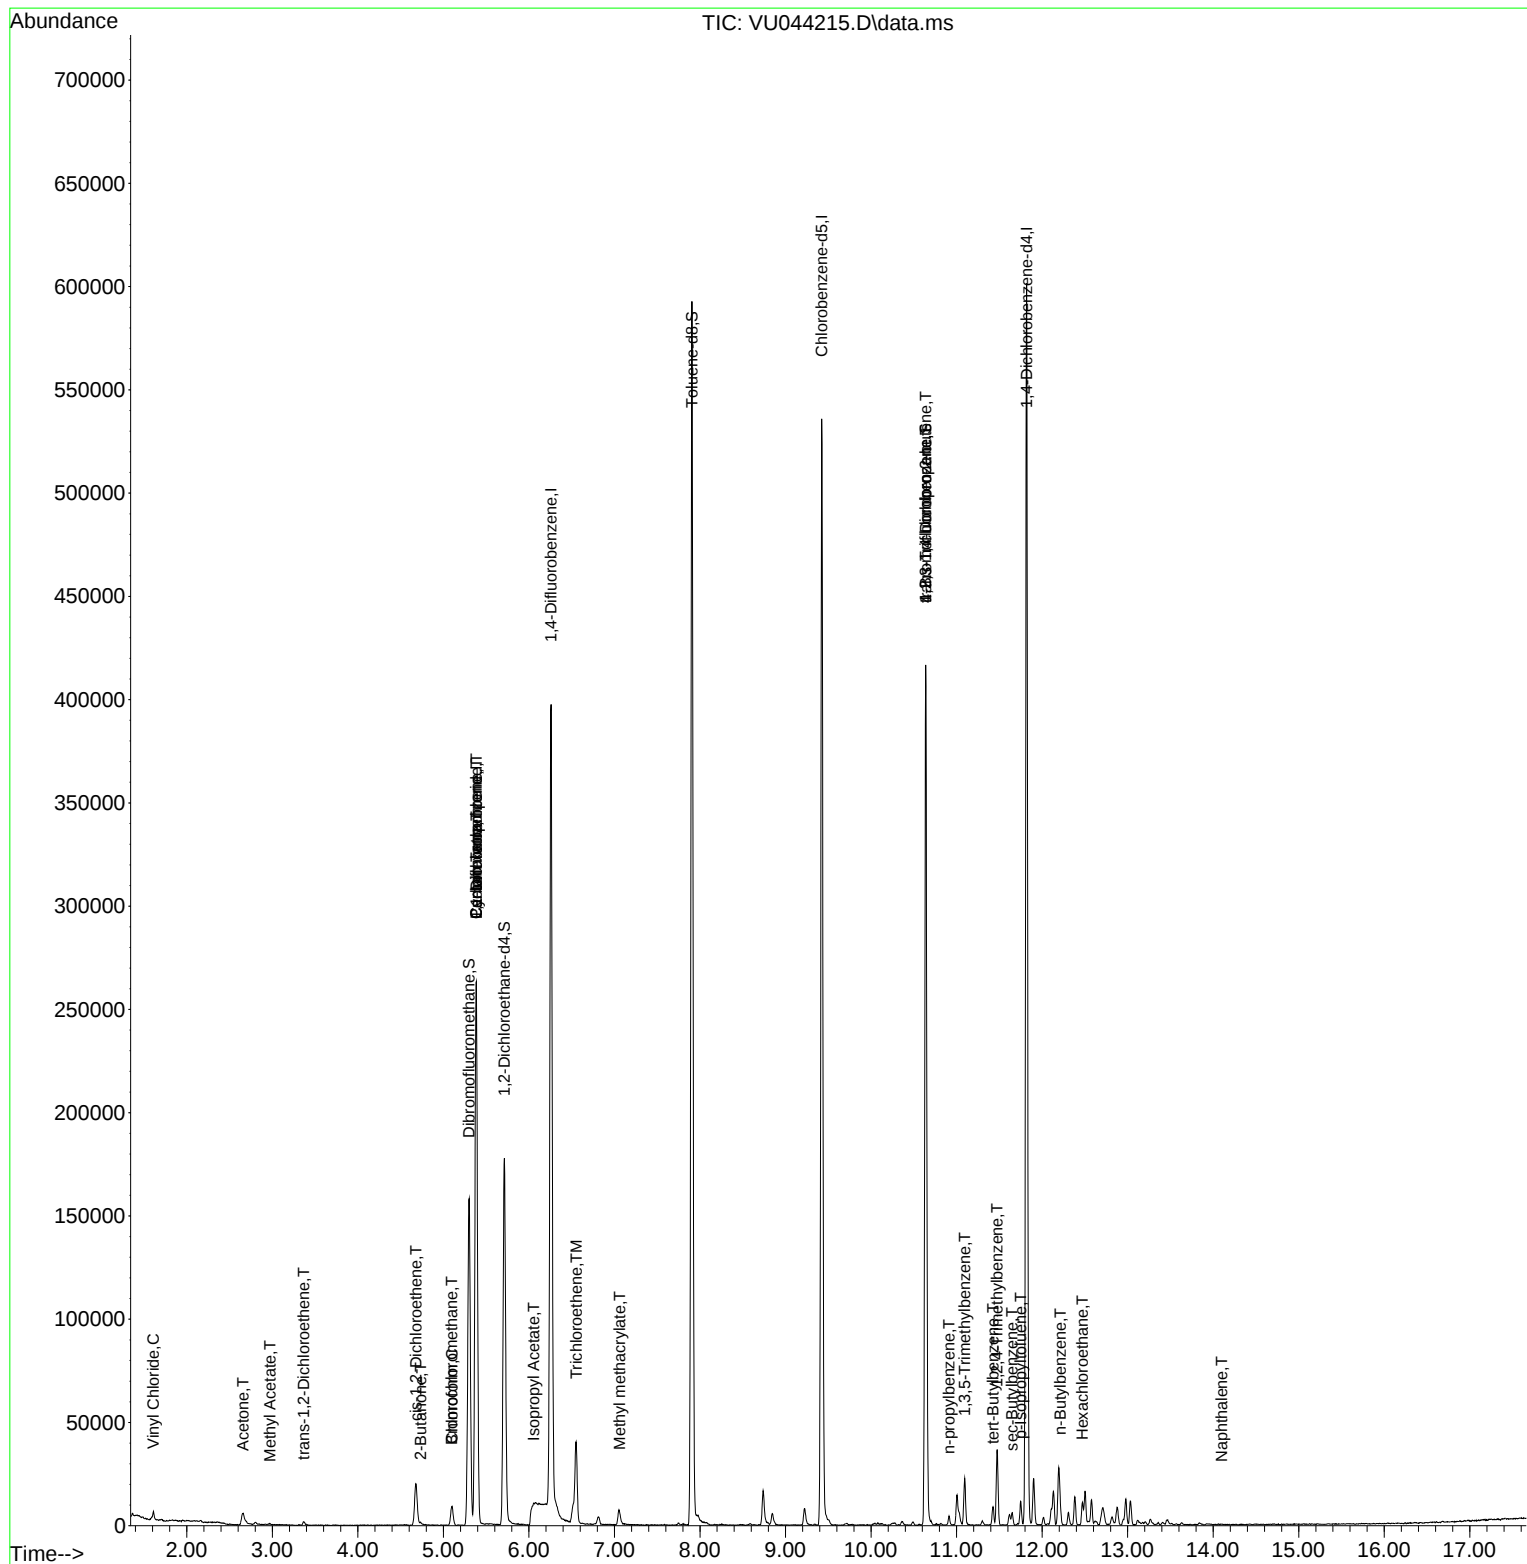




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.385 min Scan# 1258  
Delta R.T. 0.003 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion:168 Resp: 177180  
Ion Ratio Lower Upper  
168 100  
99 60.1 51.3 76.9

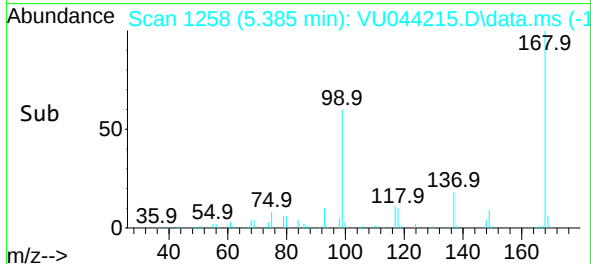

#3  
Chloromethane  
Concen: Below Cal  
RT: 1.523 min Scan# 57  
Delta R.T. 0.000 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07

Tgt Ion: 50 Resp: 302  
Ion Ratio Lower Upper  
50 100  
52 34.9 26.6 39.8


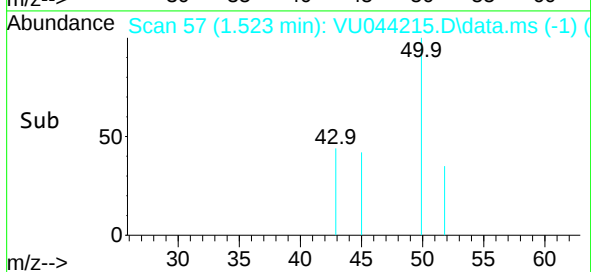




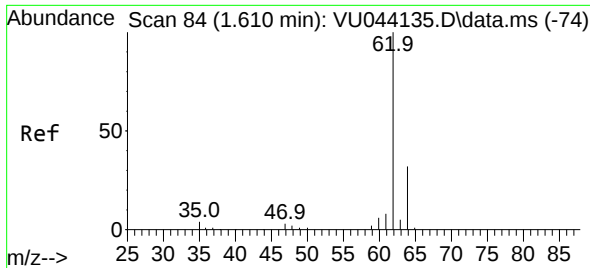

#4  
 Vinyl Chloride  
 Concen: 0.824 ug/l  
 RT: 1.610 min Scan# 84  
 Delta R.T. 0.000 min  
 Lab File: VU044215.D  
 Acq: 15 Jun 2021 05:07




Instrument :  
 MSVOA\_U  
 ClientSampleId :


Tgt Ion: 62 Resp: 2456  
 Ion Ratio Lower Upper  
 62 100  
 64 33.4 25.5 38.3

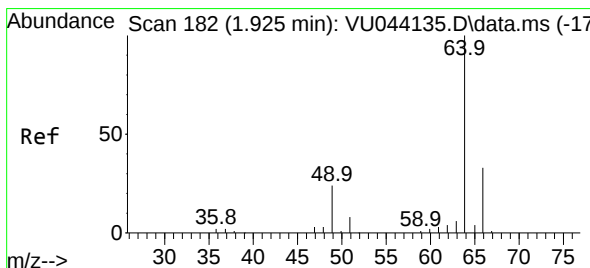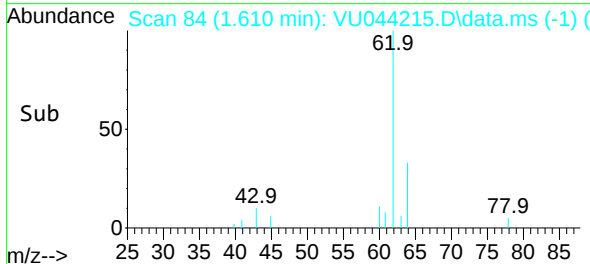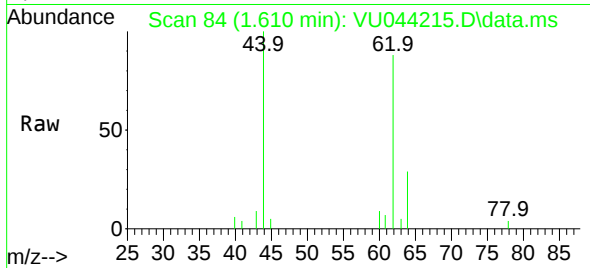

#6  
 Chloroethane  
 Concen: Below Cal  
 RT: 1.912 min Scan# 178  
 Delta R.T. -0.013 min  
 Lab File: VU044215.D  
 Acq: 15 Jun 2021 05:07

Tgt Ion: 64 Resp: 35  
 Ion Ratio Lower Upper  
 64 100  
 66 0.0 26.1 39.1#


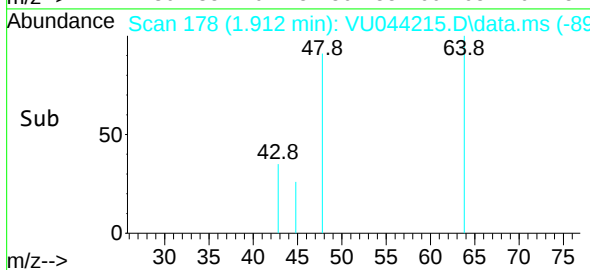

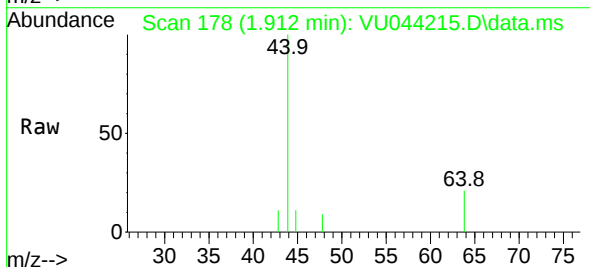




#16  
Acetone  
Concen: 5.319 ug/l  
RT: 2.658 min Scan# 410  
Delta R.T. 0.025 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion: 43 Resp: 10788  
Ion Ratio Lower Upper  
43 100  
58 35.2 28.0 42.0

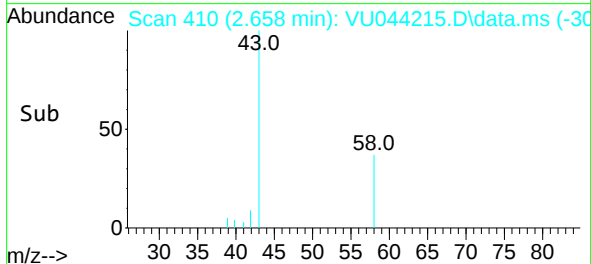

#18  
Methyl Acetate  
Concen: 0.279 ug/l  
RT: 2.973 min Scan# 508  
Delta R.T. 0.019 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07


Tgt Ion: 43 Resp: 1011  
Ion Ratio Lower Upper  
43 100  
74 8.7 20.3 30.5#

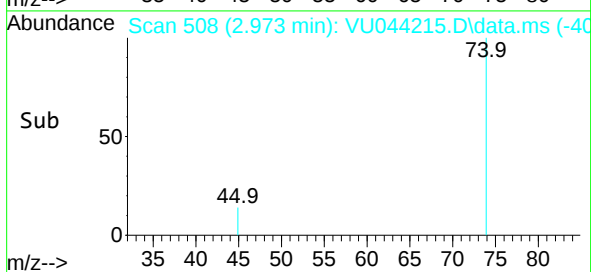






#21  
trans-1,2-Dichloroethene  
Concen: 0.223 ug/l  
RT: 3.366 min Scan# 630  
Delta R.T. 0.007 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07


Instrument :  
MSVOA\_U  
ClientSampleId :

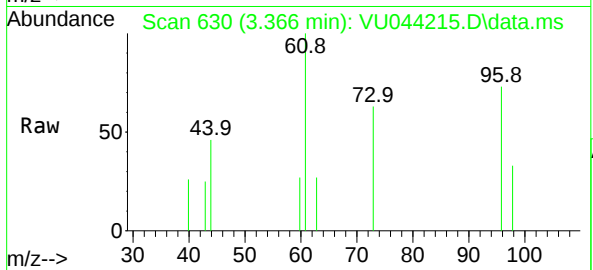



Tgt Ion: 96 Resp: 537  
Ion Ratio Lower Upper  
96 100  
61 137.3 116.3 174.5  
98 45.8 50.7 76.1#

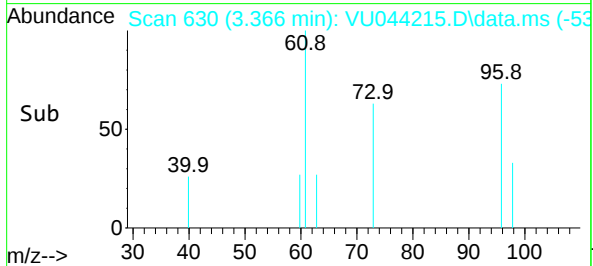


#25  
2-Butanone  
Concen: 0.787 ug/l  
RT: 4.735 min Scan# 1056  
Delta R.T. 0.025 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07

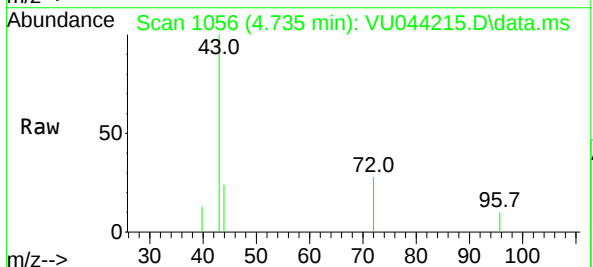

Tgt Ion: 43 Resp: 1851  
Ion Ratio Lower Upper  
43 100  
72 28.5 22.6 33.8









#27

cis-1,2-Dichloroethene  
Concen: 4.063 ug/l  
RT: 4.677 min Scan# 1038  
Delta R.T. 0.003 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07

Instrument :  
MSVOA\_U  
ClientSampleId :




|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 96    | Resp: | 10907 |
| Ion      | Ratio | Lower | Upper |
| 96       | 100   |       |       |
| 61       | 131.7 | 0.0   | 308.0 |
| 98       | 65.8  | 0.0   | 128.4 |

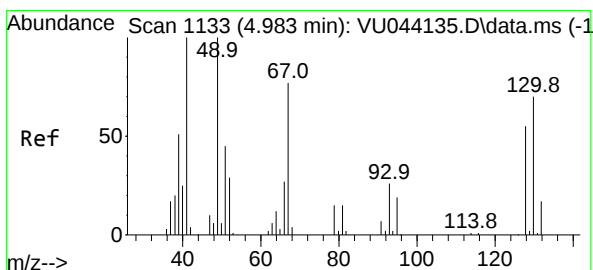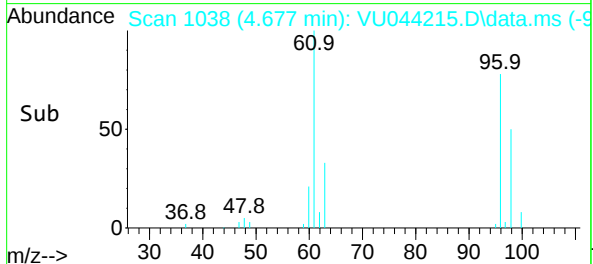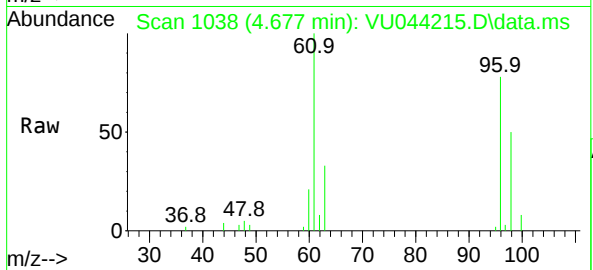


#28

Bromochloromethane  
Concen: 0.265 ug/l  
RT: 5.095 min Scan# 1168  
Delta R.T. 0.112 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 49    | Resp: | 588   |
| Ion      | Ratio | Lower | Upper |
| 49       | 100   |       |       |
| 129      | 0.0   | 0.0   | 3.2   |
| 130      | 0.0   | 55.6  | 83.4# |

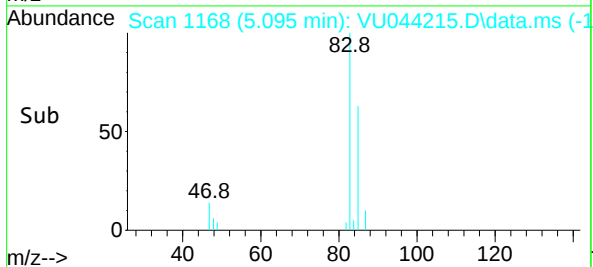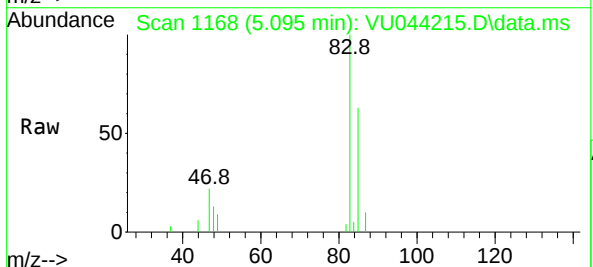



#30

Chloroform

Concen: 1.939 ug/l

RT: 5.099 min Scan# 1169

Delta R.T. 0.003 min

Lab File: VU044215.D





Acq: 15 Jun 2021 05:07

Tgt Ion: 83 Resp: 8808

Ion Ratio Lower Upper

83 100

85 62.8 51.8 77.8

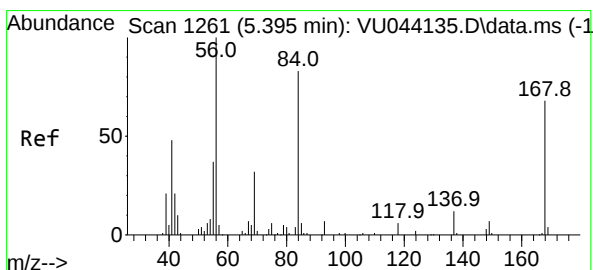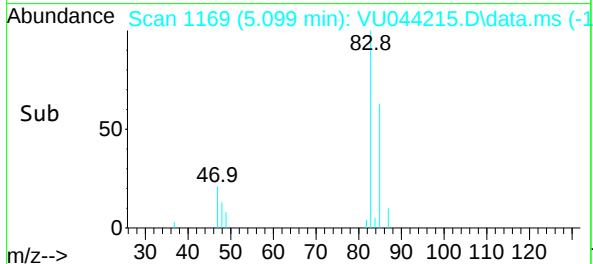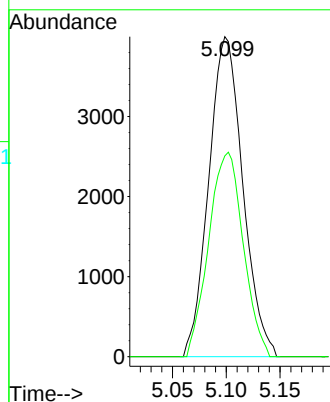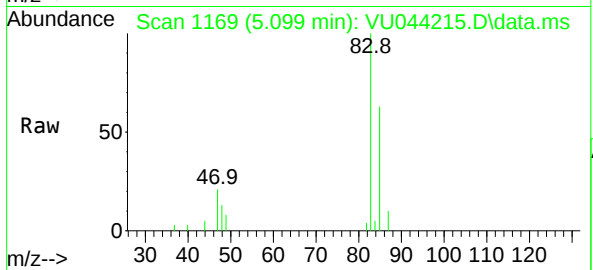

#31

Cyclohexane

Concen: 0.911 ug/l

RT: 5.385 min Scan# 1258

Delta R.T. -0.010 min

Lab File: VU044215.D

Acq: 15 Jun 2021 05:07




Tgt Ion: 56 Resp: 3624


Ion Ratio Lower Upper

56 100

69 193.2 25.5 38.3#

84 167.2 66.3 99.5#


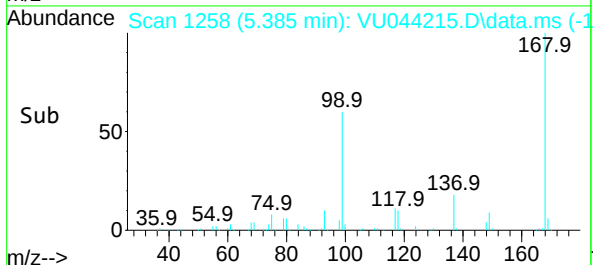
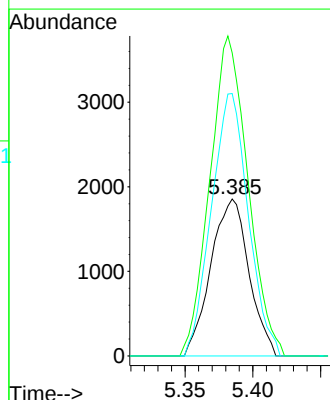
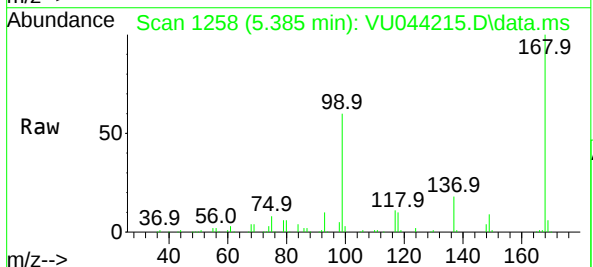


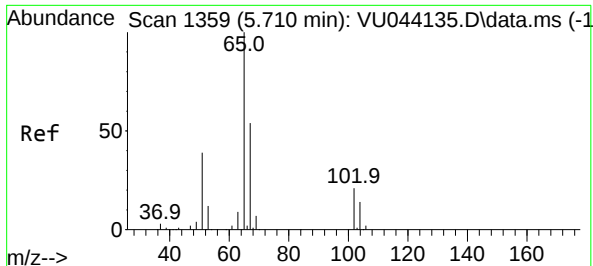

#33  
1,2-Dichloroethane-d4  
Concen: 46.791 ug/l  
RT: 5.713 min Scan# 1360  
Delta R.T. 0.003 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion: 65 Resp: 131838  
Ion Ratio Lower Upper  
65 100  
67 53.6 0.0 106.6

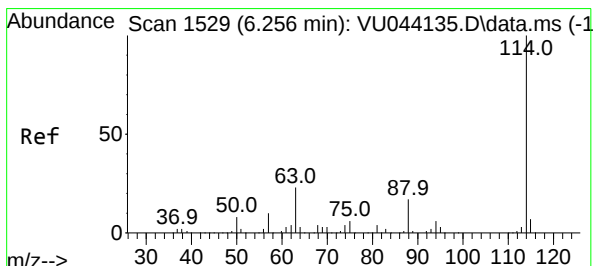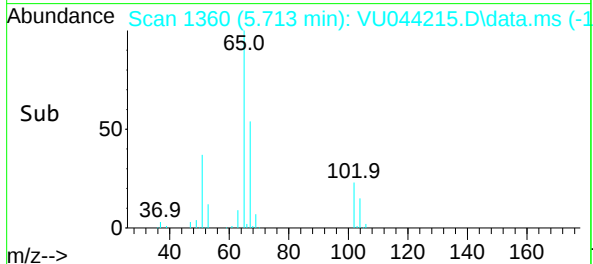

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.259 min Scan# 1530  
Delta R.T. 0.003 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07


Tgt Ion: 114 Resp: 312839  
Ion Ratio Lower Upper  
114 100  
63 21.2 0.0 45.8  
88 16.8 0.0 34.0

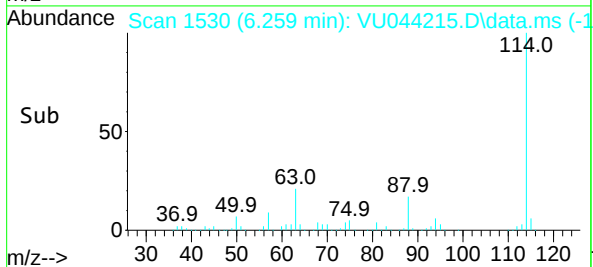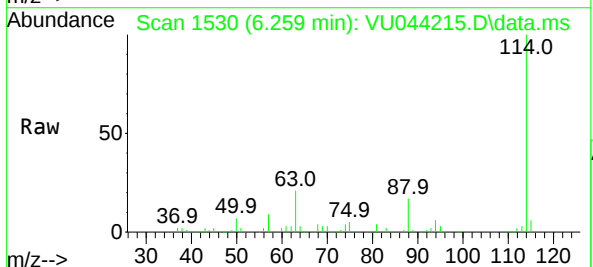



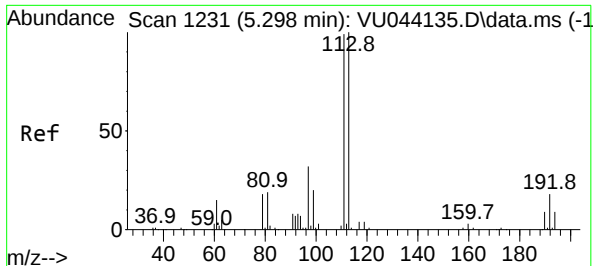


#35  
Dibromofluoromethane  
Concen: 48.032 ug/l  
RT: 5.298 min Scan# 1231  
Delta R.T. -0.000 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07


Instrument :  
MSVOA\_U  
ClientSampleId :





Tgt Ion:113 Resp: 104527  
Ion Ratio Lower Upper  
113 100  
111 102.9 81.0 121.4  
192 19.0 14.3 21.5

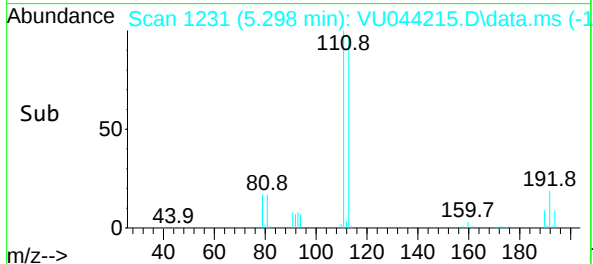


#36  
1,1-Dichloropropene  
Concen: 4.192 ug/l  
RT: 5.385 min Scan# 1258  
Delta R.T. -0.148 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07

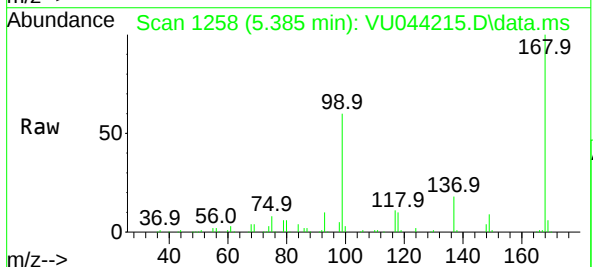


Tgt Ion: 75 Resp: 14590  
Ion Ratio Lower Upper  
75 100  
110 8.3 16.4 49.4#  
77 0.0 24.7 37.1#

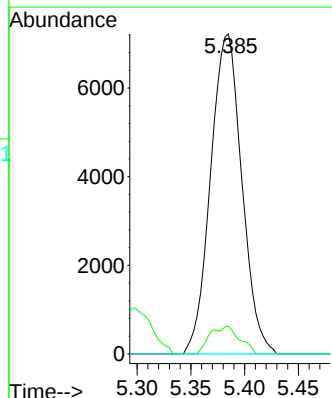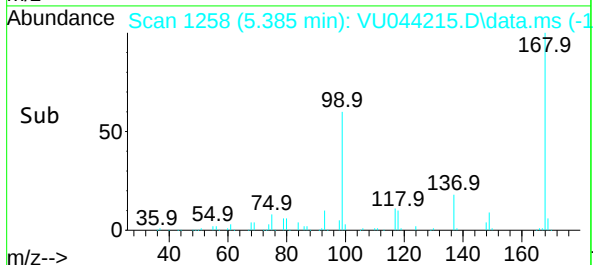



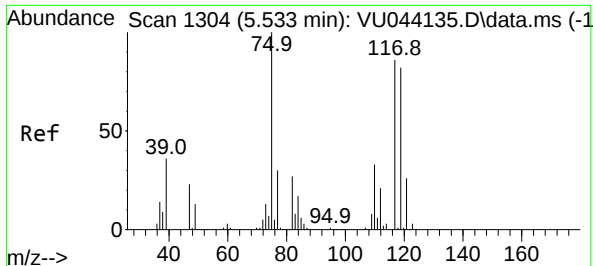


#38  
Carbon Tetrachloride  
Concen: 5.887 ug/l  
RT: 5.385 min Scan# 1258  
Delta R.T. -0.148 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07


Instrument :  
MSVOA\_U  
ClientSampleId :

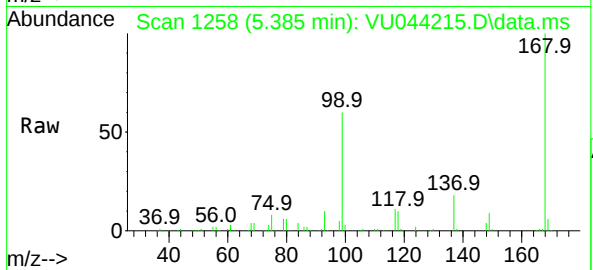



Tgt Ion:117 Resp: 18499  
Ion Ratio Lower Upper  
117 100  
119 6.1 76.6 114.8#  
121 0.0 24.6 36.8#

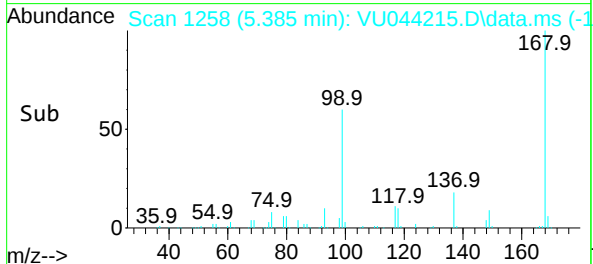


#43  
Isopropyl Acetate  
Concen: 1.421 ug/l  
RT: 6.054 min Scan# 1466  
Delta R.T. 0.135 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07

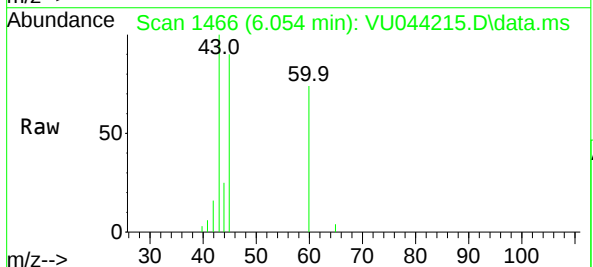

Tgt Ion: 43 Resp: 8401  
Ion Ratio Lower Upper  
43 100  
61 0.0 17.8 26.8#  
87 0.0 11.1 16.7#









#44  
Trichloroethene  
Concen: 5.678 ug/l  
RT: 6.552 min Scan# 1621  
Delta R.T. 0.003 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07




Instrument :  
MSVOA\_U  
ClientSampled :


Tgt Ion:130 Resp: 13494  
Ion Ratio Lower Upper  
130 100  
95 107.2 0.0 212.8

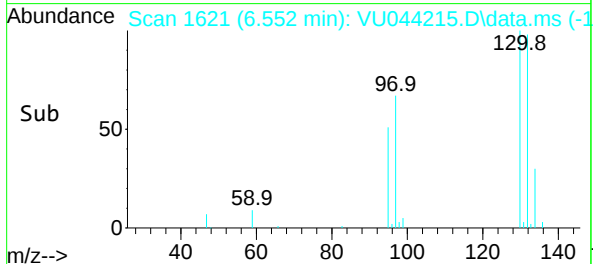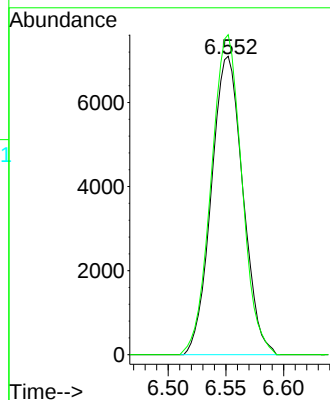

#48  
Methyl methacrylate  
Concen: 0.300 ug/l  
RT: 7.060 min Scan# 1779  
Delta R.T. 0.093 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07

Tgt Ion: 41 Resp: 862  
Ion Ratio Lower Upper  
41 100  
69 0.0 74.0 111.0#  
39 47.3 41.5 62.3


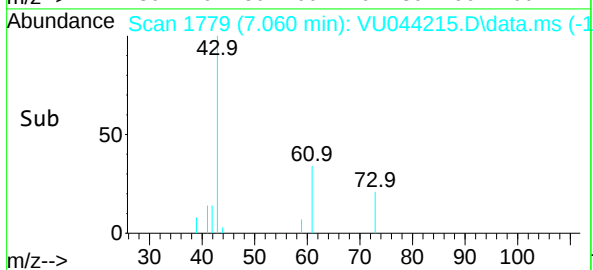
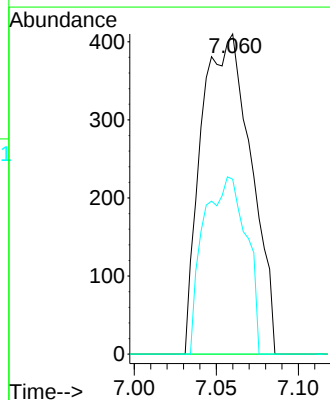
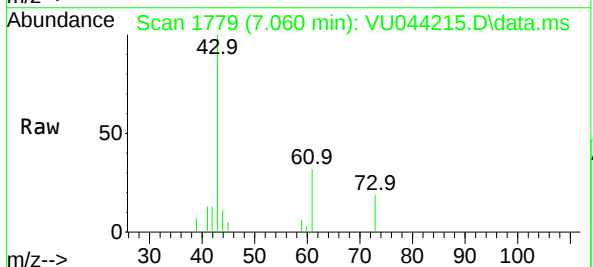




#50  
Toluene-d8  
Concen: 46.760 ug/l  
RT: 7.906 min Scan# 2042  
Delta R.T. -0.000 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07




Instrument :  
MSVOA\_U  
ClientSampled :


Tgt Ion: 98 Resp: 390806  
Ion Ratio Lower Upper  
98 100  
100 64.2 52.2 78.4

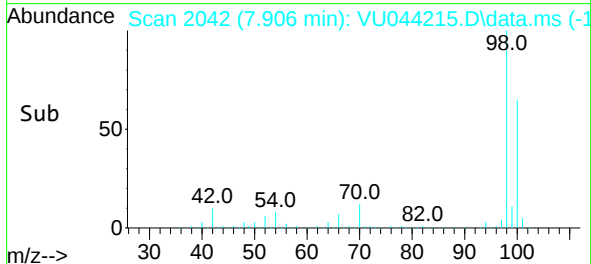

#62  
4-Bromofluorobenzene  
Concen: 42.629 ug/l  
RT: 10.639 min Scan# 2892  
Delta R.T. -0.000 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07

Tgt Ion: 95 Resp: 142779  
Ion Ratio Lower Upper  
95 100  
174 75.4 0.0 144.4  
176 71.5 0.0 138.0


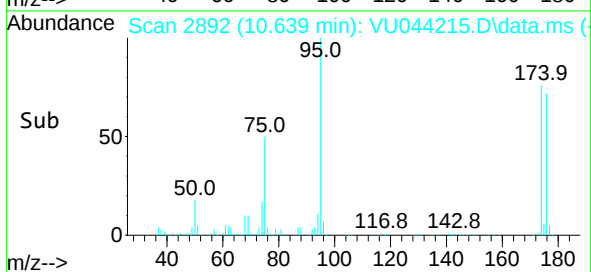

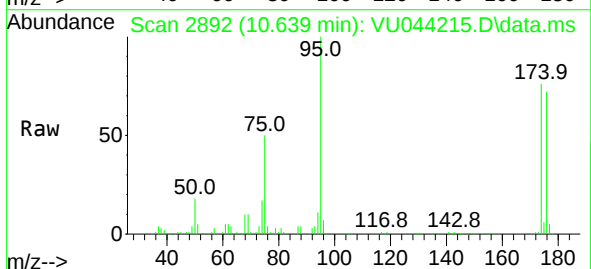




#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 9.423 min Scan# 2514  
Delta R.T. -0.000 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion:117 Resp: 298557  
Ion Ratio Lower Upper  
117 100  
82 58.6 48.8 73.2  
119 32.0 25.0 37.6

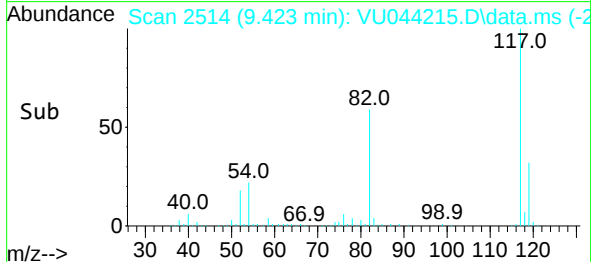

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 11.819 min Scan# 3259  
Delta R.T. -0.000 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07

Tgt Ion:152 Resp: 156706  
Ion Ratio Lower Upper  
152 100  
115 60.4 43.8 131.3  
150 155.8 0.0 350.6


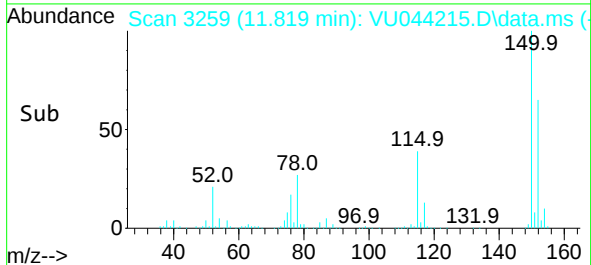

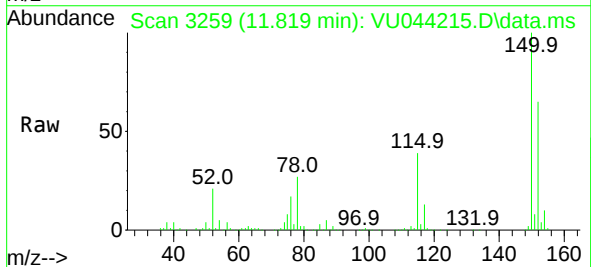




#76  
1,2,3-Trichloropropane  
Concen: 13.397 ug/l  
RT: 10.639 min Scan# 2892  
Delta R.T. -0.193 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion: 75 Resp: 70388  
Ion Ratio Lower Upper  
75 100  
77 1.2 14.9 44.5#

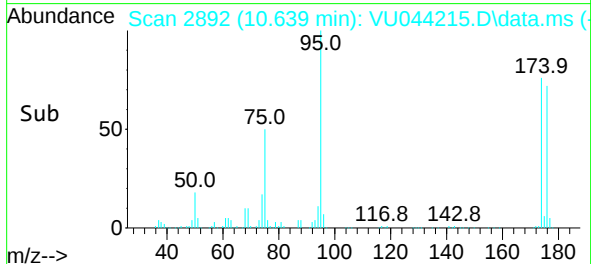

#78  
n-propylbenzene  
Concen: 0.289 ug/l  
RT: 10.912 min Scan# 2977  
Delta R.T. -0.000 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07

Tgt Ion: 91 Resp: 3949  
Ion Ratio Lower Upper  
91 100  
120 19.2 10.8 32.4


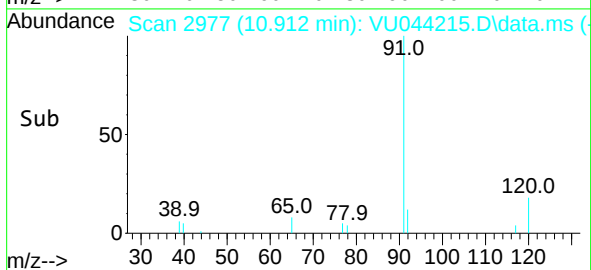

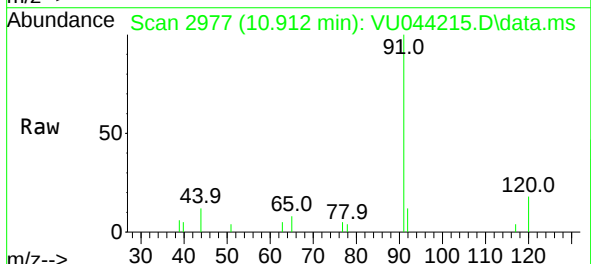




#80  
1,3,5-Trimethylbenzene  
Concen: 1.338 ug/l  
RT: 11.095 min Scan# 3034  
Delta R.T. 0.000 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion:105 Resp: 12488  
Ion Ratio Lower Upper  
105 100  
120 47.6 23.5 70.5

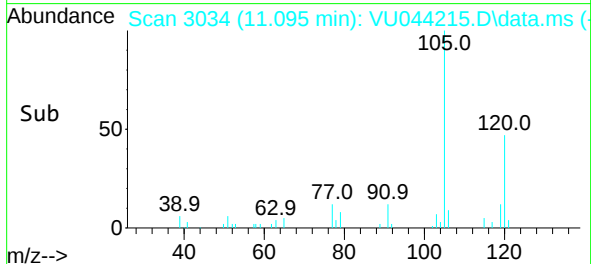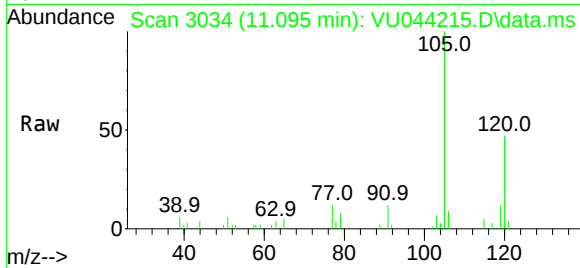

#81  
trans-1,4-Dichloro-2-butene  
Concen: 48.564 ug/l  
RT: 10.639 min Scan# 2892  
Delta R.T. 0.087 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07

Tgt Ion: 75 Resp: 70388  
Ion Ratio Lower Upper  
75 100  
53 0.0 74.2 111.2#  
89 0.0 35.0 52.6#


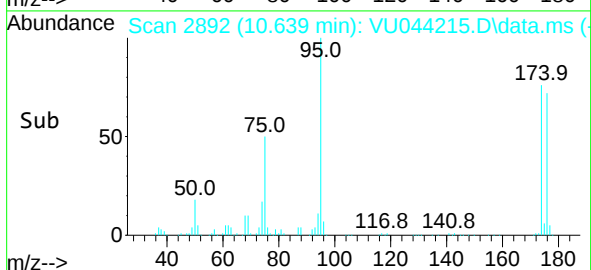

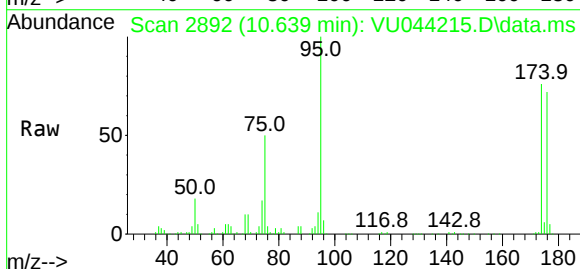




#83  
tert-Butylbenzene  
Concen: 0.496 ug/l  
RT: 11.426 min Scan# 3137  
Delta R.T. -0.001 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07




Instrument :  
MSVOA\_U  
ClientSampled :


Tgt Ion:119 Resp: 4344  
Ion Ratio Lower Upper  
119 100  
91 69.2 30.3 90.8  
134 20.4 11.5 34.5

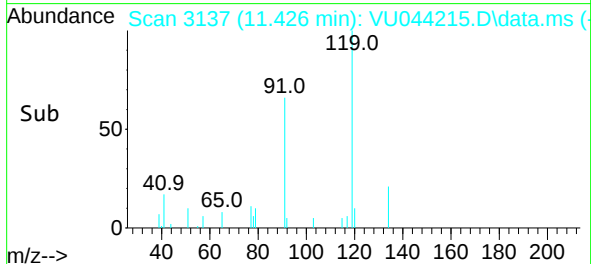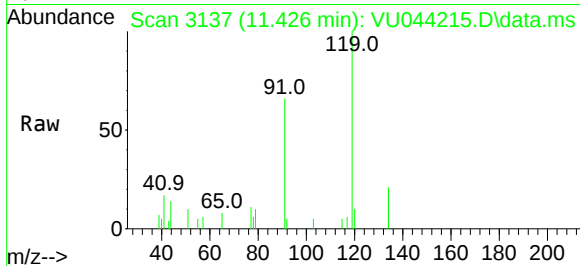

#84  
1,2,4-Trimethylbenzene  
Concen: 2.124 ug/l  
RT: 11.475 min Scan# 3152  
Delta R.T. -0.000 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07

Tgt Ion:105 Resp: 19918  
Ion Ratio Lower Upper  
105 100  
120 44.4 21.9 65.8


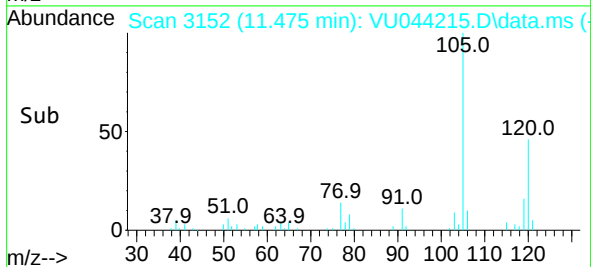

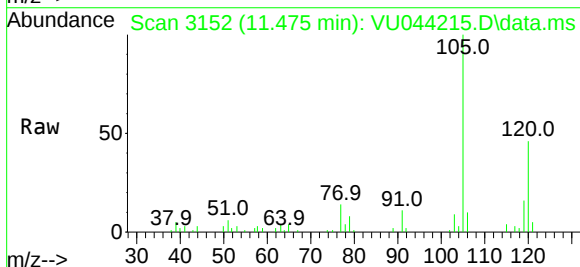




#85  
 sec-Butylbenzene  
 Concen: 0.350 ug/l  
 RT: 11.648 min Scan# 3206  
 Delta R.T. -0.004 min  
 Lab File: VU044215.D  
 Acq: 15 Jun 2021 05:07




Instrument :  
 MSVOA\_U  
 ClientSampleId :


Tgt Ion:105 Resp: 4031  
 Ion Ratio Lower Upper  
 105 100  
 134 15.7 9.4 28.2

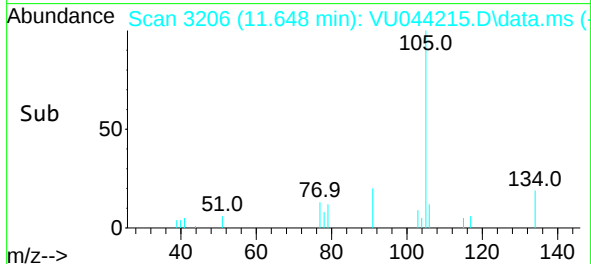

#86  
 p-Isopropyltoluene  
 Concen: 0.646 ug/l  
 RT: 11.748 min Scan# 3237  
 Delta R.T. -0.052 min  
 Lab File: VU044215.D  
 Acq: 15 Jun 2021 05:07

Tgt Ion:119 Resp: 6369  
 Ion Ratio Lower Upper  
 119 100  
 134 26.0 12.6 37.6  
 91 25.5 12.3 36.8


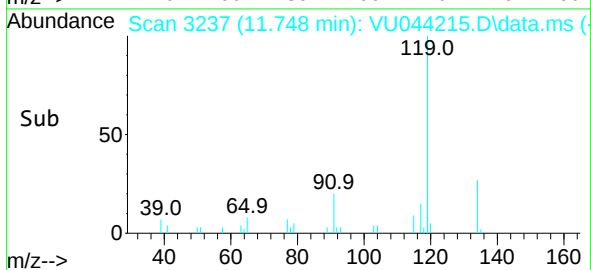

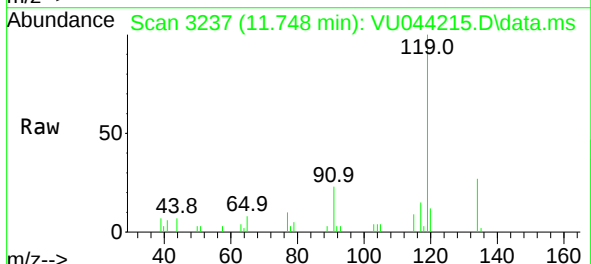




#89  
n-Butylbenzene  
Concen: 0.589 ug/l  
RT: 12.211 min Scan# 3381  
Delta R.T. -0.003 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07




Instrument :  
MSVOA\_U  
ClientSampled :


Tgt Ion: 91 Resp: 5895  
Ion Ratio Lower Upper  
91 100  
92 33.7 27.1 81.2  
134 93.4 11.9 35.5#

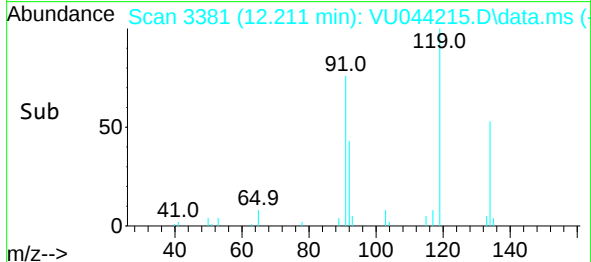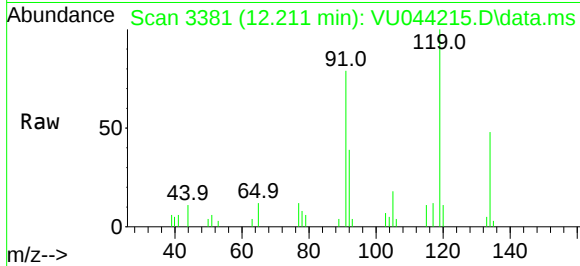

#90  
Hexachloroethane  
Concen: 0.441 ug/l  
RT: 12.471 min Scan# 3462  
Delta R.T. -0.010 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07


Tgt Ion: 117 Resp: 688  
Ion Ratio Lower Upper  
117 100  
201 0.0 35.4 106.3#

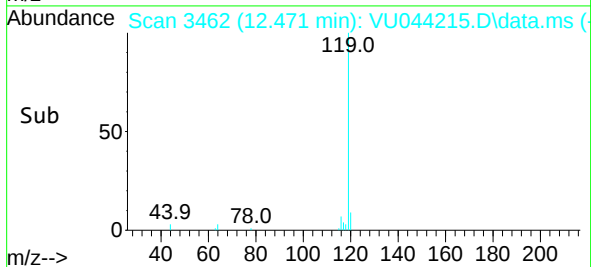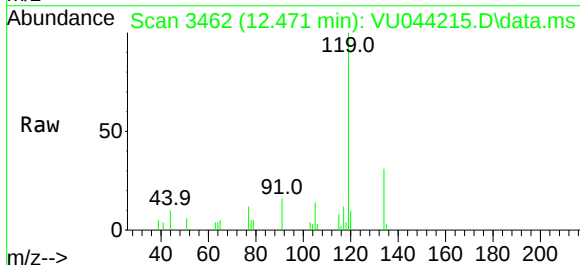

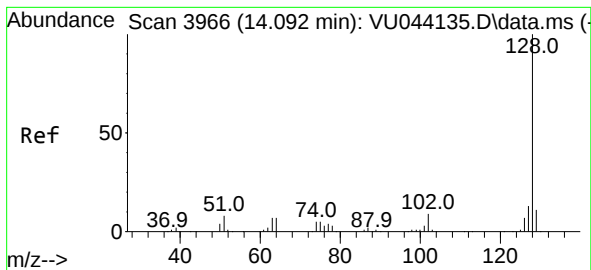

#95  
Naphthalene  
Concen: 2.875 ug/l  
RT: 14.098 min Scan# 3968  
Delta R.T. 0.006 min  
Lab File: VU044215.D  
Acq: 15 Jun 2021 05:07

Instrument :  
MSVOA\_U  
ClientSampleId :

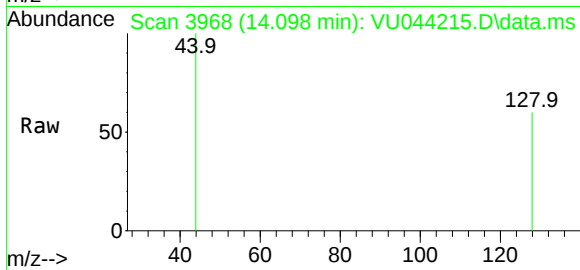

Tgt Ion:128 Resp: 459  
Ion Ratio Lower Upper  
128 100  
127 0.0 10.2 15.2#  
129 0.0 8.6 13.0#

