
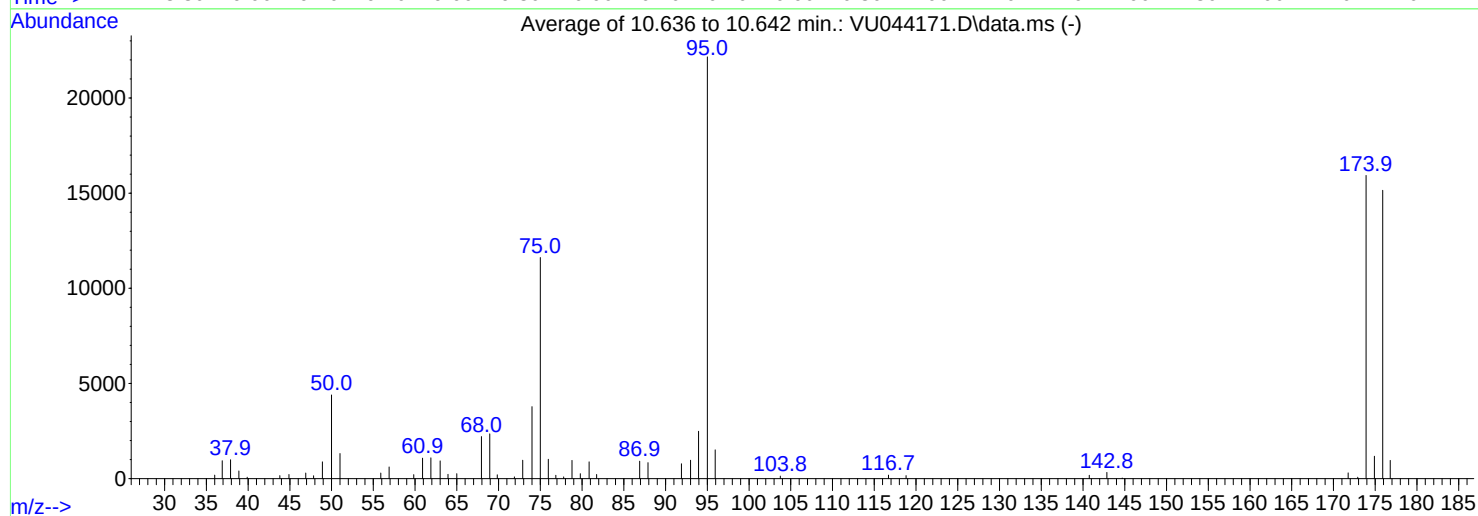


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061421\
 Data File : VU044171.D
 Acq On : 14 Jun 2021 08:54
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060921W.M
 Title : SW846 8260
 Last Update : Thu Jun 10 05:11:37 2021

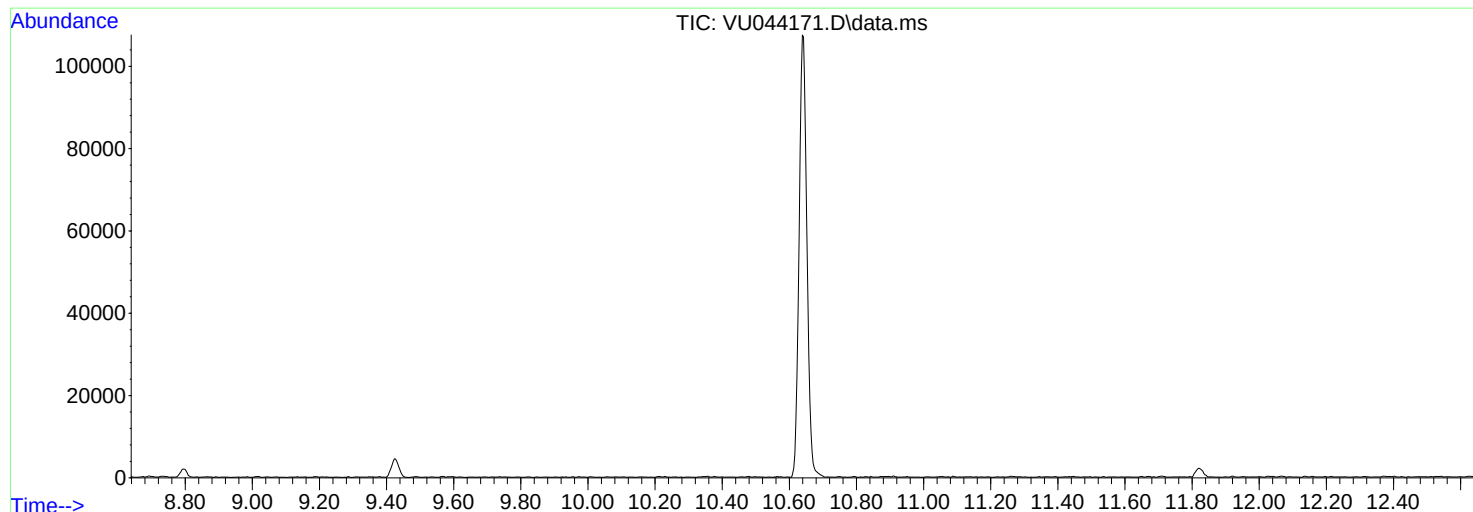

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	4395	PASS
75	95	30	60	52.4	11616	PASS
95	95	100	100	100.0	22160	PASS
96	95	5	9	6.8	1511	PASS
173	174	0.00	2	0.5	76	PASS
174	95	50	100	71.9	15928	PASS
175	174	5	9	7.4	1178	PASS
176	174	95	101	95.1	15148	PASS
177	176	5	9	6.3	959	PASS