
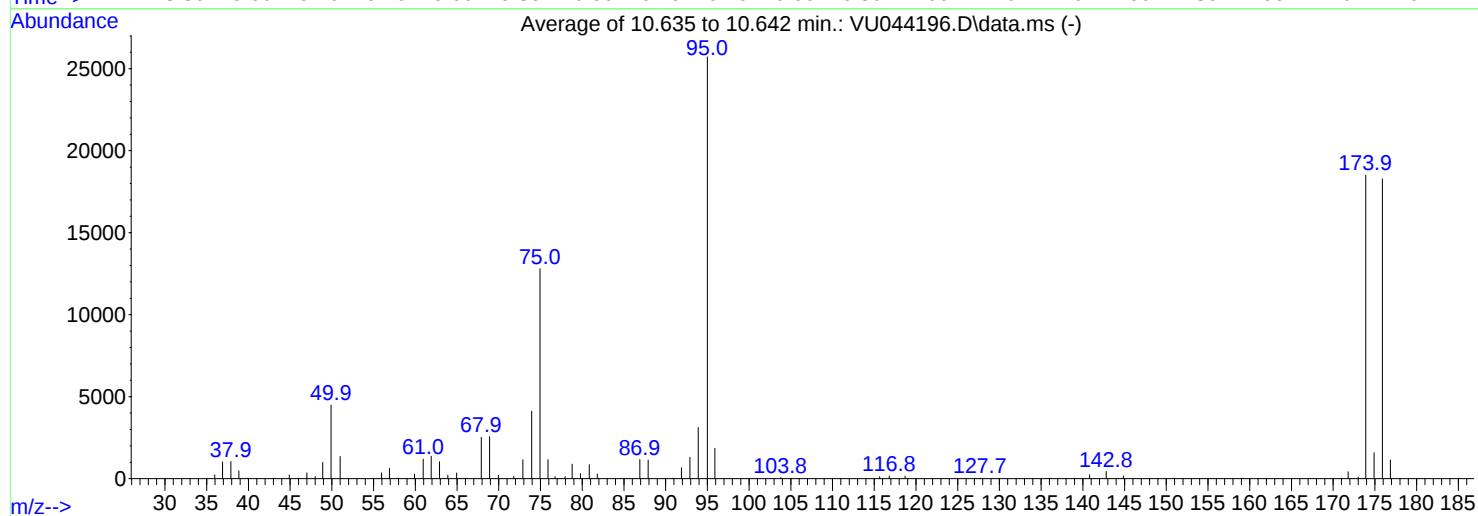


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061421\
Data File : VU044196.D
Acq On : 14 Jun 2021 21:21
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060921W.M
Title : SW846 8260
Last Update : Thu Jun 10 05:11:37 2021

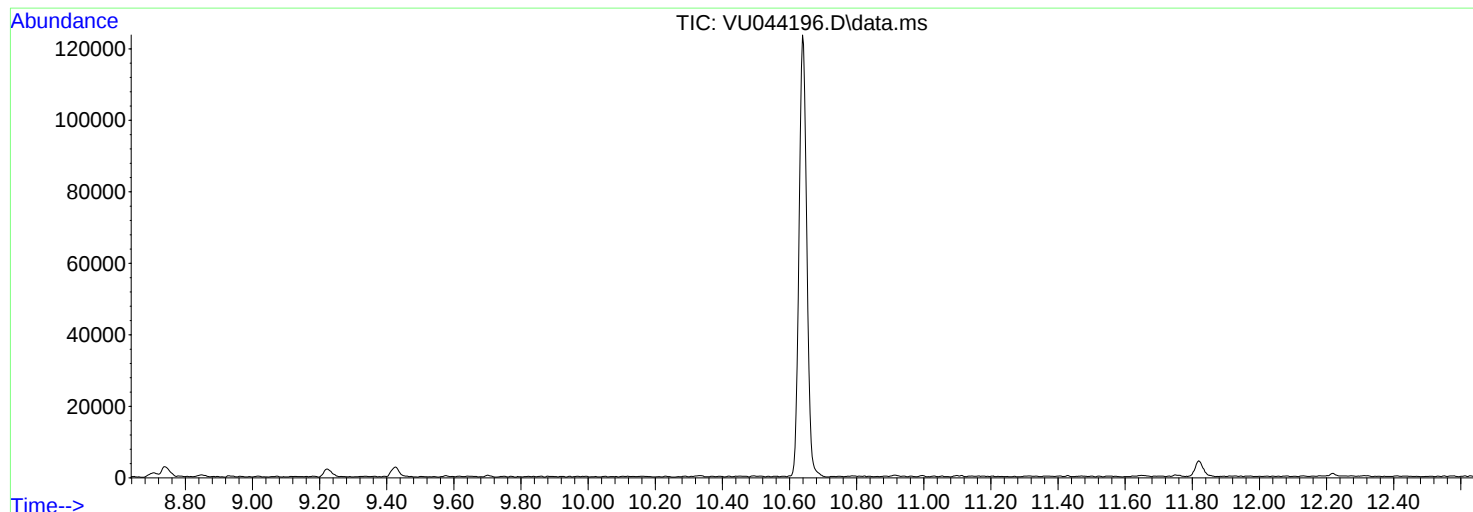

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	4487	PASS
75	95	30	60	49.8	12799	PASS
95	95	100	100	100.0	25720	PASS
96	95	5	9	7.2	1850	PASS
173	174	0.00	2	0.5	97	PASS
174	95	50	100	71.9	18501	PASS
175	174	5	9	8.5	1576	PASS
176	174	95	101	98.8	18288	PASS
177	176	5	9	6.2	1142	PASS