
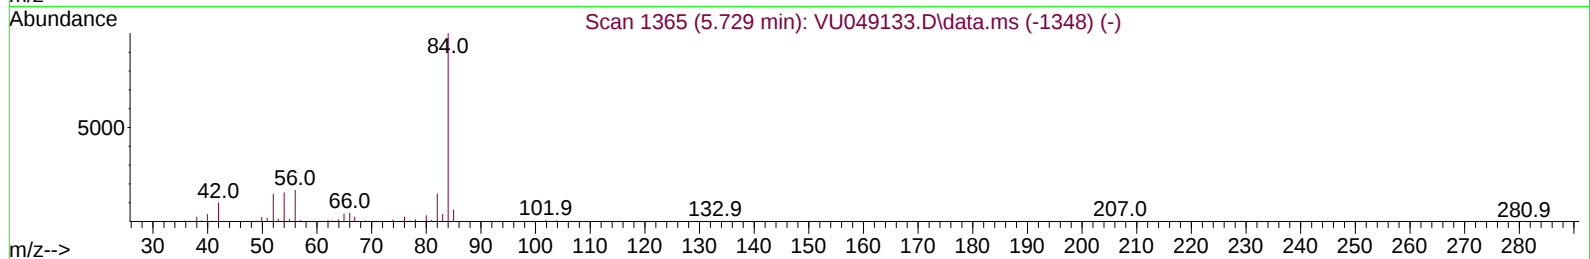
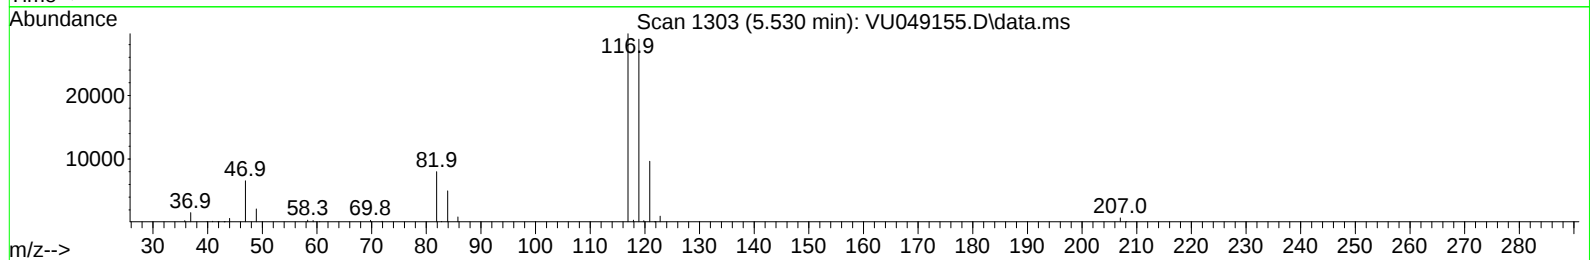


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049155.D
Acq On : 15 Jun 2022 07:59
Operator : SY/MD
Sample : VSTDCCC005EC
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 56 Sample Multiplier: 1

Quant Time: Jun 15 08:51:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 05:38:08 2022
Response via : Initial Calibration

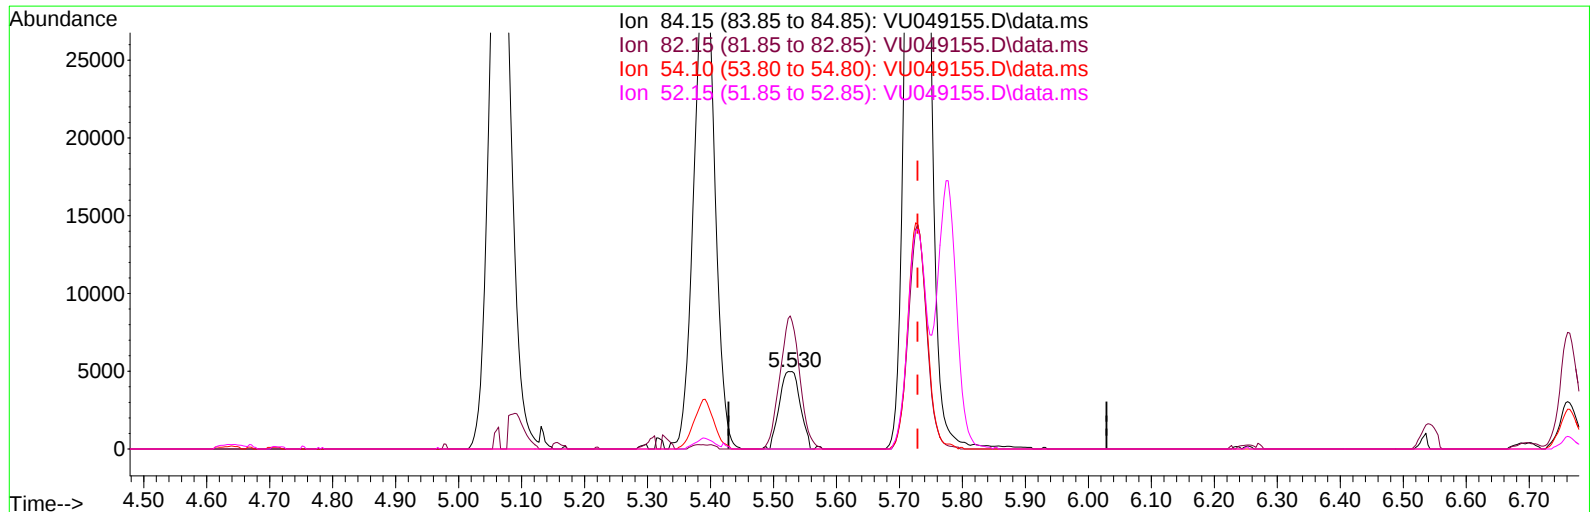

TIC: VU049155.D\data.ms

(32) Benzene-d6 (S)

5.530min (-0.199) 0.30 ug/L

response 11440

Ion	Exp%	Act%
84.15	100.00	100.00
82.15	15.00	163.78#
54.10	15.60	0.00#
52.15	15.70	0.00#