

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049121.D
 Acq On : 14 Jun 2022 18:08
 Operator : SY/MD
 Sample : N3278-14 25X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 15 03:18:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 03:15:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	140099	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	128476	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	62189	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	59559	4.865	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.400%
7) Chloroethane-d5	1.912	69	40888	4.934	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.600%
11) 1,1-Dichloroethene-d2	2.565	65	23480	4.769	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	95.400%
20) 2-Butanone-d5	4.636	46	173886	53.199	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.400%
24) Chloroform-d	5.063	84	95876	4.992	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.800%
26) 1,2-Dichloroethane-d4	5.703	65	54858	5.207	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.200%
32) Benzene-d6	5.729	84	197344	5.099	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.000%
36) 1,2-Dichloropropane-d6	6.693	67	67258	5.120	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.400%
41) Toluene-d8	7.899	98	177189	5.084	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%
43) trans-1,3-Dichloroprop...	8.182	79	29632	5.078	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.600%
46) 2-Hexanone-d5	8.636	63	126650	53.798	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.600%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	55294	5.257	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.200%
66) 1,2-Dichlorobenzene-d4	12.195	152	64952	5.443	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.800%
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.565	101	596	0.074	ug/L #	21
35) Methylcyclohexane	6.693	83	14762	0.901	ug/L #	17
37) 1,2-Dichloropropane	6.690	63	7197	0.685	ug/L #	89
61) 1,2,3-Trichloropropane	11.812	75	8343	1.196	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049121.D
Acq On : 14 Jun 2022 18:08
Operator : SY/MD
Sample : N3278-14 25X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jun 15 03:18:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 03:15:08 2022
Response via : Initial Calibration

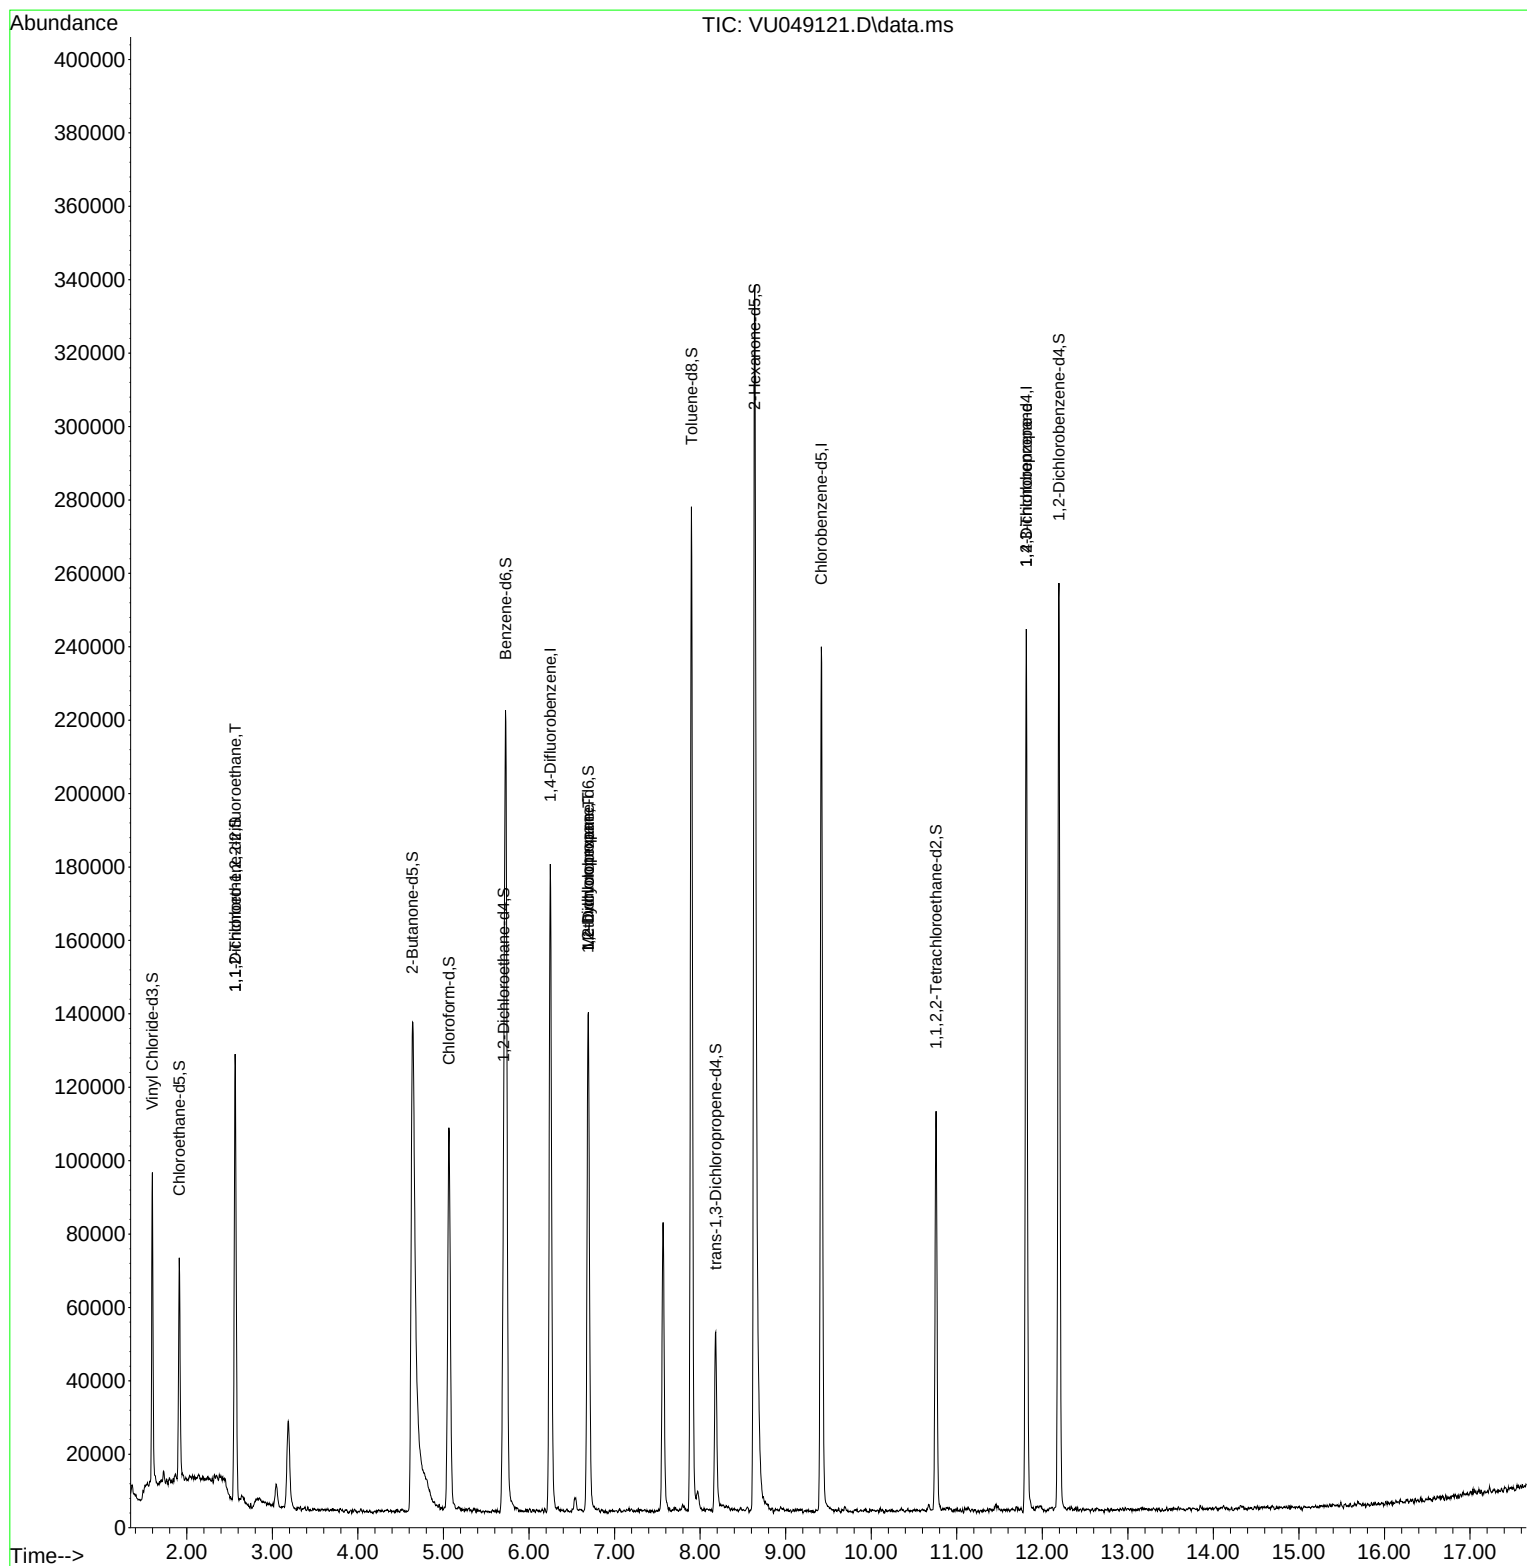

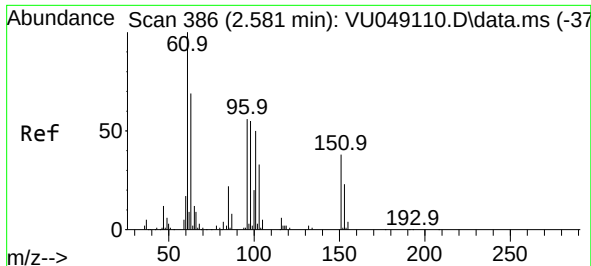

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.074 ug/L

RT: 2.565 min Scan# 381

Delta R.T. -0.016 min


Lab File: VU049121.D

Acq: 14 Jun 2022 18:08




Instrument :

MSVOA_U

ClientSampleId :

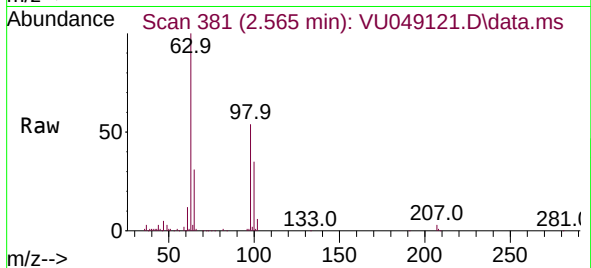

Tgt Ion:	101	Resp:	596
Ion	Ratio	Lower	Upper
101	100		
85	0.0	36.1	54.1#
151	0.0	56.8	85.2#

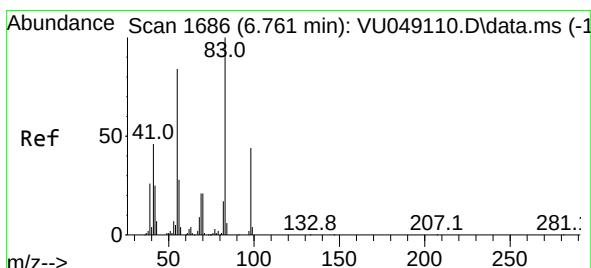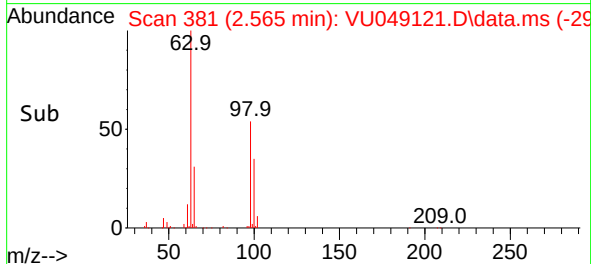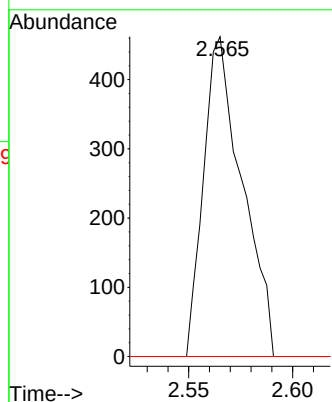

#35

Methylcyclohexane

Concen: 0.901 ug/L




RT: 6.693 min Scan# 1665


Delta R.T. -0.068 min

Lab File: VU049121.D

Acq: 14 Jun 2022 18:08

Tgt Ion:	83	Resp:	14762
Ion	Ratio	Lower	Upper
83	100		
55	1.0	66.9	100.3#
98	1.1	35.5	53.3#

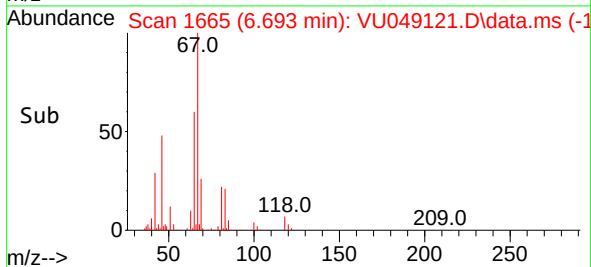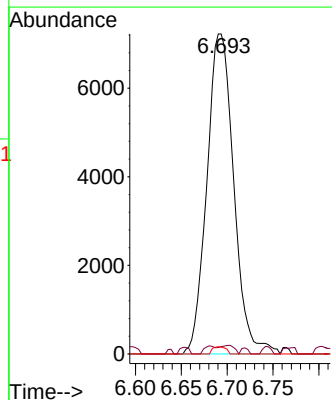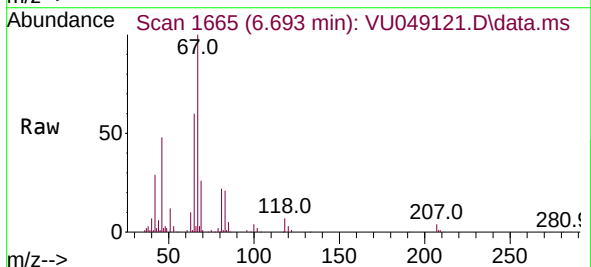

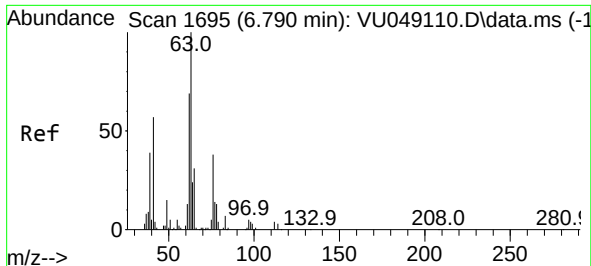

#37

1,2-Dichloropropane

Concen: 0.685 ug/L

RT: 6.690 min Scan# 1

Delta R.T. -0.100 min

Lab File: VU049121.D

Acq: 14 Jun 2022 18:08

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion: 63 Resp: 7197

Ion Ratio Lower Upper

63 100

112 0.0 2.8 4.2#

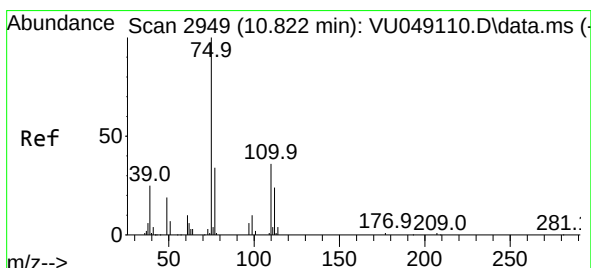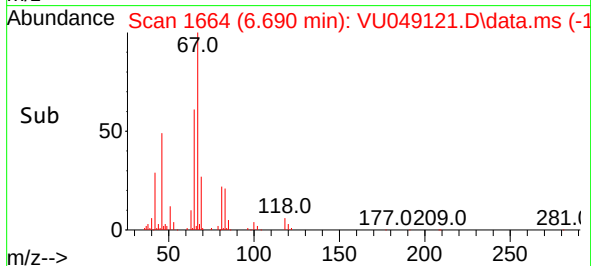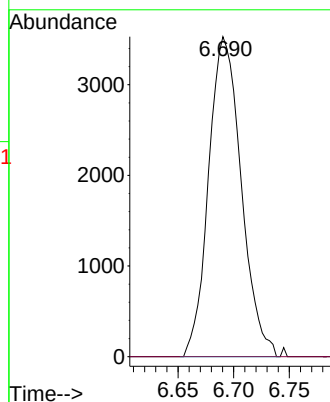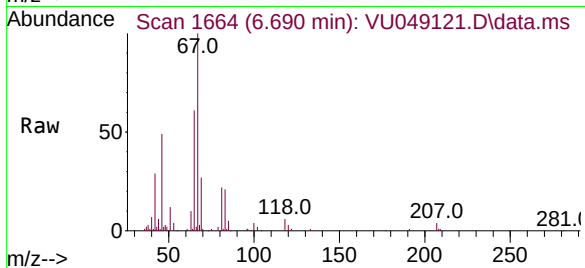

#61

1,2,3-Trichloropropane

Concen: 1.196 ug/L

RT: 11.812 min Scan# 3257

Delta R.T. 0.990 min

Lab File: VU049121.D

Acq: 14 Jun 2022 18:08

Tgt Ion: 75 Resp: 8343

Ion Ratio Lower Upper

75 100

110 1.6 29.0 43.4#

77 33.6 26.2 39.2

