

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049126.D
 Acq On : 14 Jun 2022 20:07
 Operator : SY/MD
 Sample : N3288-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGJA4

Quant Time: Jun 15 03:19:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 03:15:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	138678	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	125847	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	60965	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	56652	4.675	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	93.600%	
7) Chloroethane-d5	1.912	69	39113	4.768	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.400%	
11) 1,1-Dichloroethene-d2	2.568	65	22790	4.676	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	93.600%	
20) 2-Butanone-d5	4.633	46	178572	55.192	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	110.380%	
24) Chloroform-d	5.063	84	93694	4.928	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.600%	
26) 1,2-Dichloroethane-d4	5.703	65	54133	5.191	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.800%	
32) Benzene-d6	5.729	84	192033	5.065	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.400%	
36) 1,2-Dichloropropane-d6	6.690	67	65662	5.103	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.000%	
41) Toluene-d8	7.899	98	172077	5.041	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.800%	
43) trans-1,3-Dichloroprop...	8.182	79	26750	4.679	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	93.600%	
46) 2-Hexanone-d5	8.636	63	118782	51.510	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	103.020%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	53773	5.219	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	104.400%	
66) 1,2-Dichlorobenzene-d4	12.195	152	62260	5.322	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	106.400%	
Target Compounds					Qvalue	
13) Acetone	2.646	43	23192	14.483	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049126.D
Acq On : 14 Jun 2022 20:07
Operator : SY/MD
Sample : N3288-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGJA4

Quant Time: Jun 15 03:19:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 03:15:08 2022
Response via : Initial Calibration

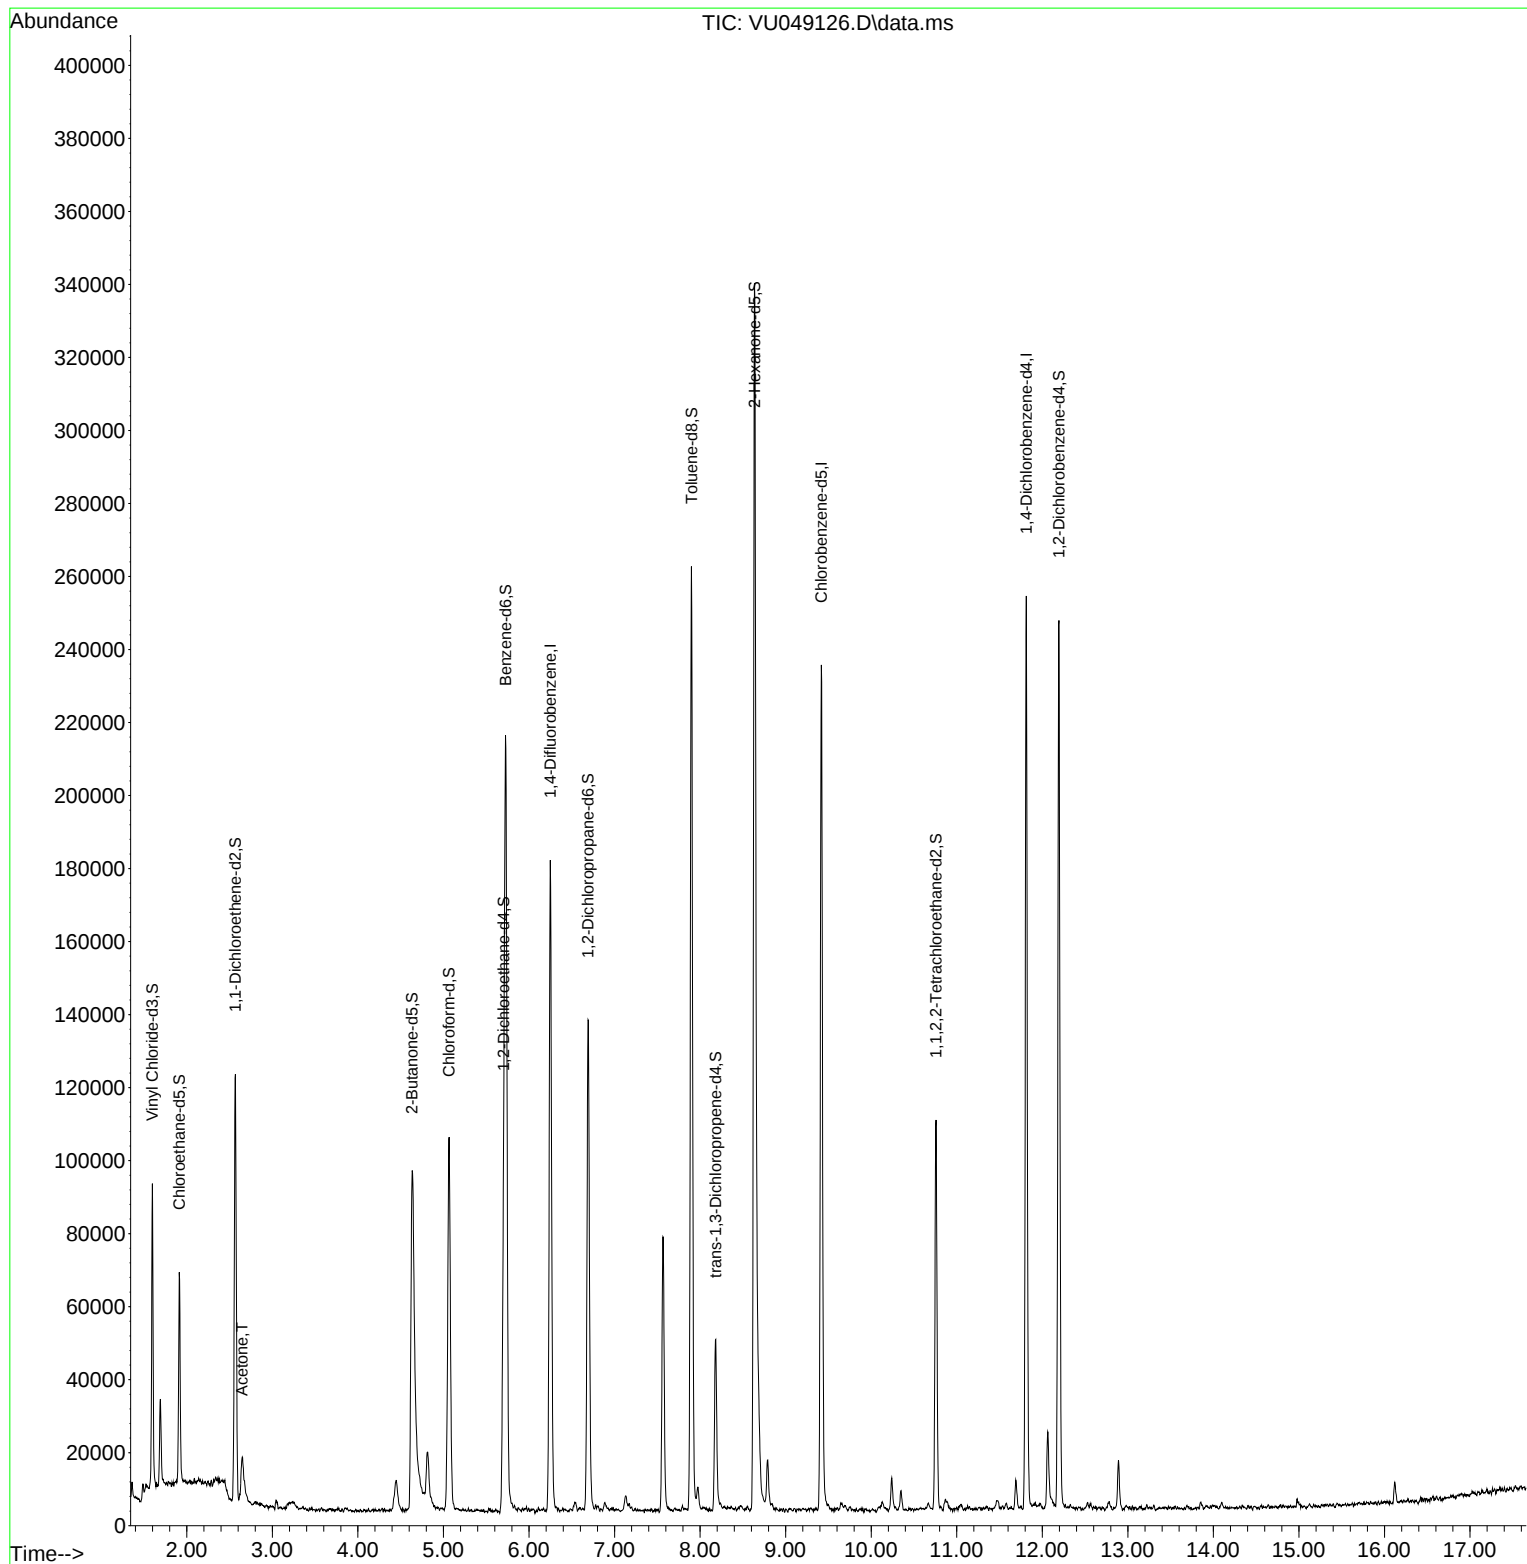

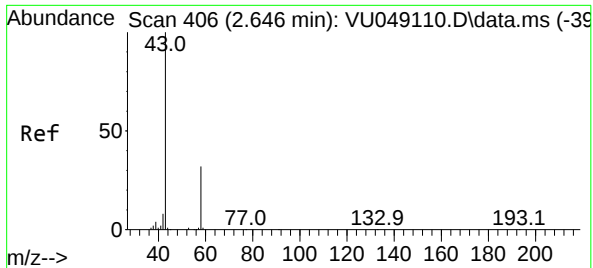

#13
 Acetone
 Concen: 14.483 ug/L
 RT: 2.646 min Scan# 406
 Delta R.T. -0.000 min
 Lab File: VU049126.D
 Acq: 14 Jun 2022 20:07

Instrument :
 MSVOA_U
 ClientSampleId :
 BGJA4

Tgt Ion: 43 Resp: 23192
 Ion Ratio Lower Upper
 43 100
 58 34.3 0.0 65.8

