

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049127.D
 Acq On : 14 Jun 2022 20:31
 Operator : SY/MD
 Sample : N3288-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGJA5

Quant Time: Jun 15 03:20:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 03:15:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	138695	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	126385	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	63172	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	56057	4.626	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.600%
7) Chloroethane-d5	1.912	69	41315	5.036	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.800%
11) 1,1-Dichloroethene-d2	2.565	65	22955	4.709	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	94.200%
20) 2-Butanone-d5	4.636	46	180958	55.923	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.840%
24) Chloroform-d	5.063	84	93021	4.892	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	5.703	65	53887	5.166	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.400%
32) Benzene-d6	5.729	84	190978	5.016	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%
36) 1,2-Dichloropropane-d6	6.694	67	67180	5.199	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.000%
41) Toluene-d8	7.899	98	171140	4.992	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.800%
43) trans-1,3-Dichloroprop...	8.182	79	26973	4.698	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.000%
46) 2-Hexanone-d5	8.636	63	121421	52.430	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.860%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	54112	5.230	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.600%
66) 1,2-Dichlorobenzene-d4	12.192	152	63332	5.225	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.400%
Target Compounds					Qvalue	
13) Acetone	2.646	43	25711	16.054	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049127.D
Acq On : 14 Jun 2022 20:31
Operator : SY/MD
Sample : N3288-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGJA5

Quant Time: Jun 15 03:20:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 03:15:08 2022
Response via : Initial Calibration

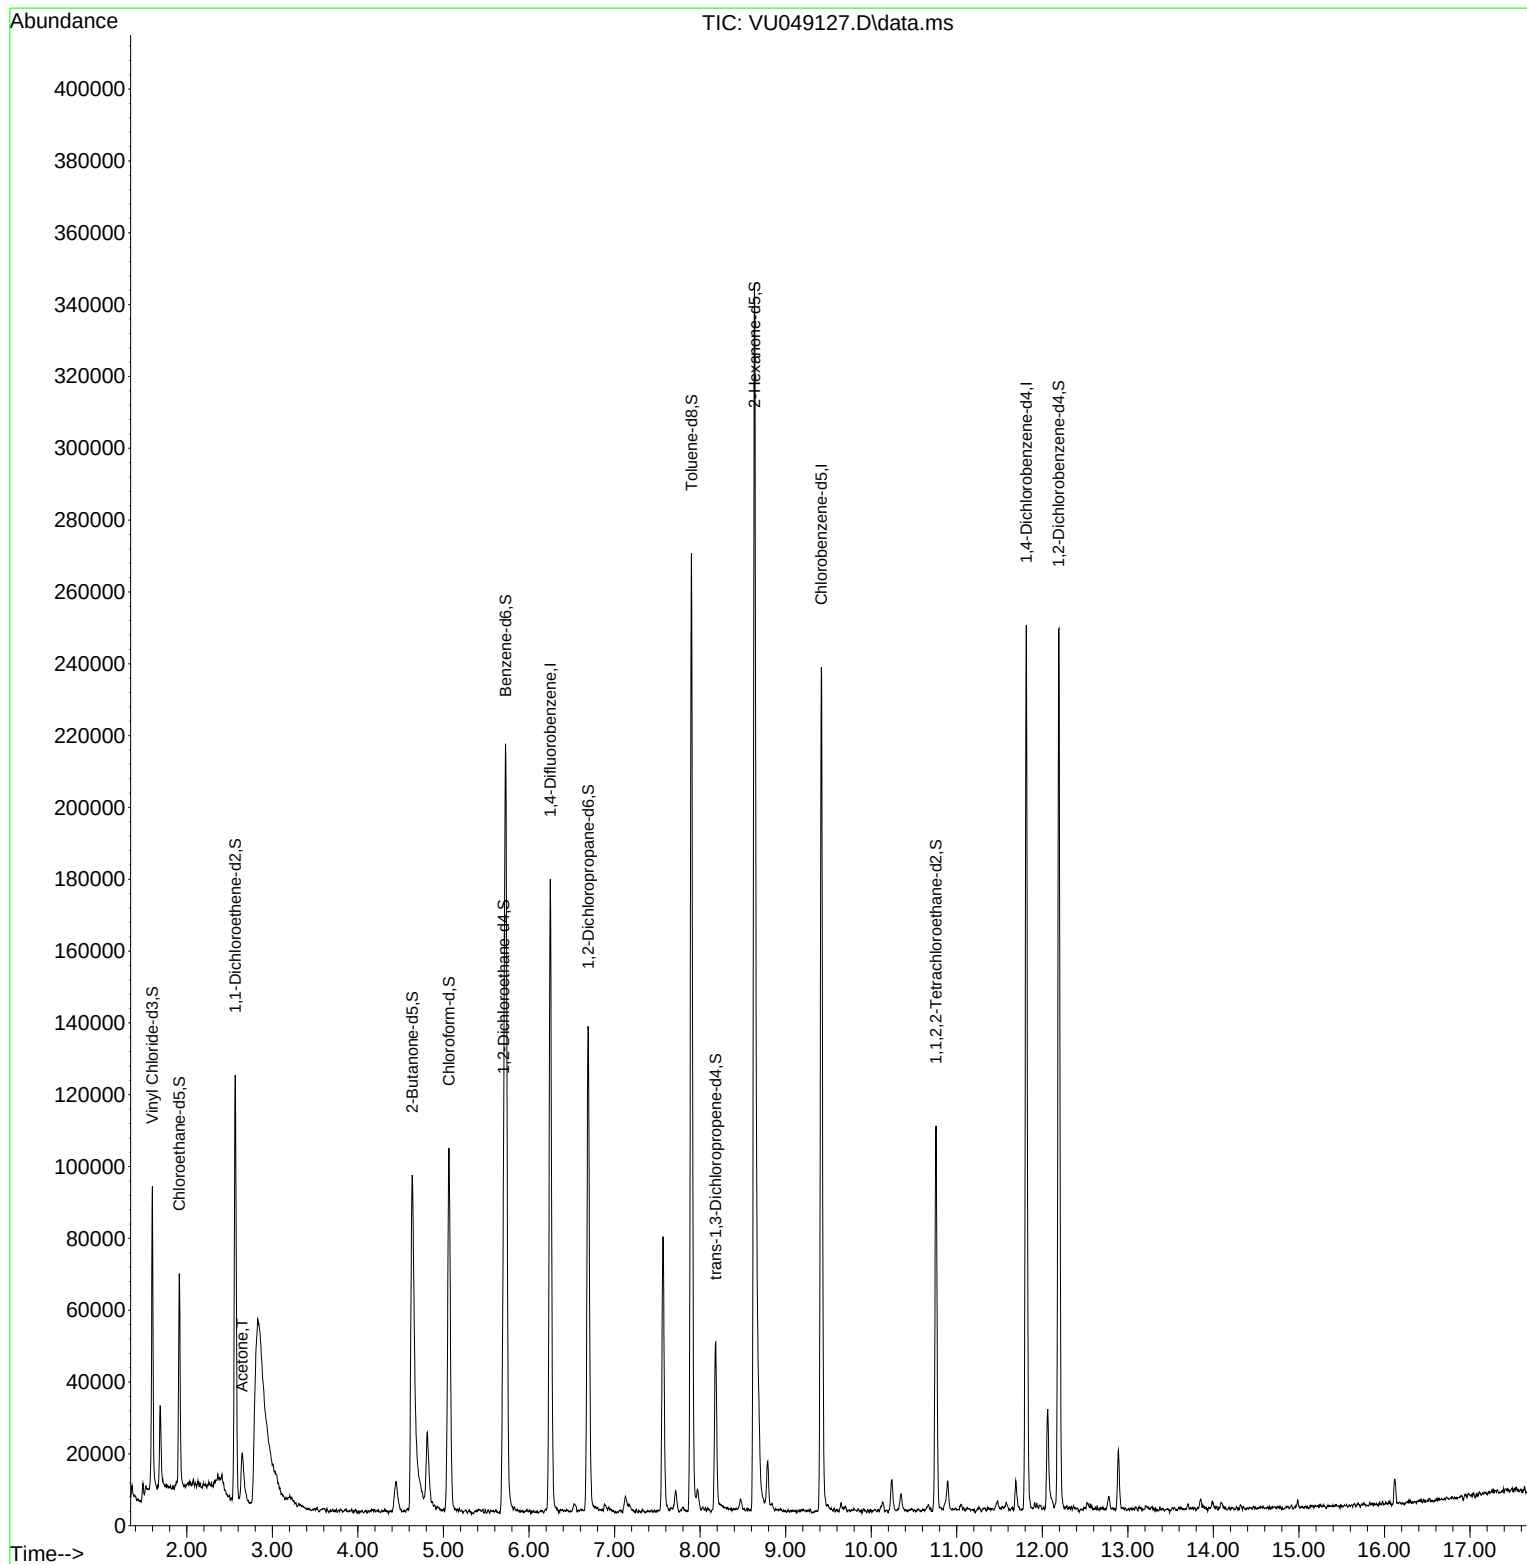

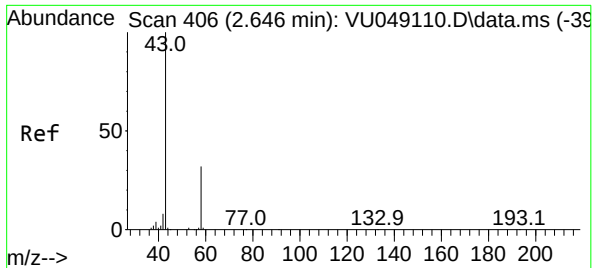

#13
 Acetone
 Concen: 16.054 ug/L
 RT: 2.646 min Scan# 406
 Delta R.T. -0.000 min
 Lab File: VU049127.D
 Acq: 14 Jun 2022 20:31

Instrument :
 MSVOA_U
 ClientSampleId :
 BGJA5

Tgt Ion: 43 Resp: 25711
 Ion Ratio Lower Upper
 43 100
 58 33.5 0.0 65.8

