

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049129.D
 Acq On : 14 Jun 2022 21:18
 Operator : SY/MD
 Sample : N3288-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGJA9

Quant Time: Jun 15 03:20:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 03:15:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	137348	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	123785	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	61689	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	55198	4.599	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.000%
7) Chloroethane-d5	1.913	69	39426	4.852	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.000%
11) 1,1-Dichloroethene-d2	2.565	65	22241	4.607	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	92.200%
20) 2-Butanone-d5	4.636	46	181992	56.794	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.580%
24) Chloroform-d	5.067	84	91204	4.844	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.800%
26) 1,2-Dichloroethane-d4	5.703	65	53099	5.141	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.800%
32) Benzene-d6	5.729	84	189636	5.085	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.800%
36) 1,2-Dichloropropane-d6	6.690	67	63786	5.040	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.800%
41) Toluene-d8	7.899	98	169882	5.059	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.200%
43) trans-1,3-Dichloroprop...	8.182	79	25687	4.568	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.400%
46) 2-Hexanone-d5	8.636	63	117501	51.803	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.600%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	53074	5.237	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.800%
66) 1,2-Dichlorobenzene-d4	12.195	152	61386	5.186	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.800%
Target Compounds						
					Qvalue	
13) Acetone	2.649	43	25464	16.056	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049129.D
Acq On : 14 Jun 2022 21:18
Operator : SY/MD
Sample : N3288-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGJA9

Quant Time: Jun 15 03:20:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 03:15:08 2022
Response via : Initial Calibration

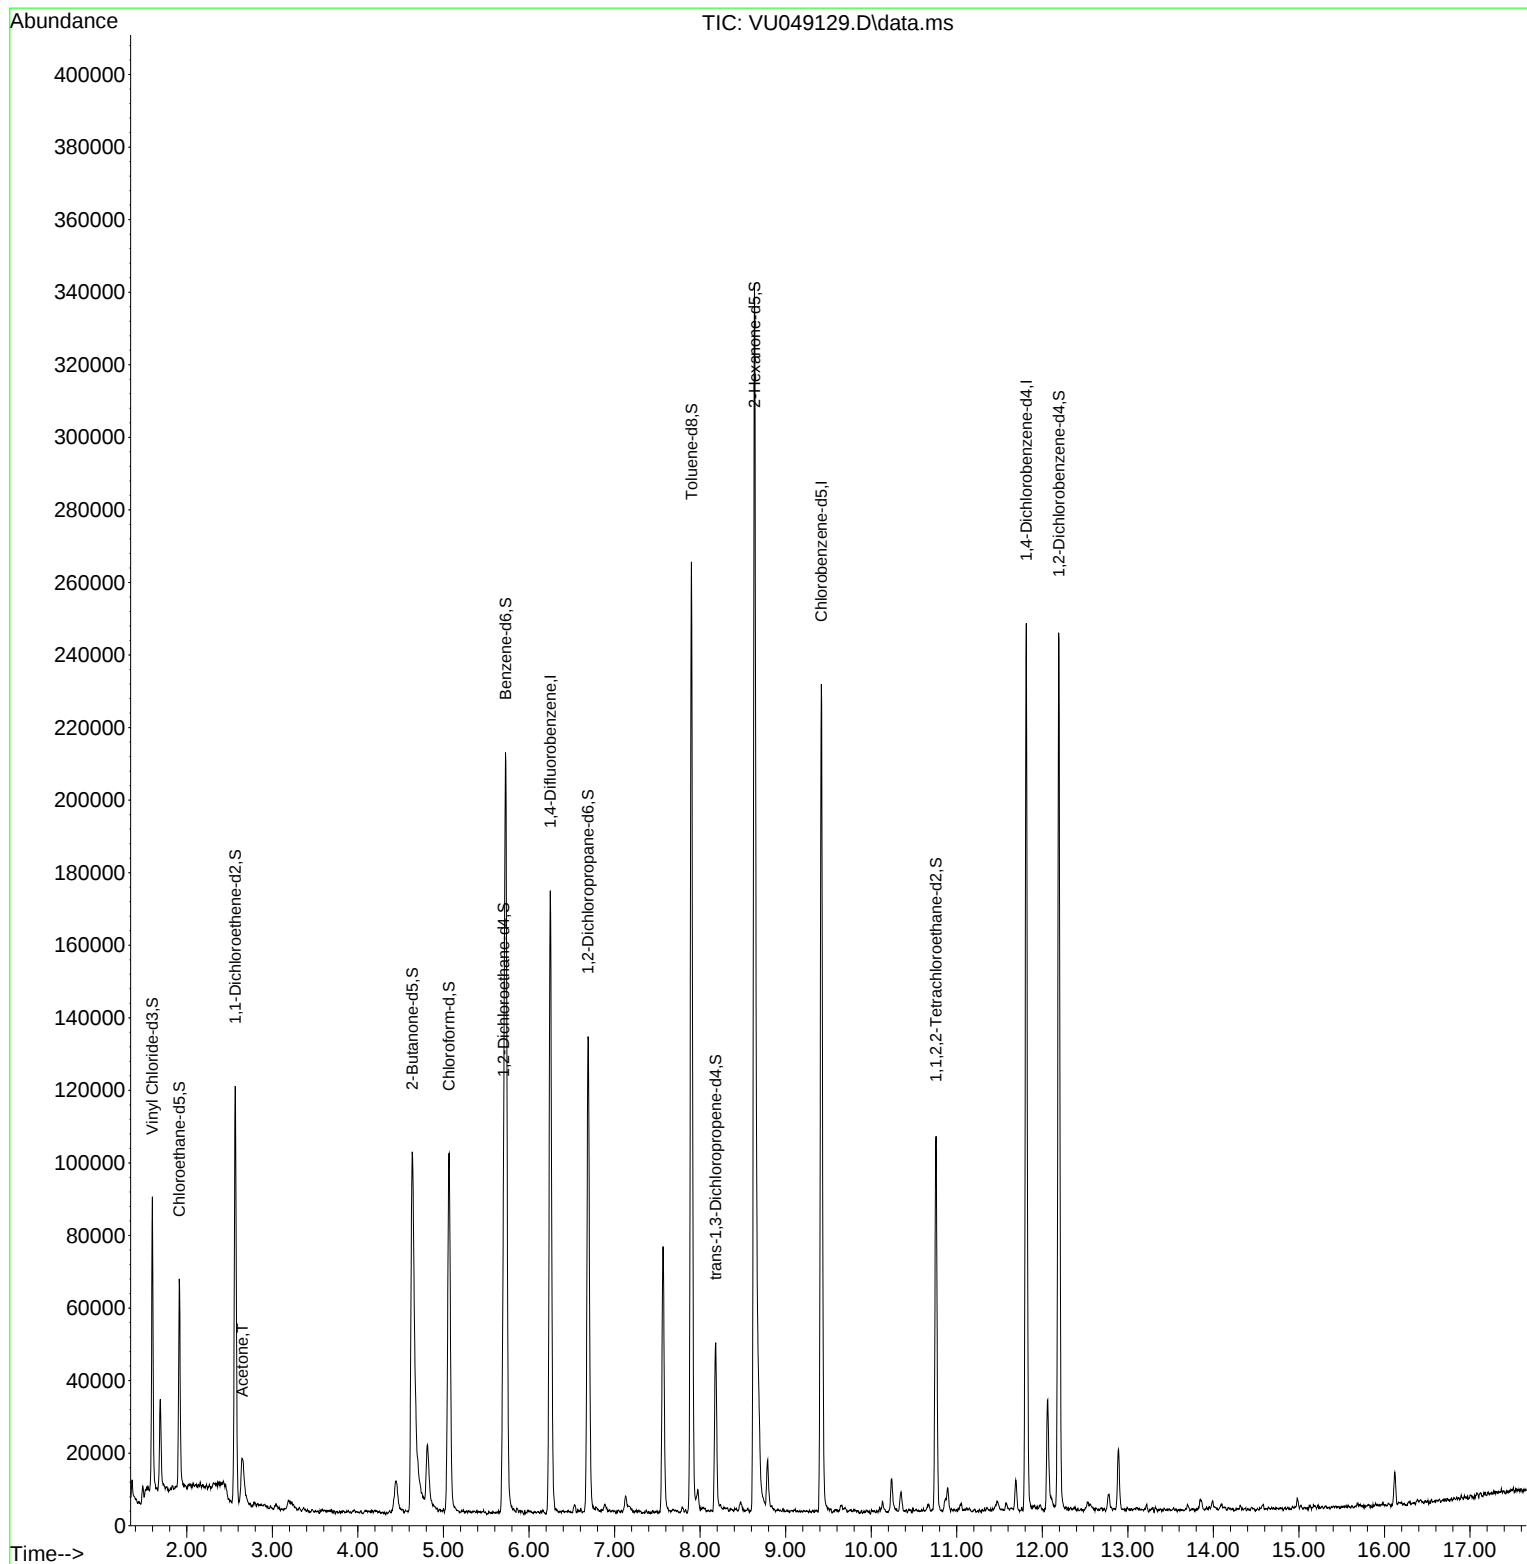

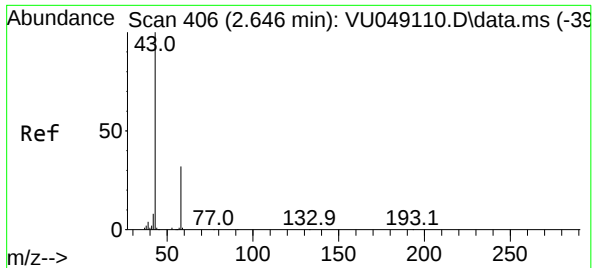

#13
 Acetone
 Concen: 16.056 ug/L
 RT: 2.649 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU049129.D
 Acq: 14 Jun 2022 21:18

Instrument :
 MSVOA_U
 ClientSampleId :
 BGJA9

Tgt Ion: 43 Resp: 25464
 Ion Ratio Lower Upper
 43 100
 58 32.6 0.0 65.8

