

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049144.D
 Acq On : 15 Jun 2022 03:39
 Operator : SY/MD
 Sample : N3274-10 250X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COBA0

Quant Time: Jun 15 07:23:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 05:38:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	139249	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	127828	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	62383	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	54735	4.499	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	90.000%	
7) Chloroethane-d5	1.916	69	39441	4.788	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.800%	
11) 1,1-Dichloroethene-d2	2.568	65	21732	4.441	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	88.800%	
20) 2-Butanone-d5	4.636	46	189787	58.418	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	116.840%	
24) Chloroform-d	5.067	84	90230	4.726	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.600%	
26) 1,2-Dichloroethane-d4	5.703	65	53091	5.070	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.400%	
32) Benzene-d6	5.729	84	187016	4.856	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.200%	
36) 1,2-Dichloropropane-d6	6.690	67	64376	4.925	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.600%	
41) Toluene-d8	7.899	98	165548	4.774	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.400%	
43) trans-1,3-Dichloroprop...	8.182	79	25364	4.368	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	87.400%	
46) 2-Hexanone-d5	8.636	63	122437	52.272	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	104.540%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	54397	5.198	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	104.000%	
66) 1,2-Dichlorobenzene-d4	12.195	152	61886	5.170	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	103.400%	
Target Compounds						
					Qvalue	
34) Trichloroethene	6.546	95	2794	0.287	ug/L	# 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049144.D
Acq On : 15 Jun 2022 03:39
Operator : SY/MD
Sample : N3274-10 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA0

Quant Time: Jun 15 07:23:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 05:38:08 2022
Response via : Initial Calibration

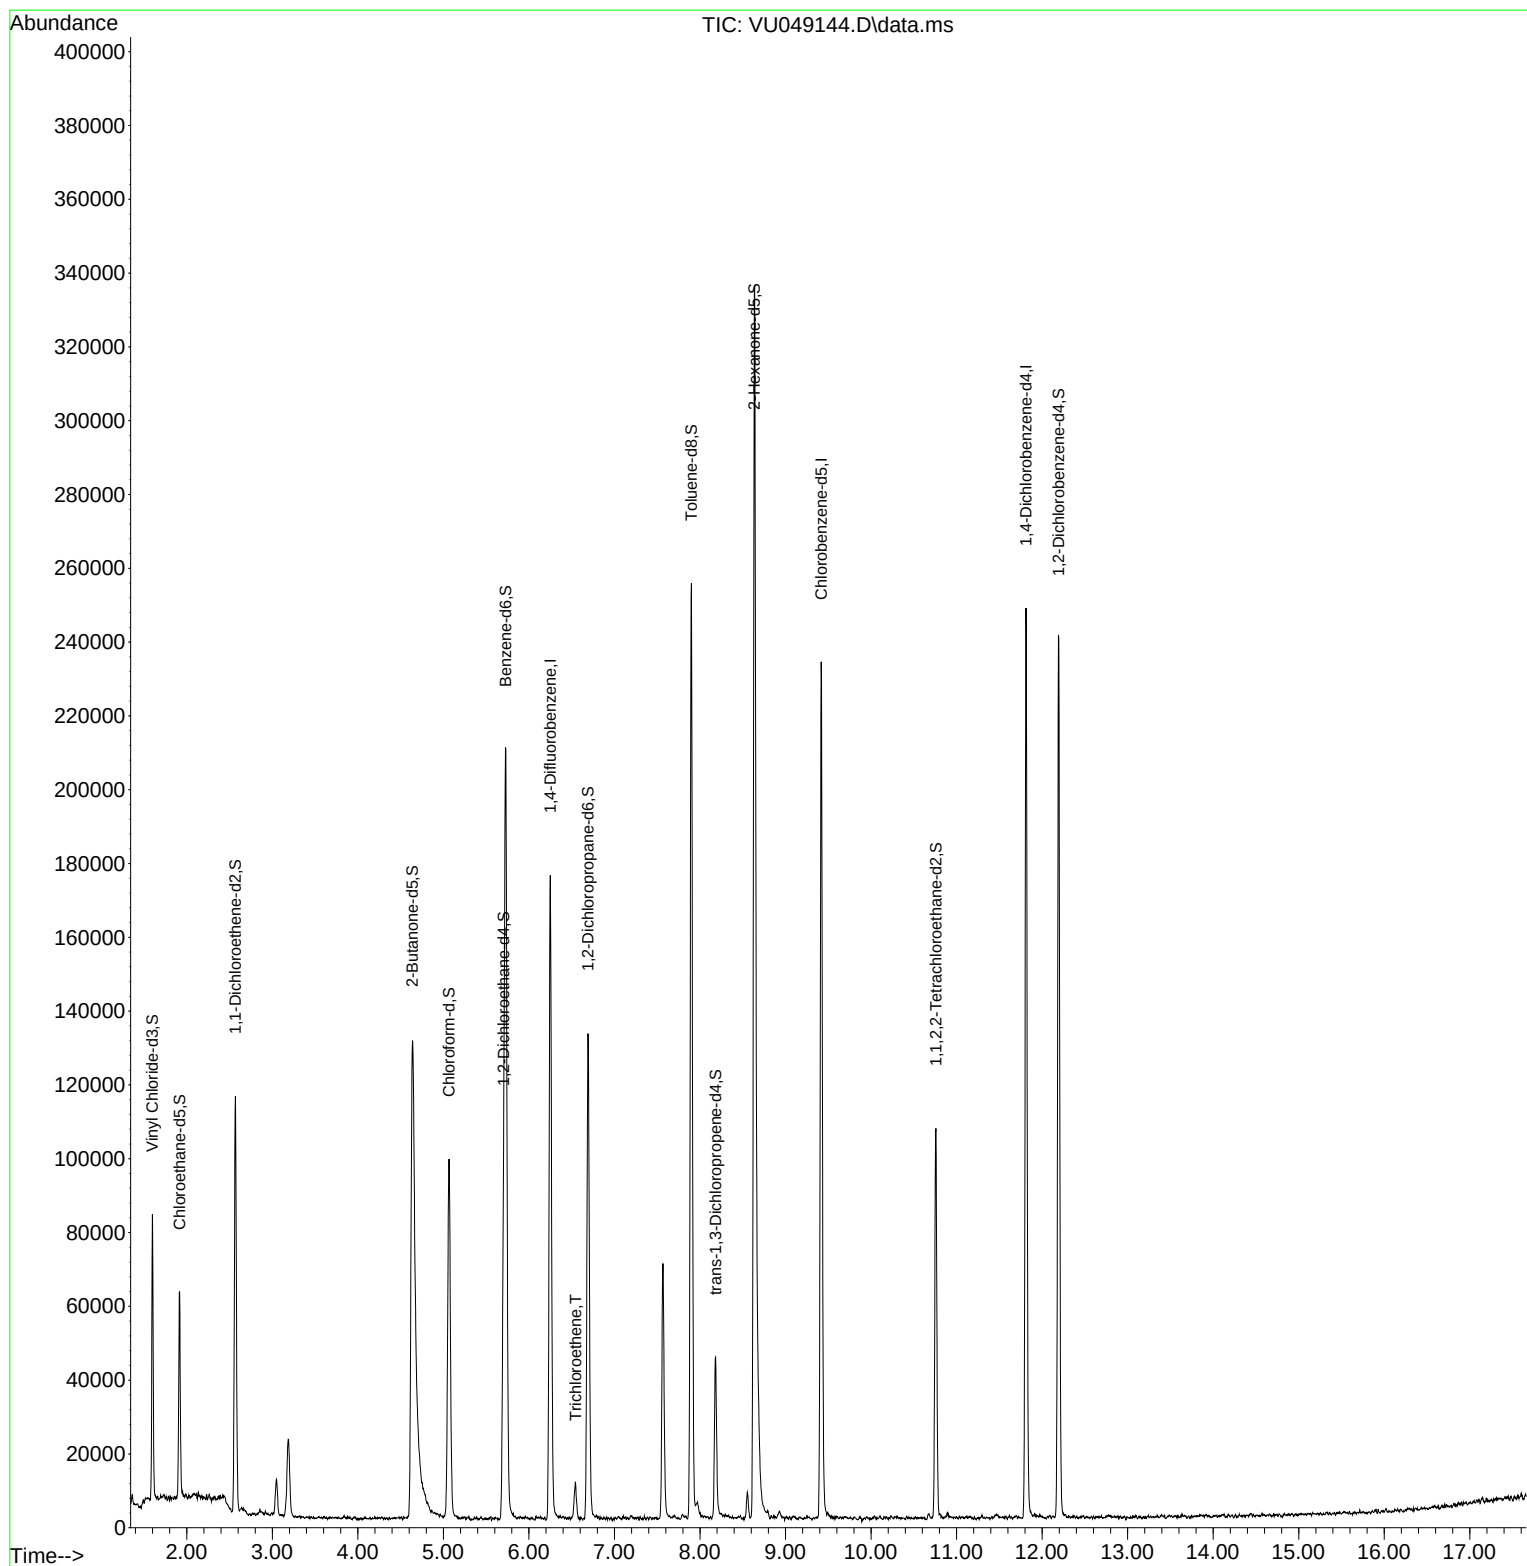

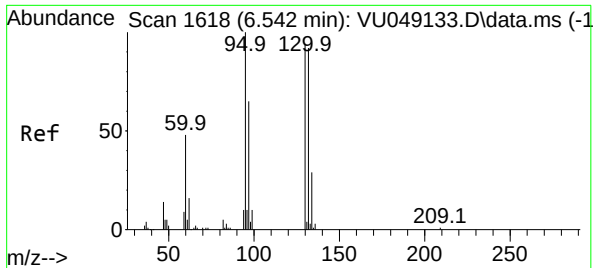

#34
 Trichloroethene
 Concen: 0.287 ug/L
 RT: 6.546 min Scan# 1
 Delta R.T. 0.003 min
 Lab File: VU049144.D
 Acq: 15 Jun 2022 03:39

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BA0

Tgt Ion: 95	Resp:	2794
Ion	Ratio	Lower Upper
95	100	
97	81.9	45.3 84.1
132	118.0	61.5 114.3#
130	91.7	65.6 121.8

