

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049152.D
 Acq On : 15 Jun 2022 06:48
 Operator : SY/MD
 Sample : N3274-18 250X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BC1

Quant Time: Jun 15 07:25:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 05:38:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	129977	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	120647	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	59829	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	51353	4.522	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.400%
7) Chloroethane-d5	1.916	69	37246	4.844	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.800%
11) 1,1-Dichloroethene-d2	2.568	65	20980	4.593	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	91.800%
20) 2-Butanone-d5	4.636	46	179143	59.075	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.160%
24) Chloroform-d	5.067	84	87017	4.883	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%
26) 1,2-Dichloroethane-d4	5.703	65	50865	5.204	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.000%
32) Benzene-d6	5.729	84	177581	4.886	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
36) 1,2-Dichloropropane-d6	6.694	67	61528	4.988	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.800%
41) Toluene-d8	7.899	98	157204	4.803	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.000%
43) trans-1,3-Dichloroprop...	8.179	79	23542	4.296	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.000%
46) 2-Hexanone-d5	8.636	63	119503	54.056	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.120%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	53609	5.428	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.600%
66) 1,2-Dichlorobenzene-d4	12.195	152	58725	5.115	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.400%
Target Compounds						
					Qvalue	
34) Trichloroethene	6.542	95	32602	3.553	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049152.D
Acq On : 15 Jun 2022 06:48
Operator : SY/MD
Sample : N3274-18 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC1


Quant Time: Jun 15 07:25:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 05:38:08 2022
Response via : Initial Calibration

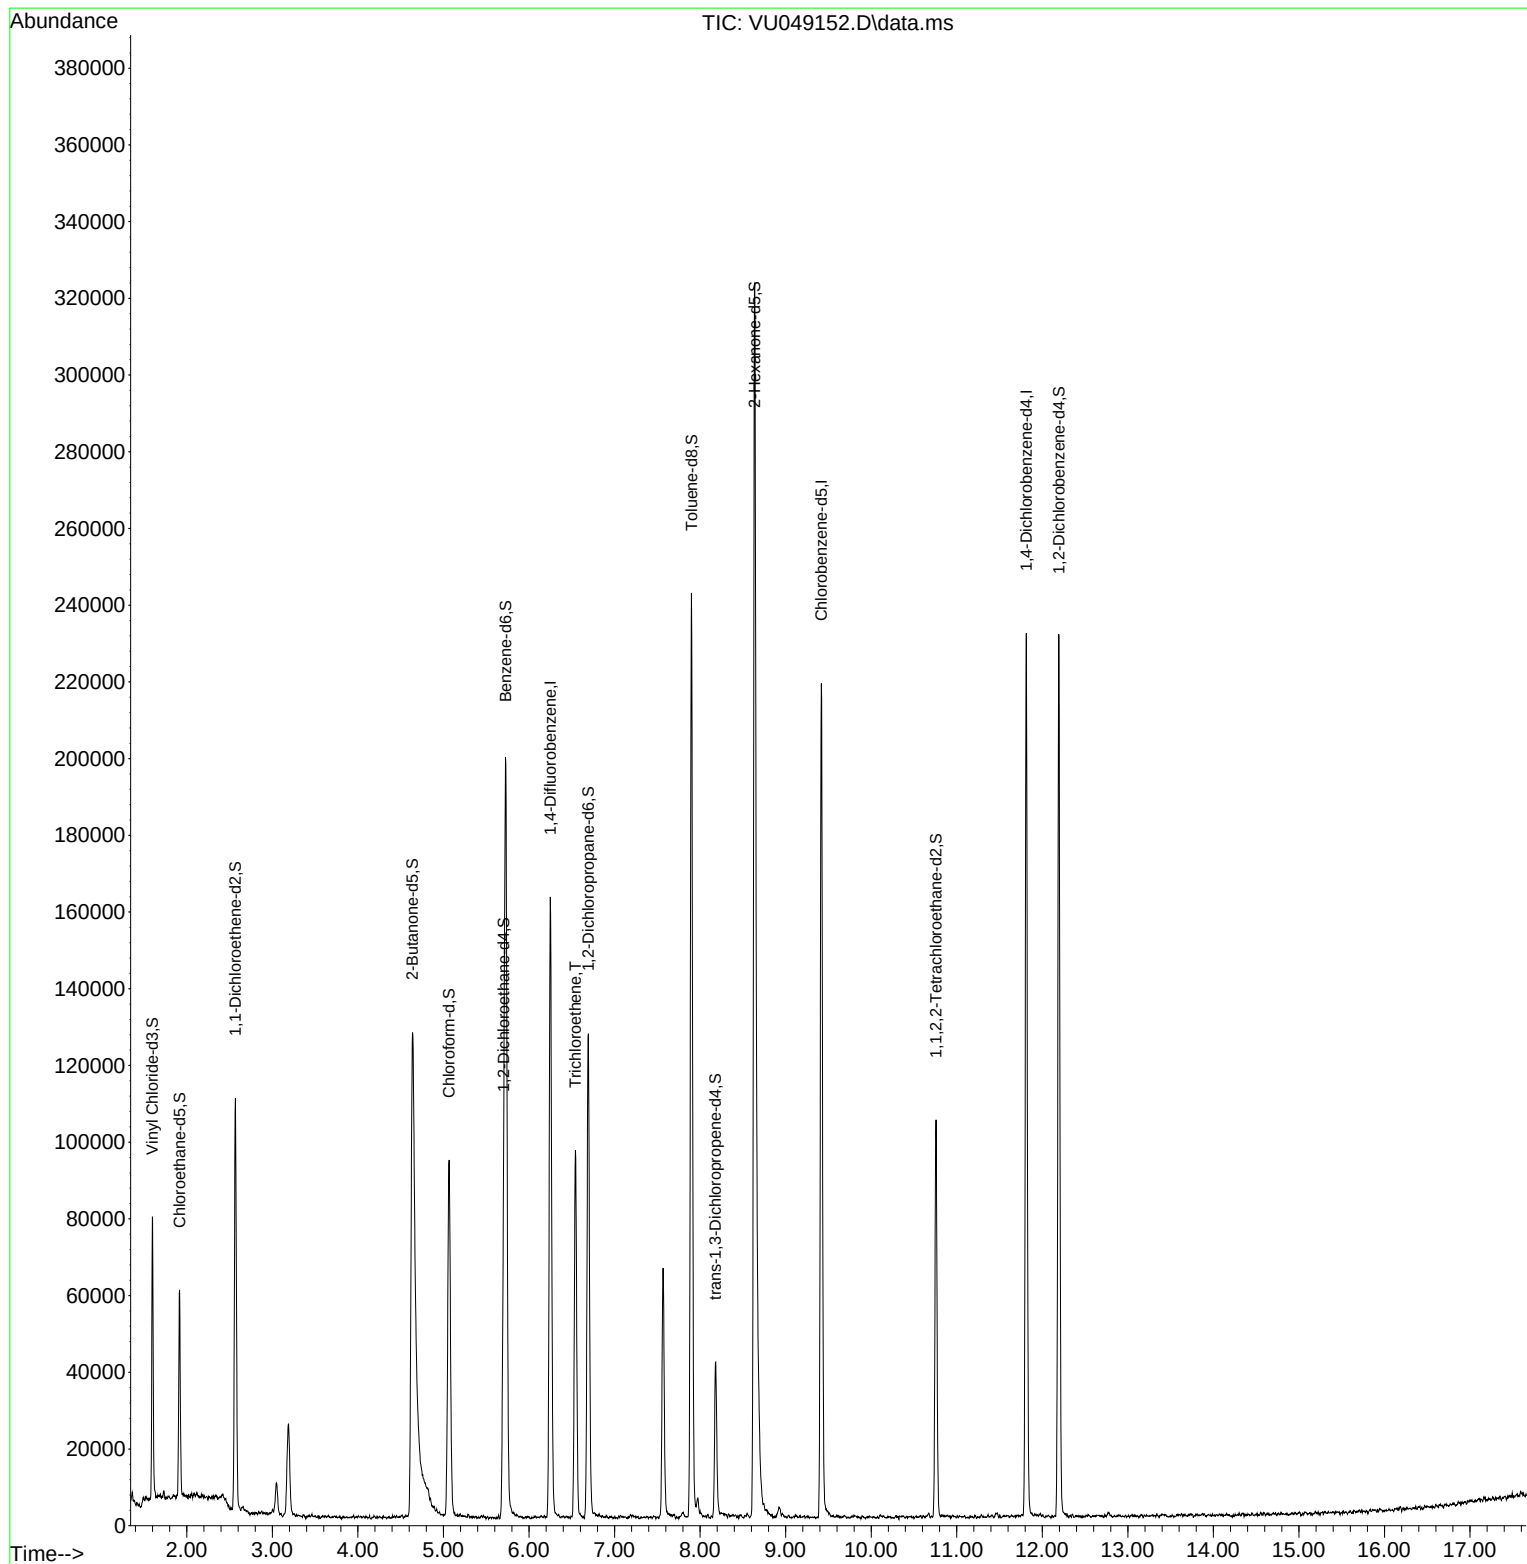

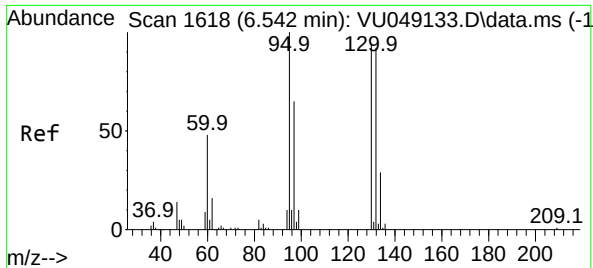

#34
 Trichloroethene
 Concen: 3.553 ug/L
 RT: 6.542 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU049152.D
 Acq: 15 Jun 2022 06:48

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BC1

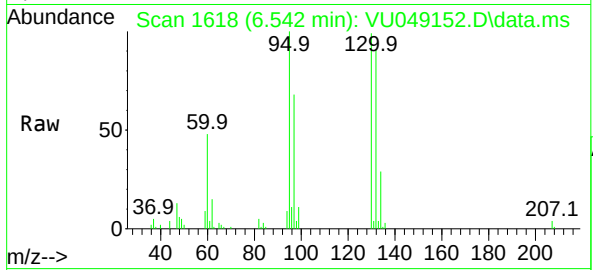

Tgt Ion:	95	Resp:	32602
Ion	Ratio	Lower	Upper
95	100		
97	68.3	45.3	84.1
132	91.4	61.5	114.3
130	99.3	65.6	121.8

