

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049114.D
 Acq On : 14 Jun 2022 15:21
 Operator : SY/MD
 Sample : N3278-03 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BD0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	74124	83002	9.29%	1.401%
2	1.912	171	178	188	rBV	59378	74282	8.31%	1.254%
3	2.141	241	249	259	rVB	14033	21282	2.38%	0.359%
4	2.568	370	382	398	rVB	106773	177664	19.88%	2.998%
5	3.051	524	532	545	rVB4	7473	13039	1.46%	0.220%
6	3.189	560	575	589	rBV	25341	59352	6.64%	1.002%
7	4.639	1011	1026	1083	rBV3	137877	560311	62.70%	9.456%
8	5.063	1142	1158	1182	rVB2	113750	251430	28.14%	4.243%
9	5.726	1340	1364	1387	rBV3	229688	616928	69.04%	10.411%
10	6.250	1512	1527	1546	rBV	162872	309533	34.64%	5.224%
11	6.546	1604	1619	1632	rBV7	7462	16002	1.79%	0.270%
12	6.693	1651	1665	1684	rBV	149976	299554	33.52%	5.055%
13	7.568	1926	1937	1958	rBV	77666	142828	15.98%	2.410%
14	7.899	2027	2040	2057	rBV	279352	491833	55.04%	8.300%
15	8.182	2115	2128	2143	rBV	50705	91324	10.22%	1.541%
16	8.555	2229	2244	2257	rBV	243356	413397	46.26%	6.977%
17	8.639	2257	2270	2305	rVV3	407014	893592	100.00%	15.080%
18	9.417	2497	2512	2530	rBV	220336	379217	42.44%	6.400%
19	10.758	2916	2929	2943	rBV	127392	209322	23.42%	3.533%
20	11.812	3245	3257	3281	rVB	221243	370101	41.42%	6.246%
21	12.195	3363	3376	3393	rBV	270258	451493	50.53%	7.620%




Sum of corrected areas: 5925486

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049114.D
Acq On : 14 Jun 2022 15:21
Operator : SY/MD
Sample : N3278-03 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

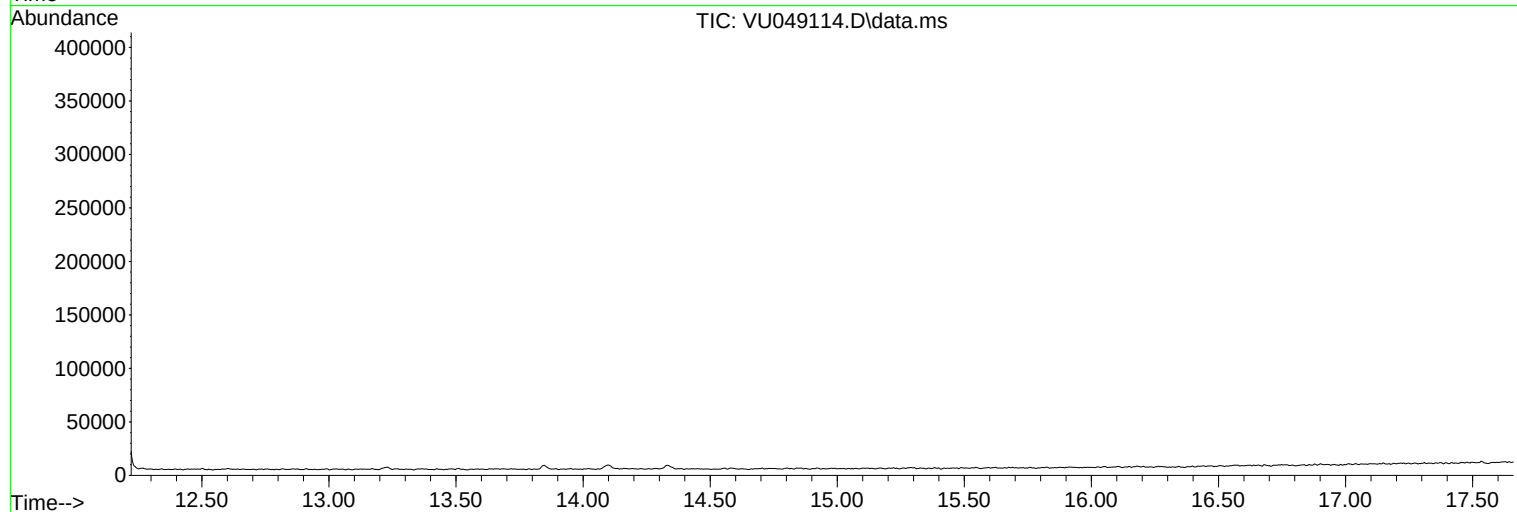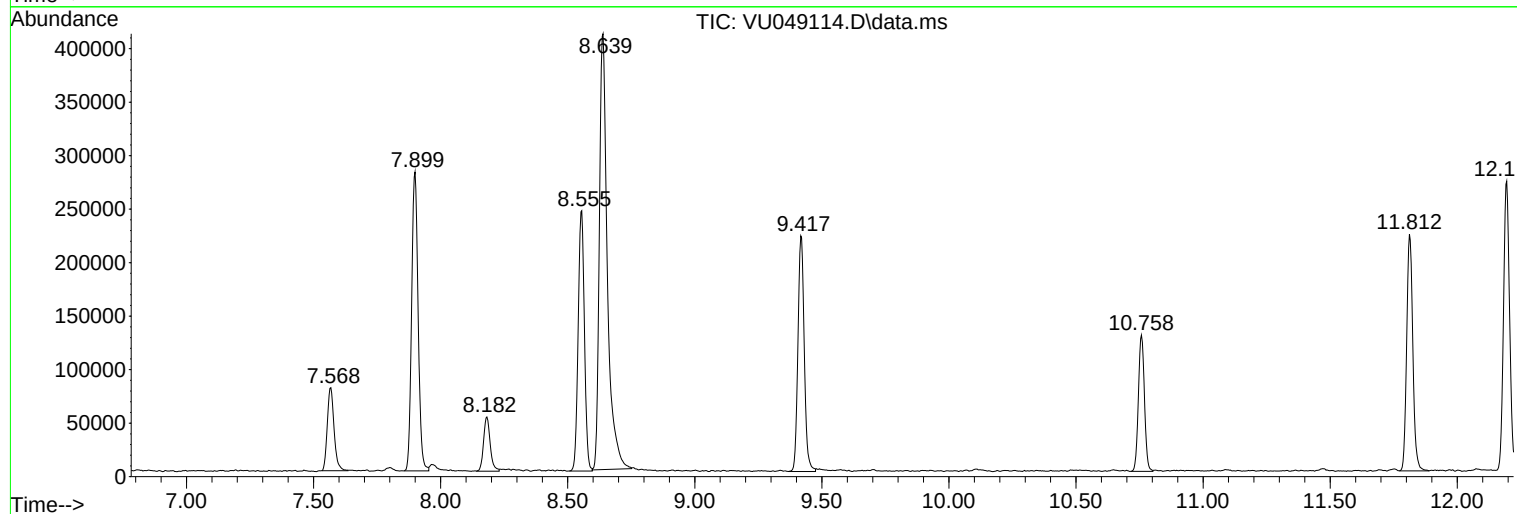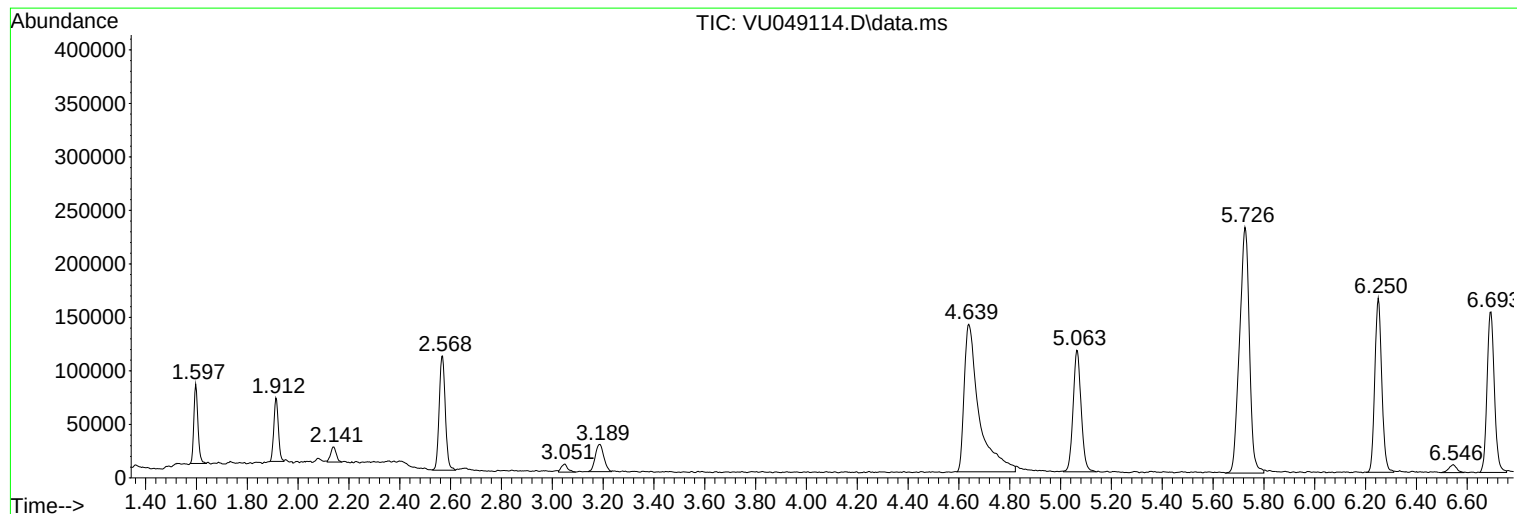

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049114.D
Acq On : 14 Jun 2022 15:21
Operator : SY/MD
Sample : N3278-03 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049114.D
Acq On : 14 Jun 2022 15:21
Operator : SY/MD
Sample : N3278-03 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc