

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049116.D
 Acq On : 14 Jun 2022 16:09
 Operator : SY/MD
 Sample : N3278-05 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BD2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	92	rBV	70606	79857	10.44%	1.540%
2	1.912	171	178	189	rVB	53983	69601	9.10%	1.343%
3	2.137	241	248	259	rVB	16695	24311	3.18%	0.469%
4	2.568	371	382	395	rBV	102121	164838	21.55%	3.180%
5	3.047	521	531	541	rVB2	8300	14749	1.93%	0.284%
6	3.186	561	574	588	rBV2	20057	44385	5.80%	0.856%
7	4.632	1007	1024	1050	rBV2	120229	377727	49.37%	7.286%
8	5.066	1141	1159	1180	rBV	97395	218727	28.59%	4.219%
9	5.726	1341	1364	1383	rBV2	204276	539912	70.57%	10.415%
10	6.250	1512	1527	1543	rBV	157851	303578	39.68%	5.856%
11	6.536	1606	1616	1629	rBV	4283	9292	1.21%	0.179%
12	6.693	1650	1665	1686	rBV	132155	266947	34.89%	5.149%
13	7.568	1924	1937	1953	rBV	67642	125441	16.40%	2.420%
14	7.899	2025	2040	2057	rBV	241332	426749	55.78%	8.232%
15	8.182	2114	2128	2145	rBV	43650	80198	10.48%	1.547%
16	8.555	2231	2244	2257	rBV	238667	408541	53.40%	7.880%
17	8.635	2258	2269	2302	rVV2	329996	765062	100.00%	14.758%
18	9.417	2501	2512	2531	rBV	205812	353315	46.18%	6.815%
19	10.758	2911	2929	2943	rBV	110330	180650	23.61%	3.485%
20	11.812	3245	3257	3273	rBV	212460	343921	44.95%	6.634%
21	12.195	3358	3376	3391	rBV	228970	386403	50.51%	7.453%




Sum of corrected areas: 5184204

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049116.D
Acq On : 14 Jun 2022 16:09
Operator : SY/MD
Sample : N3278-05 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

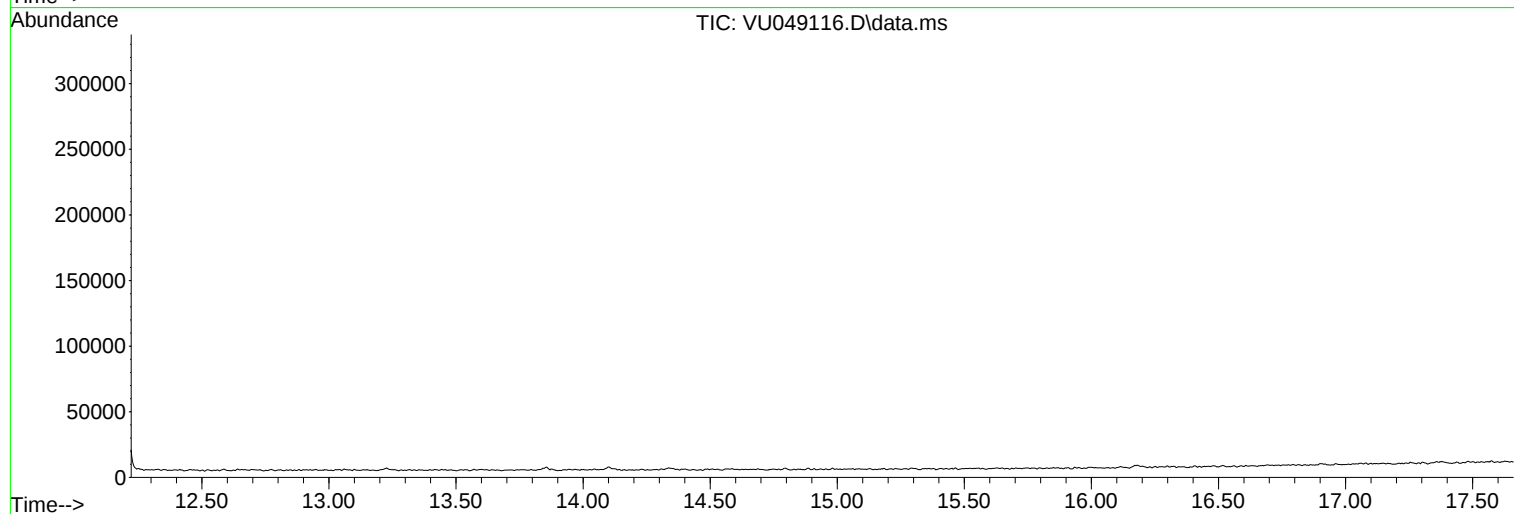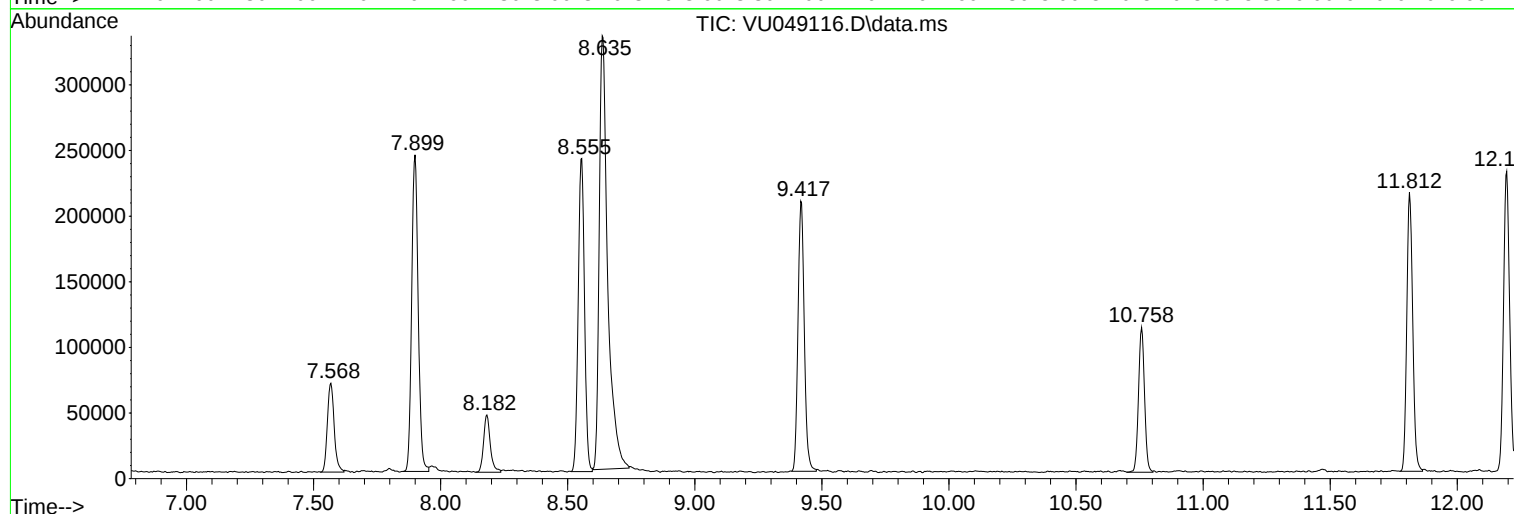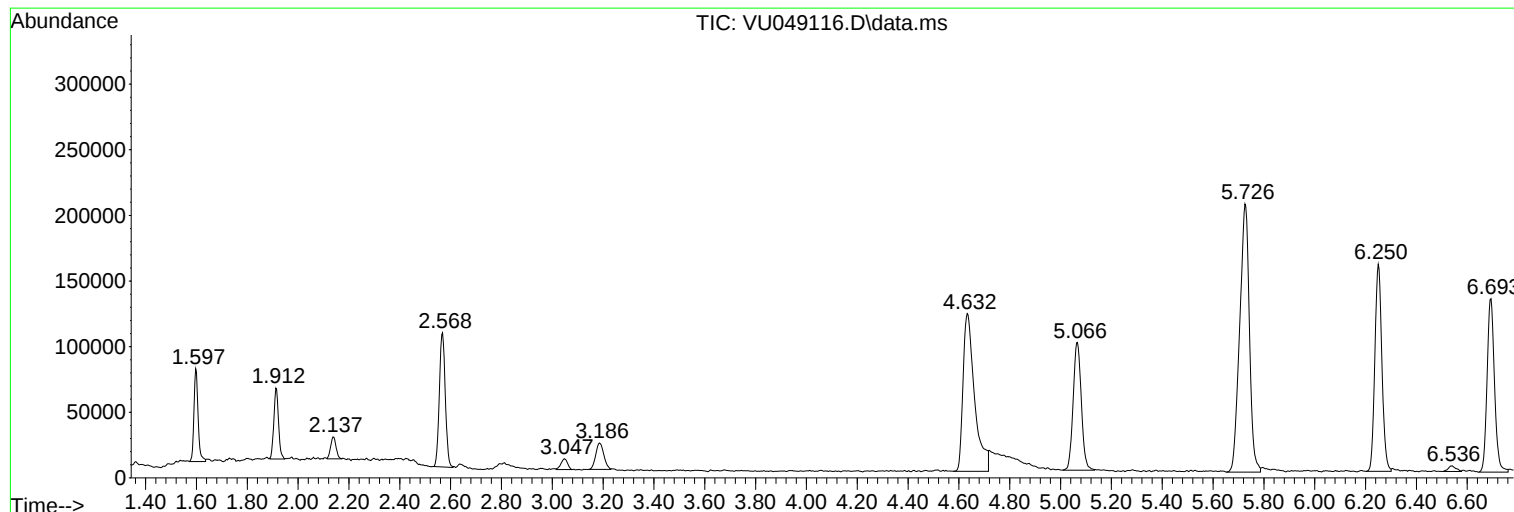

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049116.D
Acq On : 14 Jun 2022 16:09
Operator : SY/MD
Sample : N3278-05 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049116.D
Acq On : 14 Jun 2022 16:09
Operator : SY/MD
Sample : N3278-05 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
