

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049118.D
 Acq On : 14 Jun 2022 16:57
 Operator : SY/MD
 Sample : N3278-11 8000X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BF2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rBV	87897	97408	12.75%	1.646%
2	1.912	170	178	190	rBV	60999	77130	10.09%	1.304%
3	2.568	369	382	397	rVB	126309	207870	27.21%	3.513%
4	3.047	520	531	540	rBV6	5241	10178	1.33%	0.172%
5	3.186	562	574	587	rBV	21080	46683	6.11%	0.789%
6	4.636	1010	1025	1058	rBV3	155359	495830	64.89%	8.380%
7	5.063	1139	1158	1176	rBV	109592	244024	31.94%	4.124%
8	5.726	1345	1364	1391	rBV2	229229	591332	77.39%	9.995%
9	6.250	1513	1527	1549	rBV	177454	344514	45.09%	5.823%
10	6.542	1603	1618	1637	rBV2	292232	561028	73.43%	9.482%
11	6.690	1651	1664	1683	rBV	140276	276836	36.23%	4.679%
12	7.565	1924	1936	1954	rBV	83146	150317	19.67%	2.541%
13	7.899	2025	2040	2055	rBV	285483	500732	65.54%	8.463%
14	7.970	2060	2062	2078	rVB3	6089	8324	1.09%	0.141%
15	8.182	2116	2128	2143	rBV2	52903	95093	12.45%	1.607%
16	8.555	2233	2244	2253	rBV2	20437	33533	4.39%	0.567%
17	8.636	2257	2269	2301	rBV2	358952	764057	100.00%	12.914%
18	9.417	2498	2512	2529	rBV	237495	404013	52.88%	6.829%
19	10.758	2917	2929	2945	rBV	111806	181064	23.70%	3.060%
20	11.812	3246	3257	3273	rBV	244405	399481	52.28%	6.752%
21	12.195	3362	3376	3392	rBV	258614	427110	55.90%	7.219%




Sum of corrected areas: 5916557

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049118.D
Acq On : 14 Jun 2022 16:57
Operator : SY/MD
Sample : N3278-11 8000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

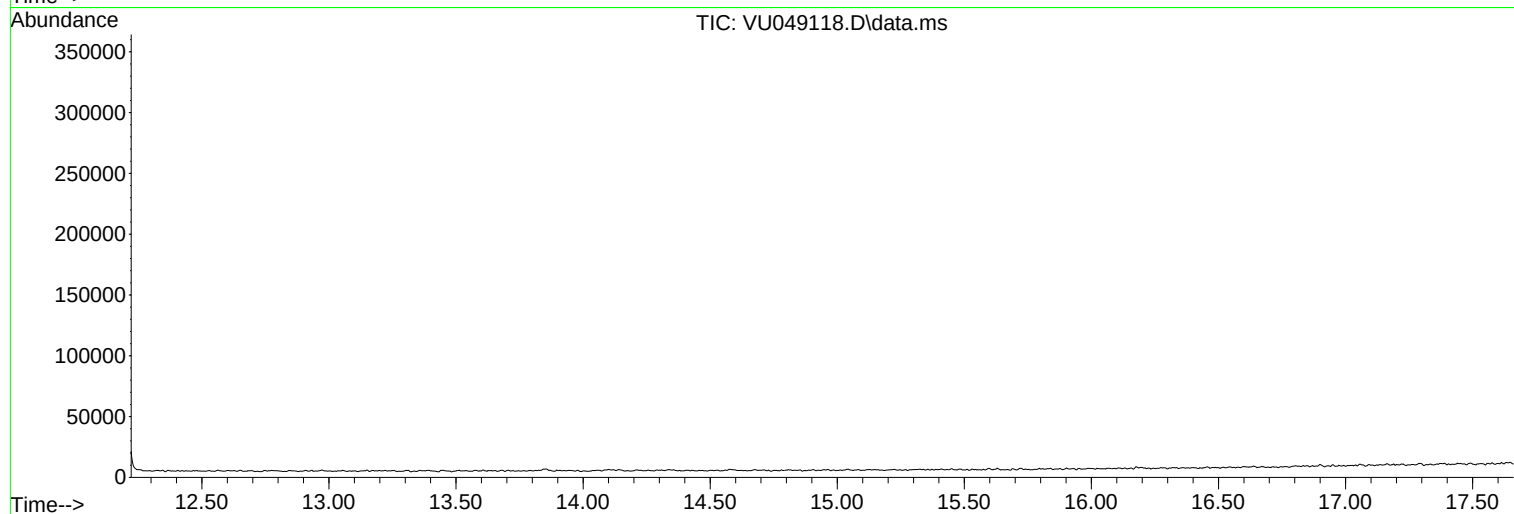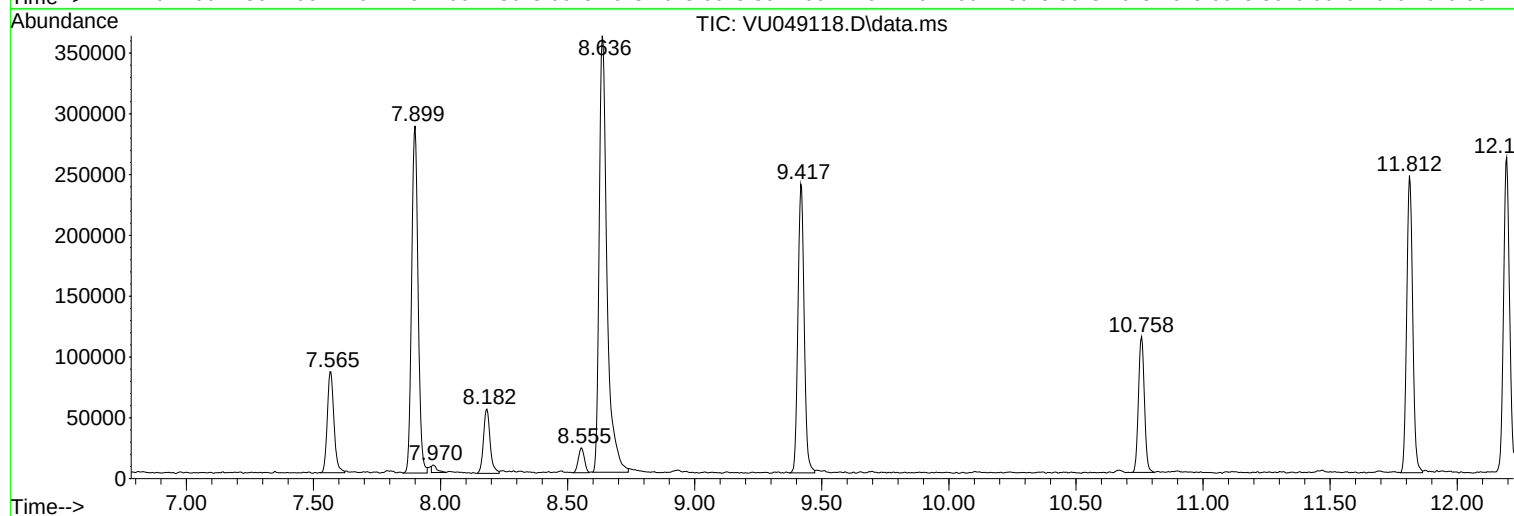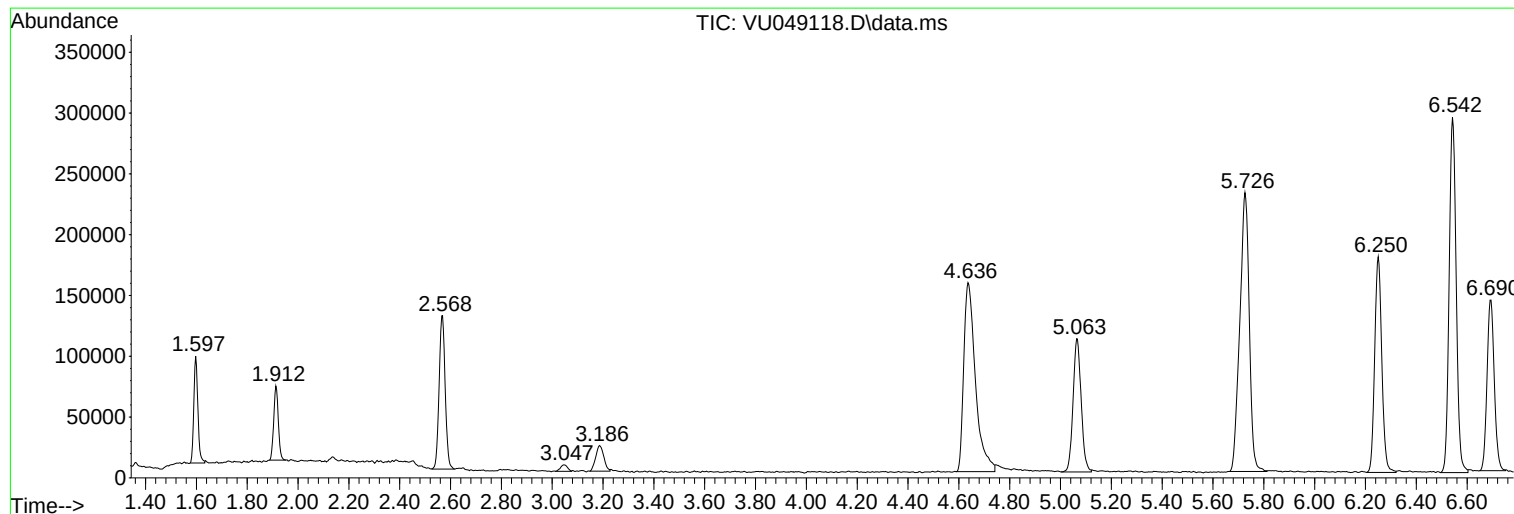

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049118.D
Acq On : 14 Jun 2022 16:57
Operator : SY/MD
Sample : N3278-11 8000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049118.D
Acq On : 14 Jun 2022 16:57
Operator : SY/MD
Sample : N3278-11 8000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc