

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049122.D
 Acq On : 14 Jun 2022 18:32
 Operator : SY/MD
 Sample : N3278-16 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BF7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049122.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.523	43	57	60	rBV10	4347	7910	1.08%	0.139%
2	1.597	73	80	90	rBV	79749	88424	12.09%	1.549%
3	1.912	171	178	190	rVB	57308	72954	9.98%	1.278%
4	2.568	370	382	399	rBV	116770	190121	26.00%	3.331%
5	3.047	523	531	539	rVB3	4948	8647	1.18%	0.152%
6	3.186	559	574	590	rBV	29692	68364	9.35%	1.198%
7	4.639	1008	1026	1058	rBV2	172419	562514	76.92%	9.856%
8	5.063	1144	1158	1181	rVB	101868	225154	30.79%	3.945%
9	5.726	1344	1364	1388	rBV2	212990	559198	76.47%	9.798%
10	6.250	1512	1527	1548	rBV	179323	343423	46.96%	6.017%
11	6.542	1603	1618	1634	rBV	256986	491257	67.18%	8.607%
12	6.693	1649	1665	1684	rBV	132891	262805	35.94%	4.605%
13	7.568	1924	1937	1958	rBV2	75236	139730	19.11%	2.448%
14	7.899	2027	2040	2057	rBV	263765	466706	63.82%	8.177%
15	8.182	2116	2128	2148	rBV	48270	89472	12.24%	1.568%
16	8.552	2233	2243	2254	rBV4	9934	16430	2.25%	0.288%
17	8.636	2254	2269	2302	rBV3	343520	731252	100.00%	12.812%
18	9.417	2494	2512	2535	rBV	232884	404337	55.29%	7.084%
19	10.758	2912	2929	2943	rBV	106063	174102	23.81%	3.050%
20	11.812	3243	3257	3278	rBV	248111	398792	54.54%	6.987%
21	12.195	3361	3376	3396	rBV	241637	405857	55.50%	7.111%




Sum of corrected areas: 5707449

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049122.D
Acq On : 14 Jun 2022 18:32
Operator : SY/MD
Sample : N3278-16 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

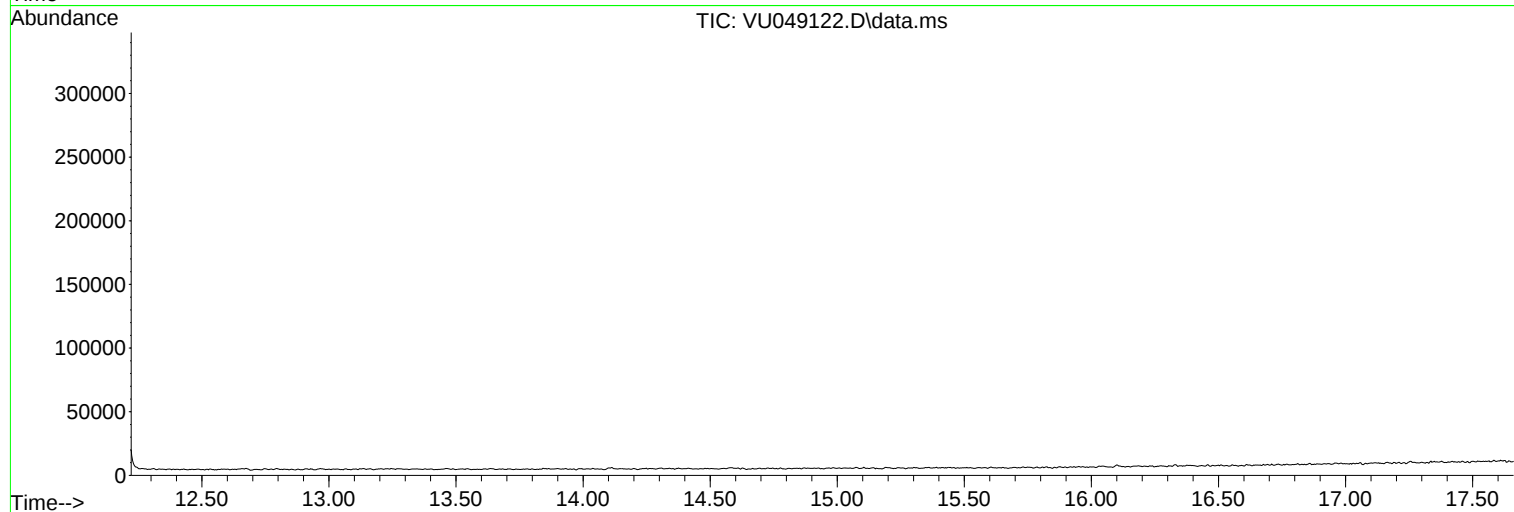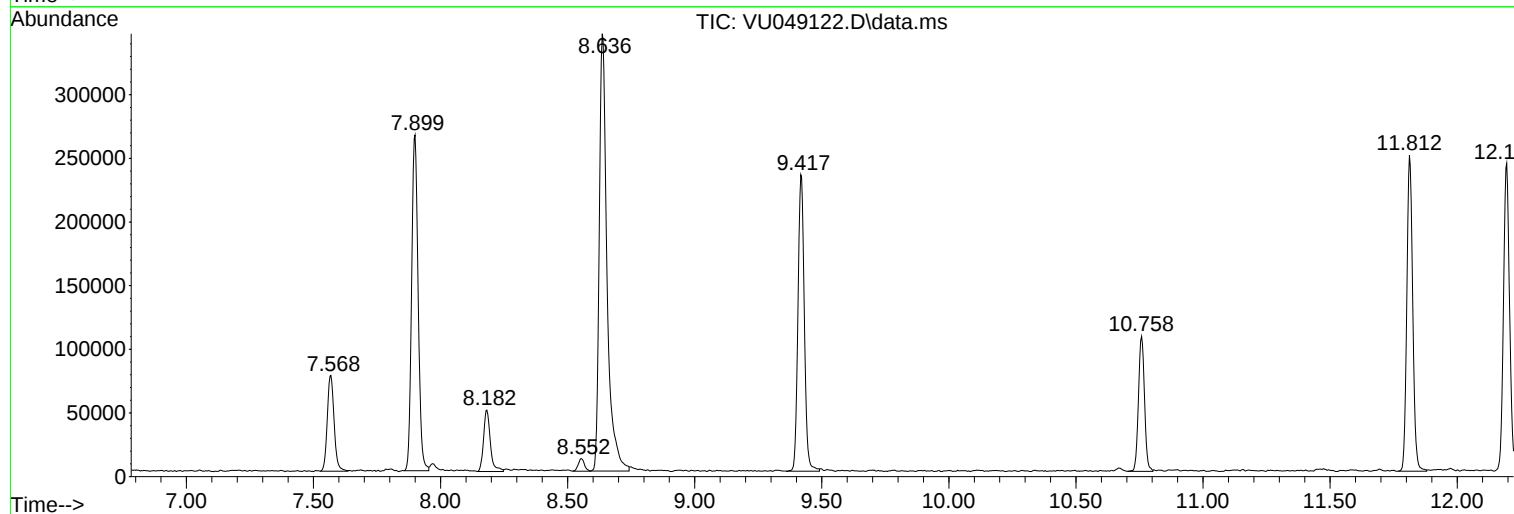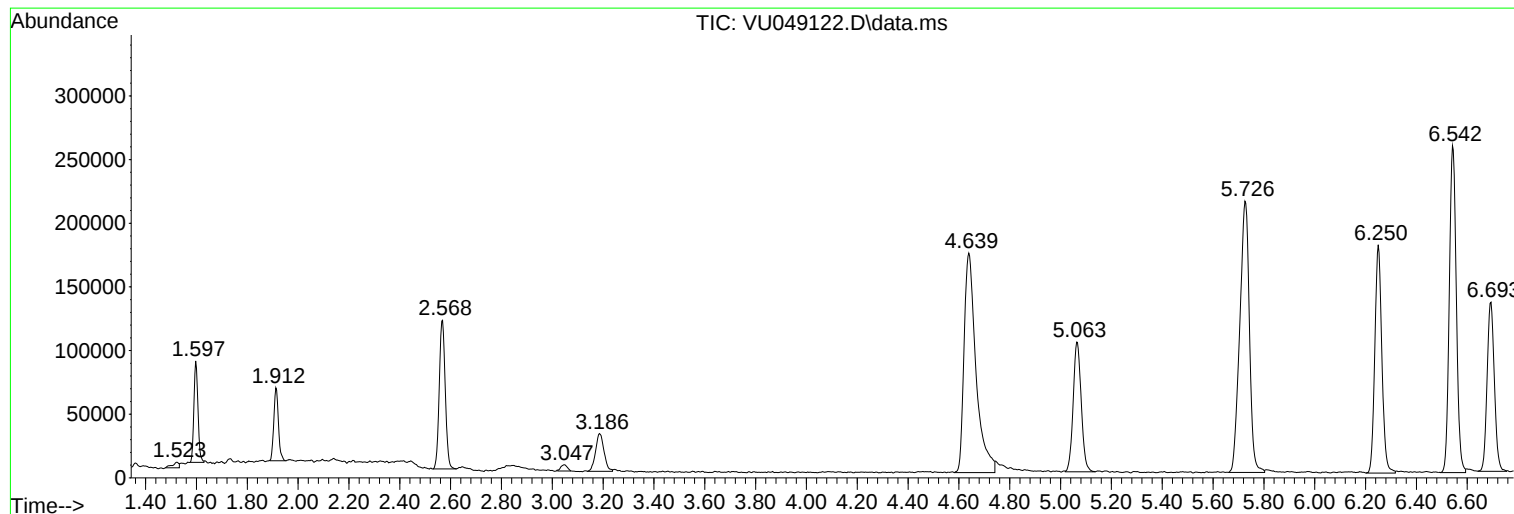

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049122.D
Acq On : 14 Jun 2022 18:32
Operator : SY/MD
Sample : N3278-16 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049122.D
Acq On : 14 Jun 2022 18:32
Operator : SY/MD
Sample : N3278-16 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc