

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049123.D
 Acq On : 14 Jun 2022 18:56
 Operator : SY/MD
 Sample : N3278-19 25X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BG0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	90	rBV	82824	95397	8.81%	1.613%
2	1.912	171	178	188	rVB	56826	70236	6.49%	1.187%
3	2.079	225	230	240	rVB	8556	11880	1.10%	0.201%
4	2.565	370	381	395	rBV	119584	193887	17.91%	3.278%
5	3.047	521	531	545	rVB4	5511	10973	1.01%	0.186%
6	3.186	561	574	588	rBV	23369	50900	4.70%	0.860%
7	4.665	1011	1034	1069	rBV3	348763	1082676	100.00%	18.303%
8	5.063	1143	1158	1176	rBV2	100707	224638	20.75%	3.798%
9	5.726	1344	1364	1383	rBV3	217373	562086	51.92%	9.502%
10	6.250	1513	1527	1546	rBV	182731	352037	32.52%	5.951%
11	6.542	1605	1618	1632	rBV	69390	134896	12.46%	2.280%
12	6.690	1647	1664	1680	rBV	135012	268308	24.78%	4.536%
13	7.568	1924	1937	1957	rBV	77642	141037	13.03%	2.384%
14	7.899	2027	2040	2056	rBV	267384	465951	43.04%	7.877%
15	8.182	2113	2128	2142	rBV	48666	86374	7.98%	1.460%
16	8.639	2257	2270	2306	rBV2	331805	739715	68.32%	12.505%
17	9.417	2499	2512	2535	rBV	248735	426181	39.36%	7.205%
18	10.758	2917	2929	2951	rVB	106571	174663	16.13%	2.953%
19	11.812	3245	3257	3279	rBV	255357	415936	38.42%	7.032%
20	12.195	3356	3376	3394	rBV	244072	407439	37.63%	6.888%




Sum of corrected areas: 5915210

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049123.D
Acq On : 14 Jun 2022 18:56
Operator : SY/MD
Sample : N3278-19 25X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

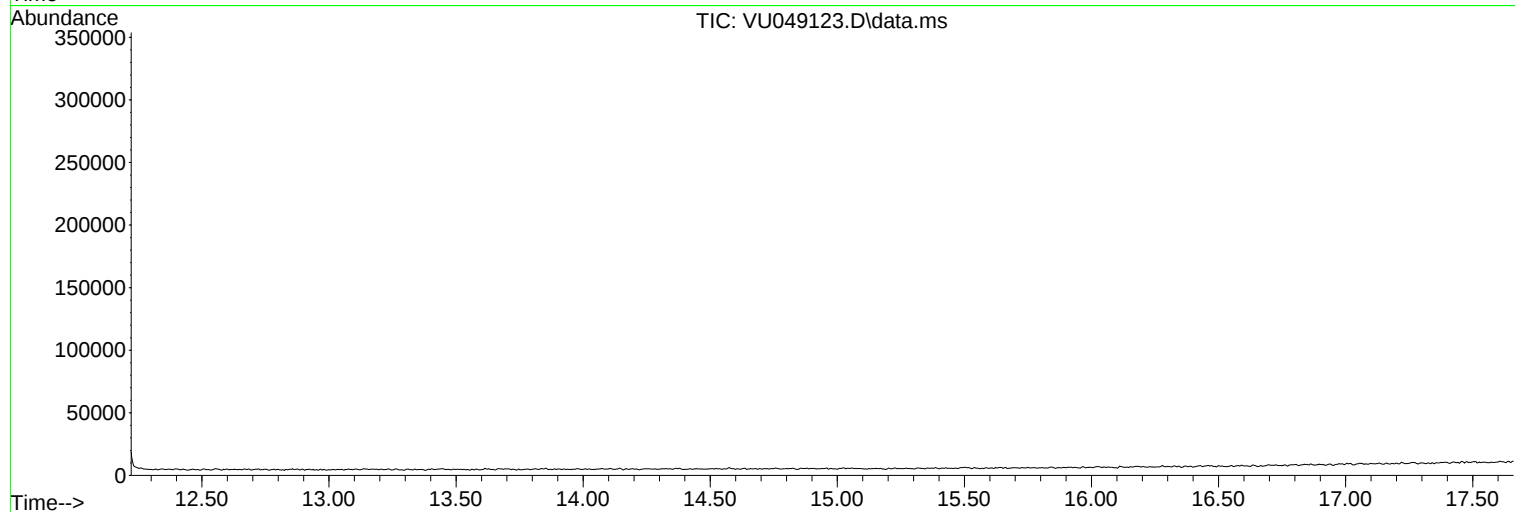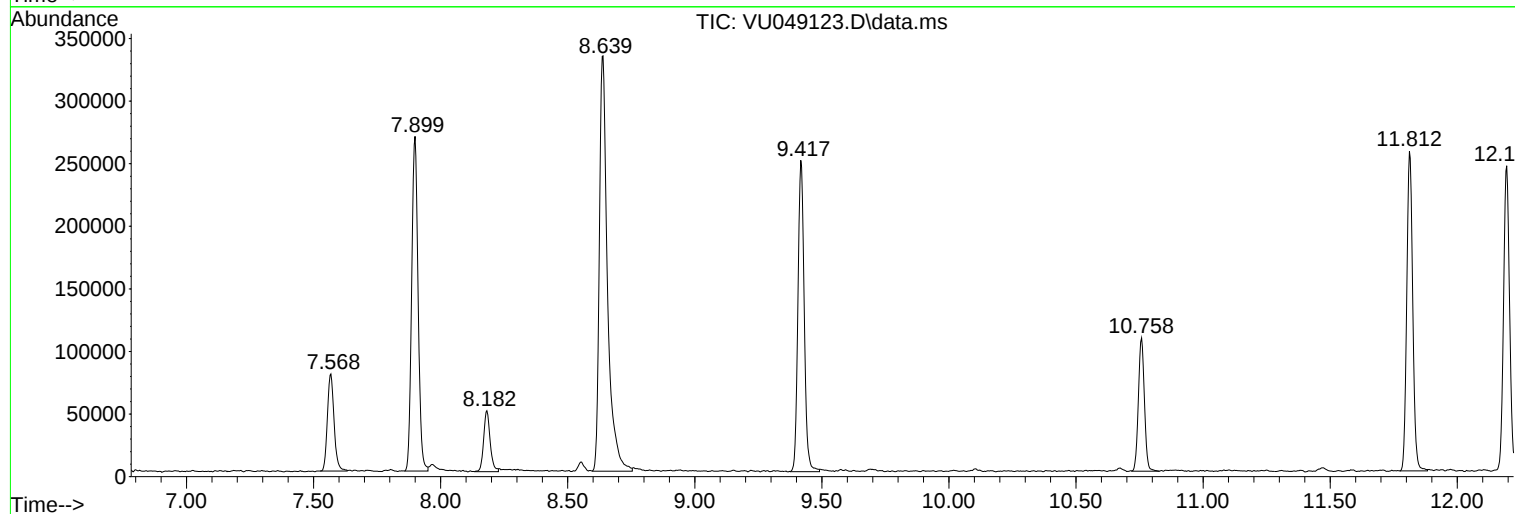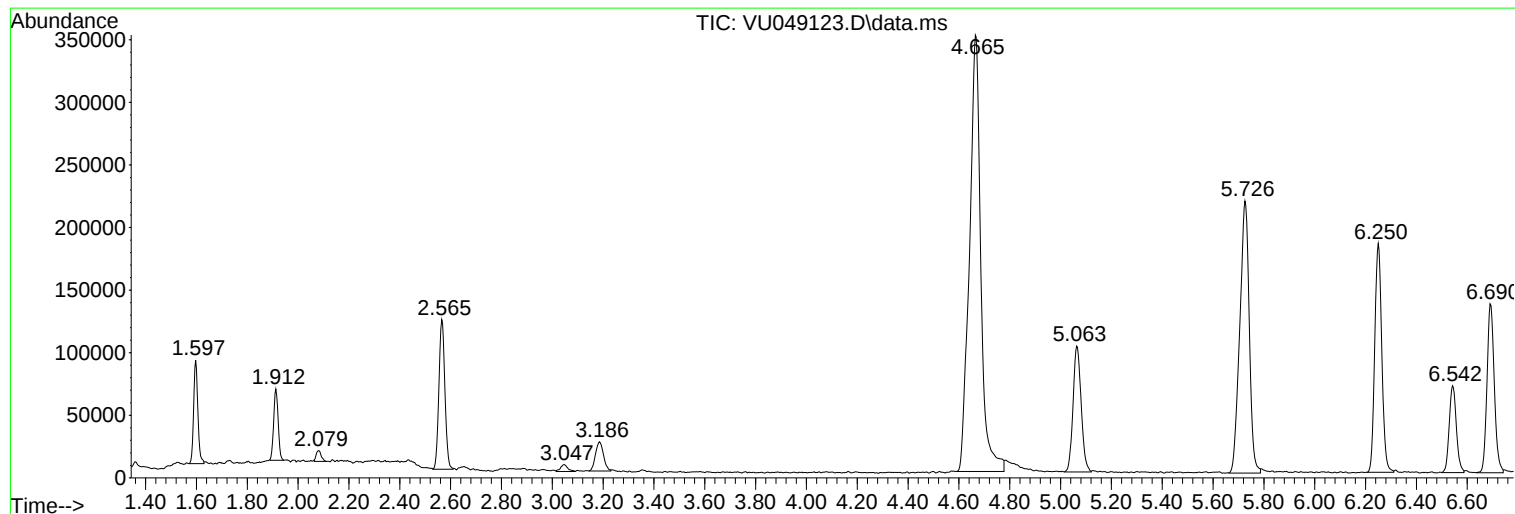

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049123.D
Acq On : 14 Jun 2022 18:56
Operator : SY/MD
Sample : N3278-19 25X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049123.D
Acq On : 14 Jun 2022 18:56
Operator : SY/MD
Sample : N3278-19 25X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc